

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112024\
 Data File : VN084966.D
 Acq On : 20 Nov 2024 14:08
 Operator : JC\MD
 Sample : PB165108TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB165108TB

Quant Time: Nov 21 00:37:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 31 18:45:38 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.218	168	174556	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	321916	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	287968	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	120018	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.576	65	126349	50.115	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 100.240%			
35) Dibromofluoromethane	8.165	113	102758	47.159	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 94.320%			
50) Toluene-d8	10.565	98	377162	46.989	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 93.980%			
62) 4-Bromofluorobenzene	12.847	95	139122	46.377	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 92.760%			
Target Compounds						Qvalue
3) Chloromethane	2.365	50	582	Below Cal	#	41
6) Chloroethane	3.124	64	148	Below Cal	#	45
11) Tert butyl alcohol	5.500	59	920	2.765	ug/l #	73
16) Acetone	4.436	43	19276	23.888	ug/l	98
18) Methyl Acetate	5.030	43	3911	Below Cal		92
20) Methylene Chloride	5.271	84	3124	1.409	ug/l #	69
25) 2-Butanone	7.494	43	2868	2.438	ug/l #	88
29) Tetrahydrofuran	7.847	42	352	0.451	ug/l #	45
31) Cyclohexane	8.218	56	4040	1.161	ug/l #	1
36) 1,1-Dichloropropene	8.218	75	15124	5.005	ug/l #	51
37) Ethyl Acetate	7.559	43	958	0.349	ug/l #	80
38) Carbon Tetrachloride	8.224	117	18351	5.433	ug/l #	16
41) Methacrylonitrile	7.853	41	344	0.233	ug/l #	24
43) Isopropyl Acetate	8.688	43	139307	27.059	ug/l #	85
45) 1,2-Dichloropropane	9.735	63	1443	0.634	ug/l #	44
48) Methyl methacrylate	9.665	41	3058	1.433	ug/l #	43
49) 1,4-Dioxane	9.741	88	60	1.587	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	7813	2.989	ug/l #	76
54) cis-1,3-Dichloropropene	10.359	75	36816	9.924	ug/l #	60
56) Ethyl methacrylate	10.982	69	1069	0.346	ug/l #	1
57) 1,3-Dichloropropane	11.200	76	4912	1.339	ug/l #	42
59) 2-Hexanone	11.200	43	56304	29.594	ug/l #	56
71) Bromoform	12.847	173	963	0.571	ug/l #	1
74) N-amyl acetate	12.482	43	730	0.204	ug/l #	42
76) 1,2,3-Trichloropropane	12.847	75	72341	30.153	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	72341	71.536	ug/l #	11
87) 1,3-Dichlorobenzene	13.729	146	948	0.215	ug/l	87
88) 1,4-Dichlorobenzene	13.729	146	948	Below Cal		88
93) 1,2,4-Trichlorobenzene	15.394	180	696	0.300	ug/l #	77
95) Naphthalene	15.641	128	2092	0.301	ug/l #	73
96) 1,2,3-Trichlorobenzene	15.841	180	571	0.253	ug/l #	71

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 21 00:37:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 31 18:45:38 2024
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.006 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion:168 Resp: 174556
Ion Ratio Lower Upper
168 100
99 58.9 54.2 81.2

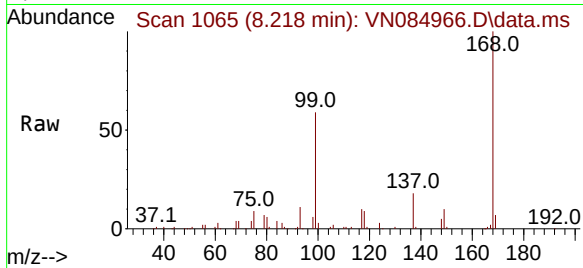

#3
Chloromethane
Concen: Below Cal
RT: 2.365 min Scan# 70
Delta R.T. 0.006 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 50 Resp: 582
Ion Ratio Lower Upper
50 100
52 0.0 26.8 40.2#




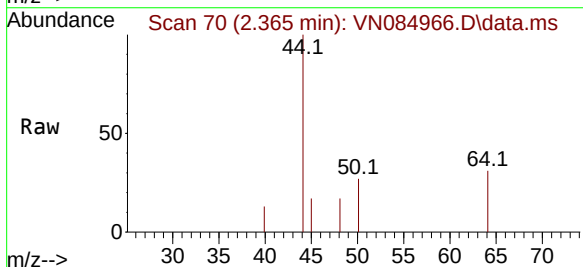




#6
Chloroethane
Concen: Below Cal
RT: 3.124 min Scan# 190
Delta R.T. 0.006 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion: 64 Resp: 148
Ion Ratio Lower Upper
64 100
66 0.0 23.5 35.3#



#11
Tert butyl alcohol
Concen: 2.765 ug/l
RT: 5.500 min Scan# 603
Delta R.T. -0.024 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 59 Resp: 920
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#


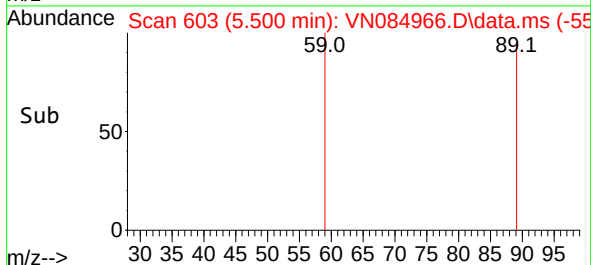

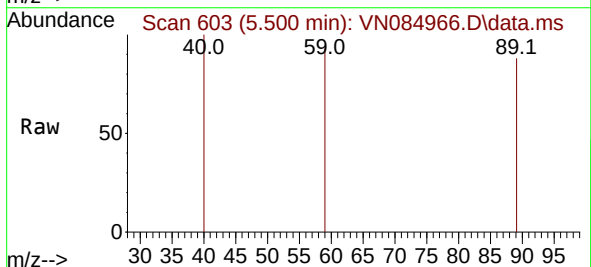




#16
Acetone
Concen: 23.888 ug/l
RT: 4.436 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion: 43 Resp: 19276
Ion Ratio Lower Upper
43 100
58 29.7 24.4 36.6



#18
Methyl Acetate
Concen: Below Cal
RT: 5.030 min Scan# 523
Delta R.T. 0.012 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 43 Resp: 3911
Ion Ratio Lower Upper
43 100
74 20.1 19.2 28.8




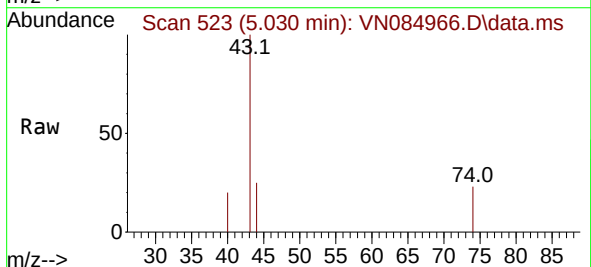




#20
Methylene Chloride
Concen: 1.409 ug/l
RT: 5.271 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion:	84	Resp:	3124
Ion	Ratio	Lower	Upper
84	100		
49	80.4	107.2	160.8#
51	57.3	31.8	47.8#
86	69.3	52.9	79.3



#25
2-Butanone
Concen: 2.438 ug/l
RT: 7.494 min Scan# 942
Delta R.T. 0.012 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion:	43	Resp:	2868
Ion	Ratio	Lower	Upper
43	100		
72	20.8	21.4	32.2#





#29

Tetrahydrofuran

Concen: 0.451 ug/l

RT: 7.847 min Scan# 1065

Delta R.T. 0.012 min

Lab File: VN084966.D

Acq: 20 Nov 2024 14:08

Instrument :

MSVOA_N

ClientSampleId :

PB165108TB





Tgt Ion: 42 Resp: 352

Ion Ratio Lower Upper

42 100

72 0.0 34.6 51.8#

71 15.1 32.2 48.4#

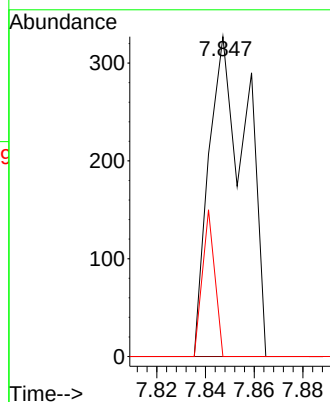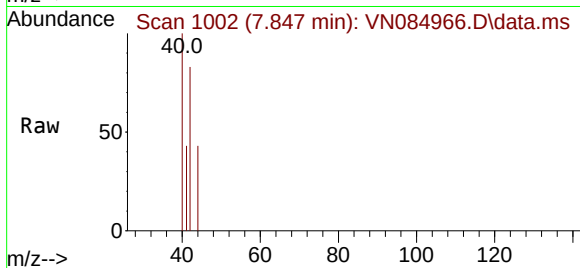

#31

Cyclohexane

Concen: 1.161 ug/l

RT: 8.218 min Scan# 1065

Delta R.T. -0.035 min

Lab File: VN084966.D

Acq: 20 Nov 2024 14:08




Tgt Ion: 56 Resp: 4040


Ion Ratio Lower Upper

56 100

69 176.5 23.8 35.6#

84 145.0 68.8 103.2#

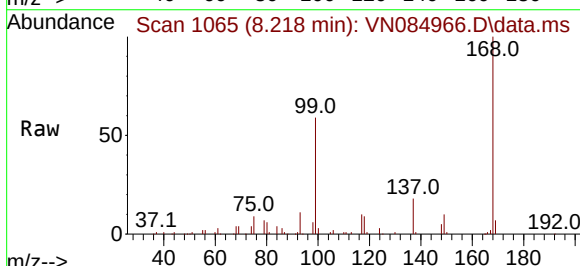

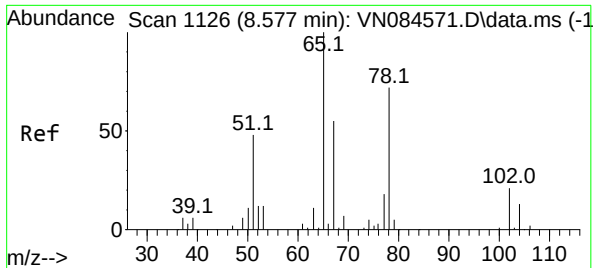

#33

1,2-Dichloroethane-d4

Concen: 50.115 ug/l

RT: 8.576 min Scan# 1126

Delta R.T. -0.001 min

Lab File: VN084966.D

Acq: 20 Nov 2024 14:08

Instrument :

MSVOA_N

ClientSampleId :





PB165108TB

Tgt Ion: 65 Resp: 126349

Ion Ratio Lower Upper

65 100

67 52.5 0.0 102.0

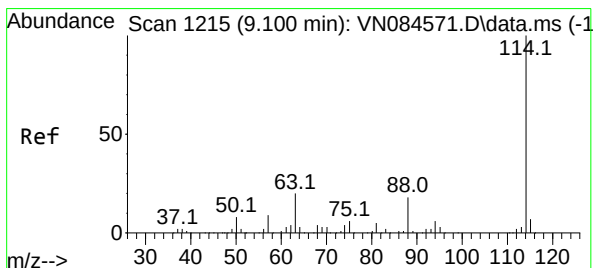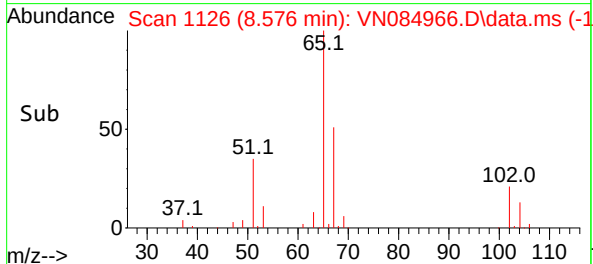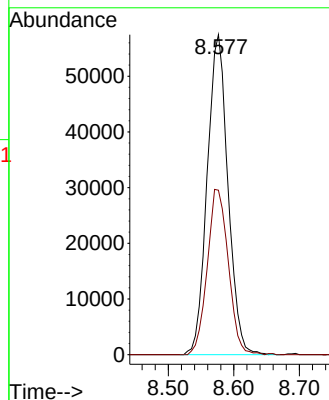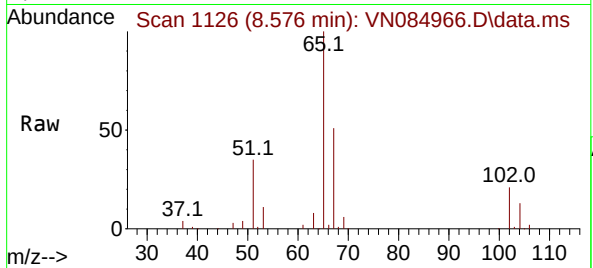

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. 0.000 min

Lab File: VN084966.D

Acq: 20 Nov 2024 14:08




Tgt Ion: 114 Resp: 321916


Ion Ratio Lower Upper

114 100

63 20.0 0.0 43.8

88 16.4 0.0 31.6

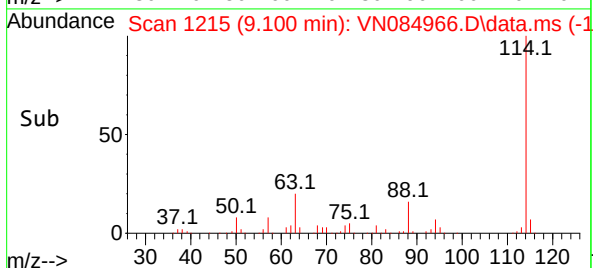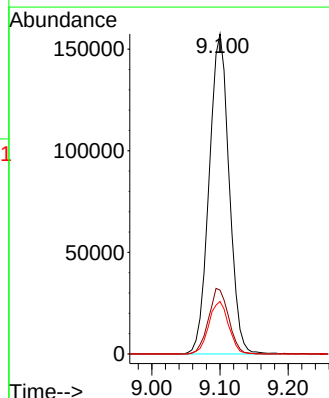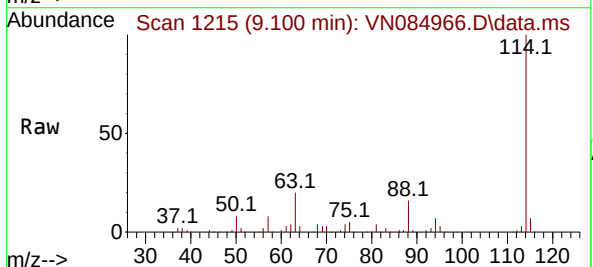

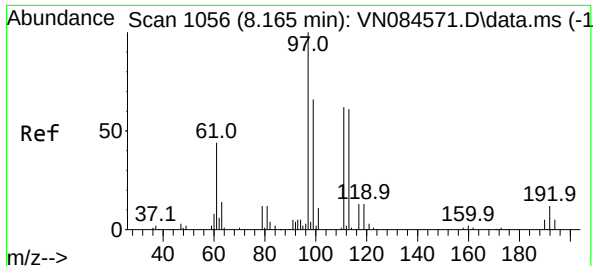

#35

Dibromofluoromethane

Concen: 47.159 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN084966.D

Acq: 20 Nov 2024 14:08

Instrument :

MSVOA_N

ClientSampleId :

PB165108TB





Tgt Ion:113 Resp: 102758

Ion Ratio Lower Upper

113 100

111 102.3 83.3 124.9

192 17.4 13.5 20.3

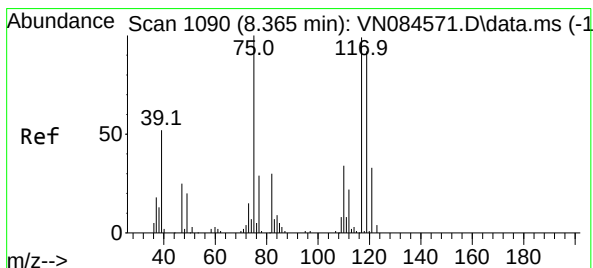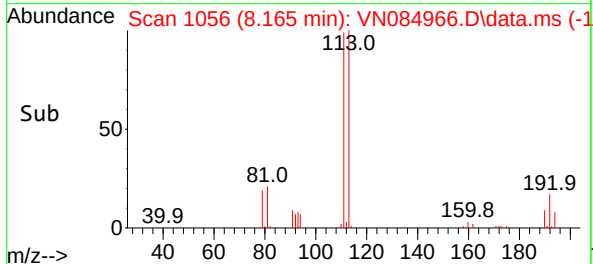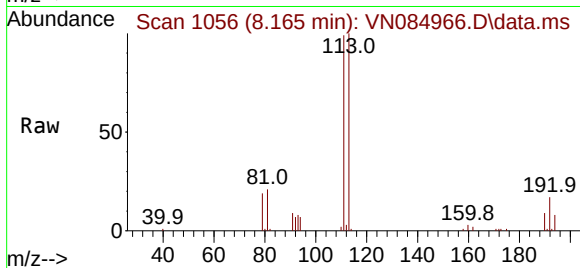

#36

1,1-Dichloropropene

Concen: 5.005 ug/l

RT: 8.218 min Scan# 1065

Delta R.T. -0.153 min

Lab File: VN084966.D

Acq: 20 Nov 2024 14:08




Tgt Ion: 75 Resp: 15124


Ion Ratio Lower Upper

75 100

110 9.1 16.9 50.7#

77 0.0 24.7 37.1#

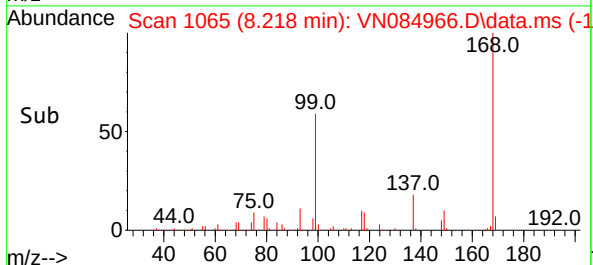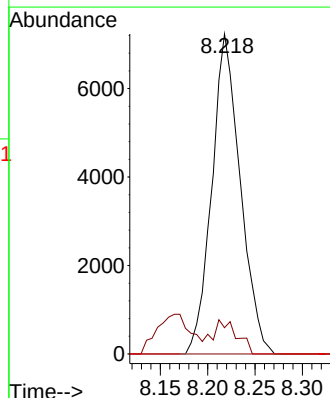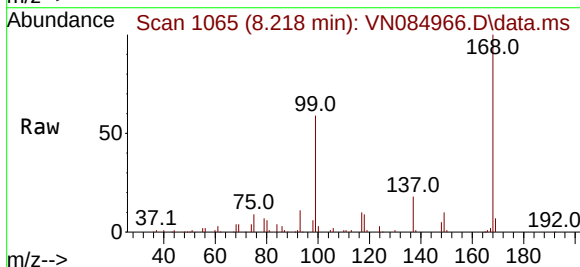



#37

Ethyl Acetate

Concen: 0.349 ug/l

RT: 7.559 min Scan# 91

Delta R.T. -0.000 min

Lab File: VN084966.D

Acq: 20 Nov 2024 14:08

Instrument :

MSVOA_N

ClientSampleId :

PB165108TB





Tgt Ion: 43 Resp: 958

Ion Ratio Lower Upper

43 100

61 18.8 10.7 16.1#

70 0.0 8.8 13.2#

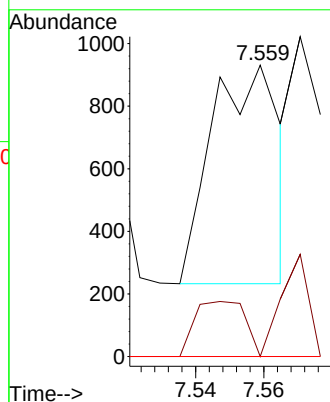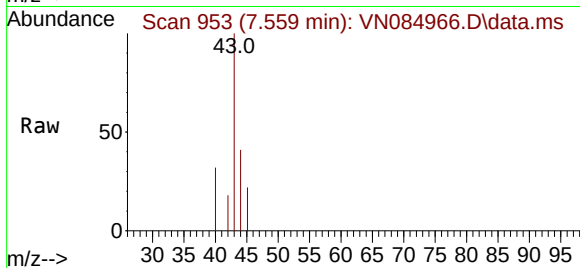

#38

Carbon Tetrachloride

Concen: 5.433 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.135 min

Lab File: VN084966.D

Acq: 20 Nov 2024 14:08




Tgt Ion: 117 Resp: 18351


Ion Ratio Lower Upper

117 100

119 6.2 78.7 118.1#

121 0.0 24.4 36.6#




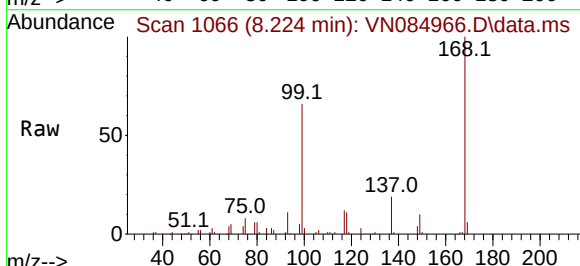




#41
Methacrylonitrile
Concen: 0.233 ug/l
RT: 7.853 min Scan# 1003
Delta R.T. 0.076 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion: 41	Resp: 344
Ion Ratio	Lower Upper
41 100	
39 0.0	43.3 64.9#
67 0.0	56.1 84.1#
52 0.0	24.5 36.7#

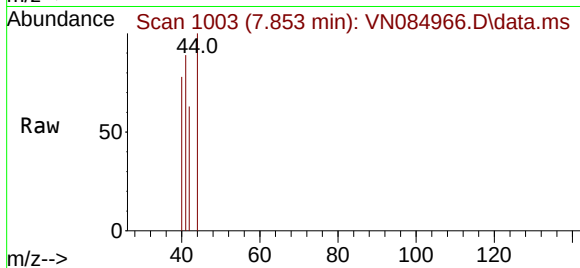

#43
Isopropyl Acetate
Concen: 27.059 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. 0.000 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 43	Resp: 139307
Ion Ratio	Lower Upper
43 100	
61 16.1	20.4 30.6#
87 10.1	10.3 15.5#




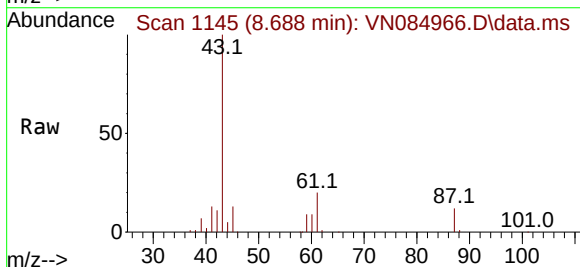


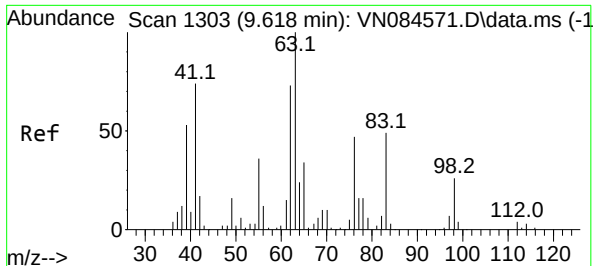

#45
1,2-Dichloropropane
Concen: 0.634 ug/l
RT: 9.735 min Scan# 11
Delta R.T. 0.117 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion: 63 Resp: 1443
Ion Ratio Lower Upper
63 100
65 0.0 24.6 37.0#

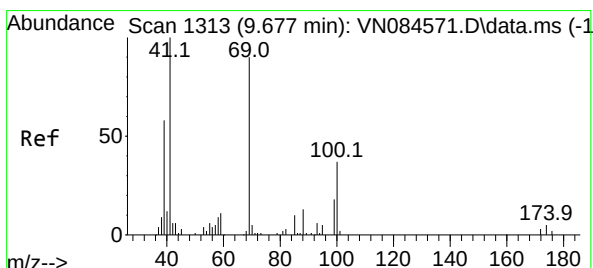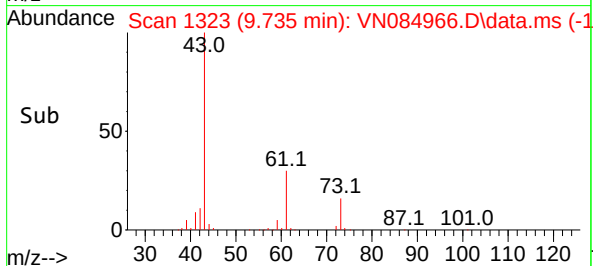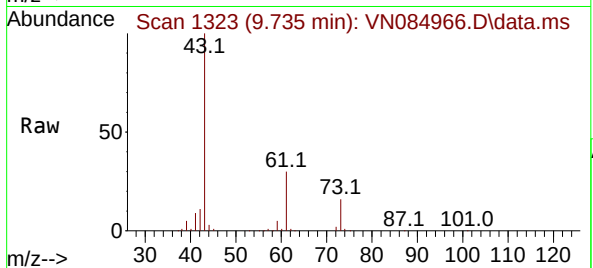

#48
Methyl methacrylate
Concen: 1.433 ug/l
RT: 9.665 min Scan# 1311
Delta R.T. -0.012 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 41 Resp: 3058
Ion Ratio Lower Upper
41 100
69 0.0 67.1 100.7#
39 60.5 45.8 68.6

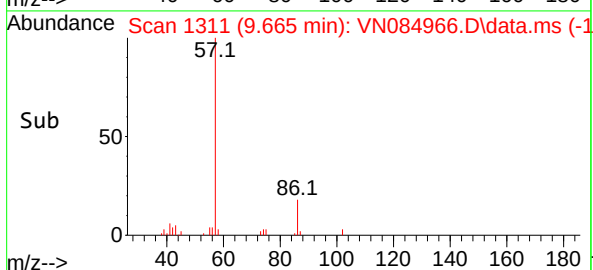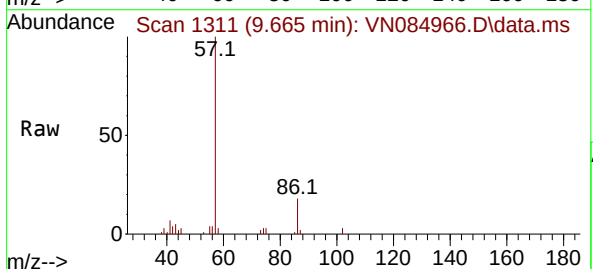

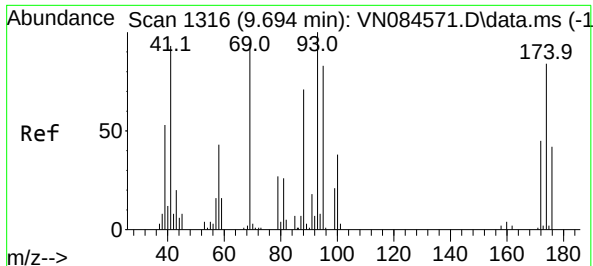

#49

1,4-Dioxane

Concen: 1.587 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.047 min

Lab File: VN084966.D

Acq: 20 Nov 2024 14:08

Instrument :

MSVOA_N

ClientSampleId :

PB165108TB





Tgt Ion: 88 Resp: 60

Ion Ratio Lower Upper

88 100

43 1575753.3 25.3 37.9#

58 6881.7 56.4 84.6#

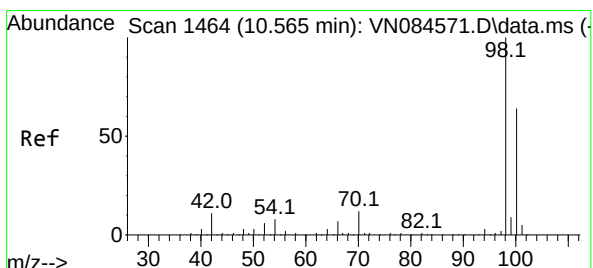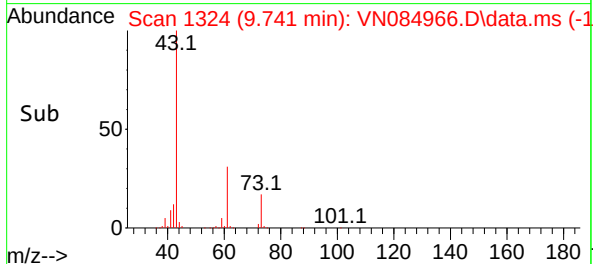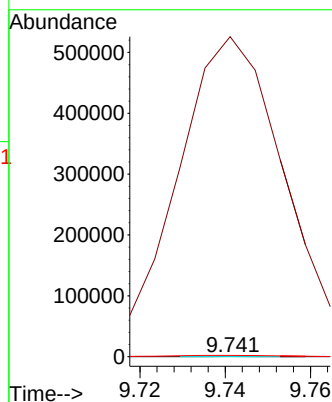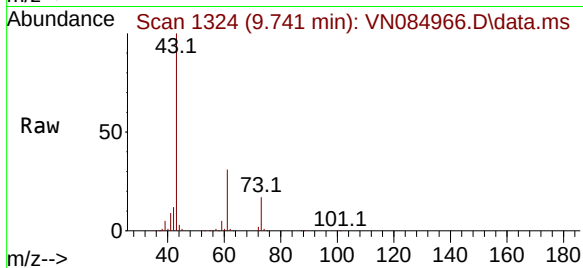

#50

Toluene-d8

Concen: 46.989 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. -0.000 min

Lab File: VN084966.D




Acq: 20 Nov 2024 14:08


Tgt Ion: 98 Resp: 377162

Ion Ratio Lower Upper

98 100

100 66.0 52.7 79.1


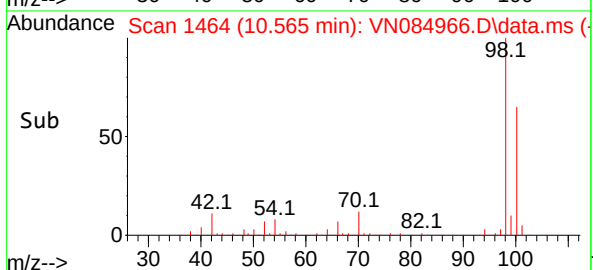

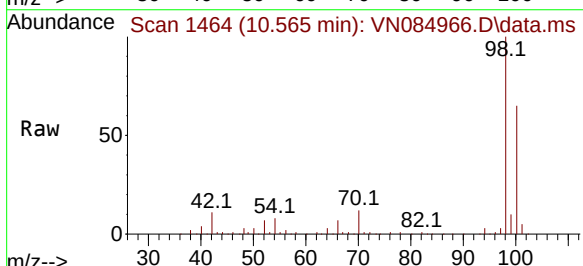




#51
4-Methyl-2-Pentanone
Concen: 2.989 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.006 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion: 43 Resp: 7813
Ion Ratio Lower Upper
43 100
58 24.5 31.6 47.4#



#54
cis-1,3-Dichloropropene
Concen: 9.924 ug/l
RT: 10.359 min Scan# 1429
Delta R.T. 0.047 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 75 Resp: 36816
Ion Ratio Lower Upper
75 100
77 0.7 24.2 36.2#
39 27.1 38.7 58.1#




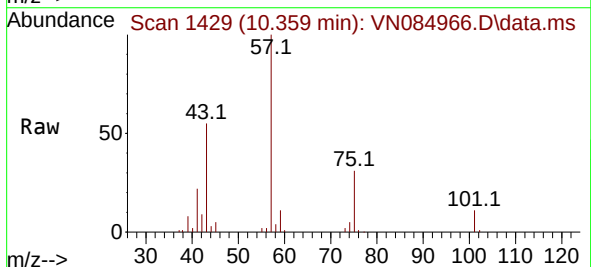


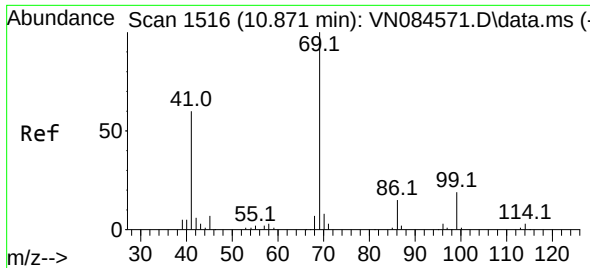

#56
Ethyl methacrylate
Concen: 0.346 ug/l
RT: 10.982 min Scan# 1535
Delta R.T. 0.112 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion: 69 Resp: 1069
Ion Ratio Lower Upper
69 100
41 4581.9 53.3 79.9#
39 1938.3 28.8 43.2#

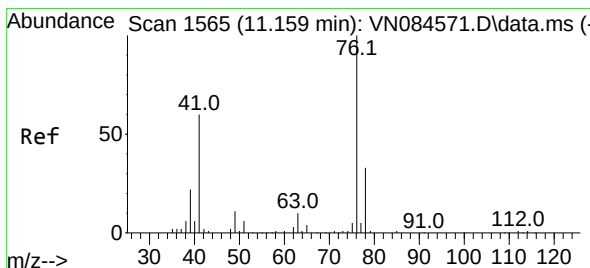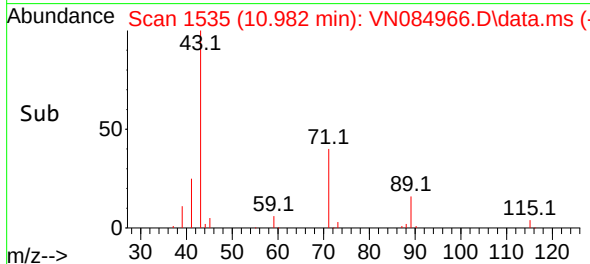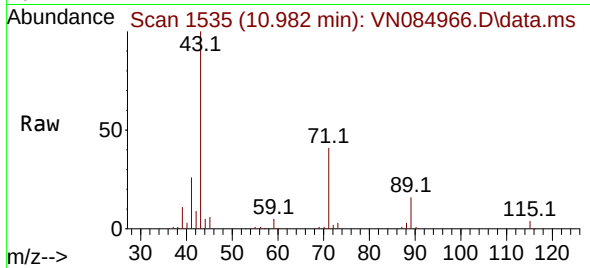

#57
1,3-Dichloropropane
Concen: 1.339 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.041 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 76 Resp: 4912
Ion Ratio Lower Upper
76 100
78 0.0 25.8 38.6#


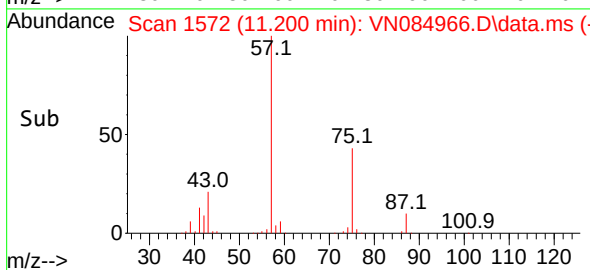

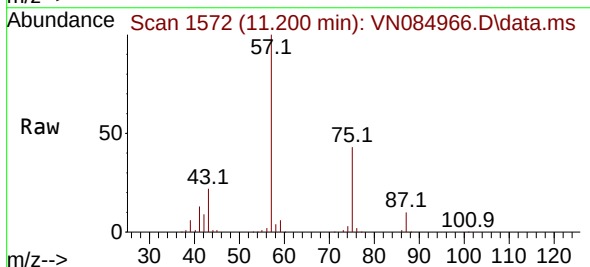




#59
2-Hexanone
Concen: 29.594 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.006 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion: 43 Resp: 56304
Ion Ratio Lower Upper
43 100
58 23.0 27.3 81.8#



#62
4-Bromofluorobenzene
Concen: 46.377 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 95 Resp: 139122
Ion Ratio Lower Upper
95 100
174 74.6 0.0 145.2
176 69.5 0.0 140.0




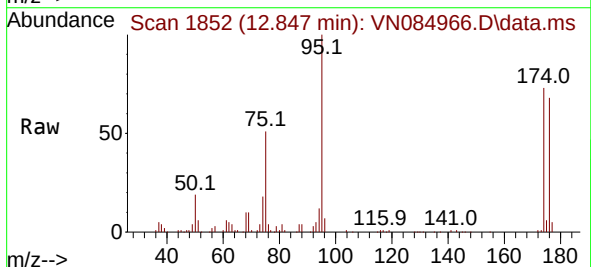




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion:117 Resp: 287968
Ion Ratio Lower Upper
117 100
82 57.1 47.2 70.8
119 32.1 25.4 38.0



#71
Bromoform
Concen: 0.571 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.270 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion:173 Resp: 963
Ion Ratio Lower Upper
173 100
175 583.1 23.5 70.6#
254 0.0 0.0 0.0




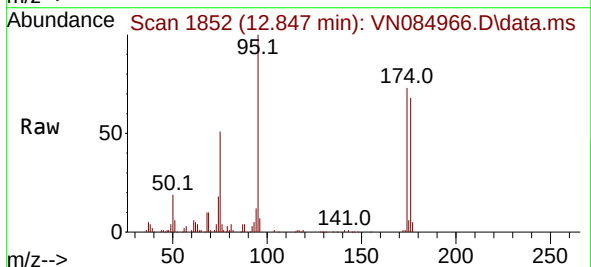


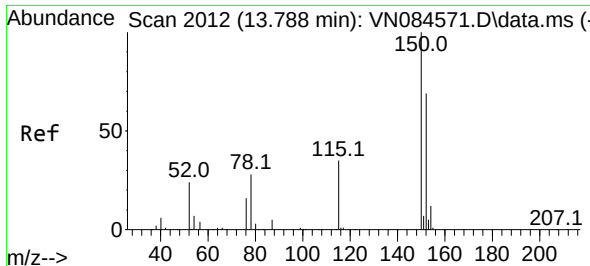

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2012
Delta R.T. 0.006 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion:152 Resp: 120018
Ion Ratio Lower Upper
152 100
115 62.4 31.3 93.9
150 158.9 0.0 349.8

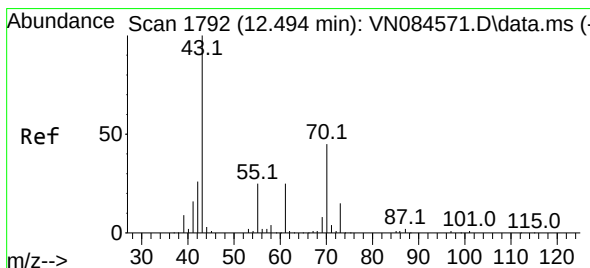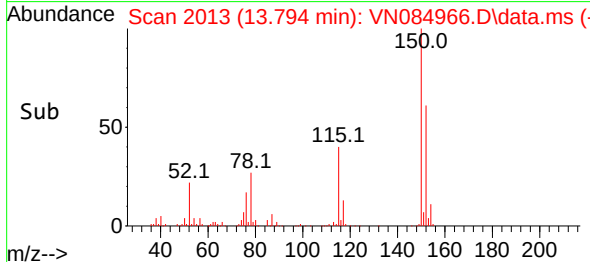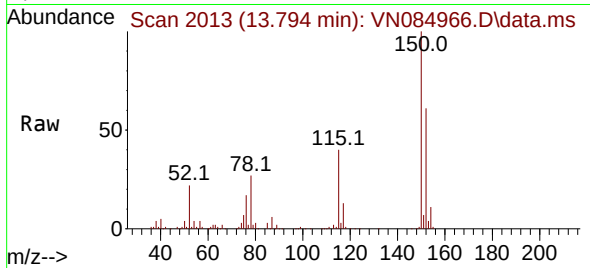

#74
N-ethyl acetate
Concen: 0.204 ug/l
RT: 12.482 min Scan# 1790
Delta R.T. -0.012 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 43 Resp: 730
Ion Ratio Lower Upper
43 100
70 0.0 34.4 51.6#
55 0.0 19.6 29.4#
61 0.0 19.6 29.4#


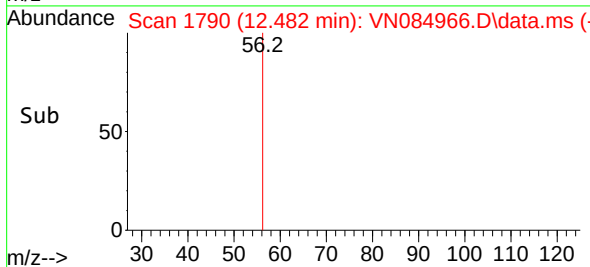

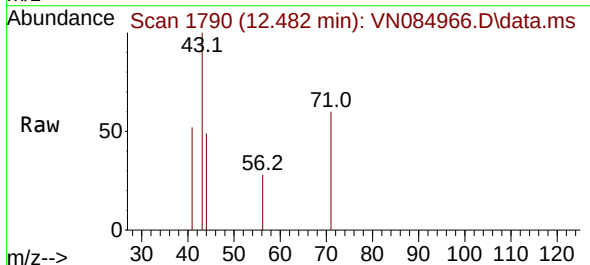




#76
1,2,3-Trichloropropane
Concen: 30.153 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08




Instrument :
MSVOA_N
ClientSampleId :
PB165108TB


Tgt Ion: 75 Resp: 72341
Ion Ratio Lower Upper
75 100
77 1.1 96.9 290.7#

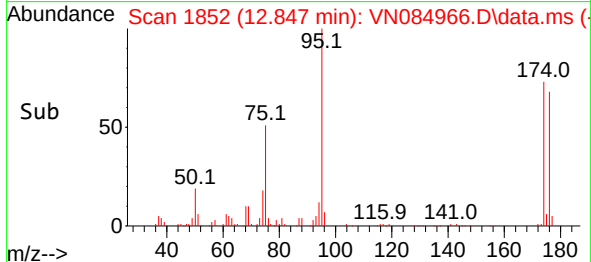

#81
trans-1,4-Dichloro-2-butene
Concen: 71.536 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN084966.D
Acq: 20 Nov 2024 14:08

Tgt Ion: 75 Resp: 72341
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 35.5 53.3#


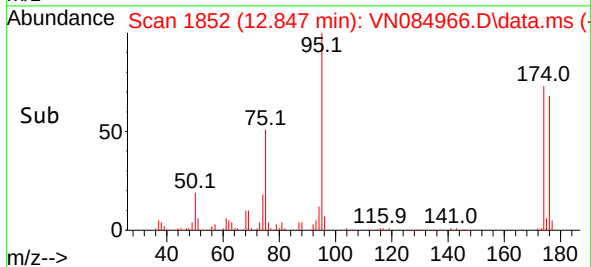

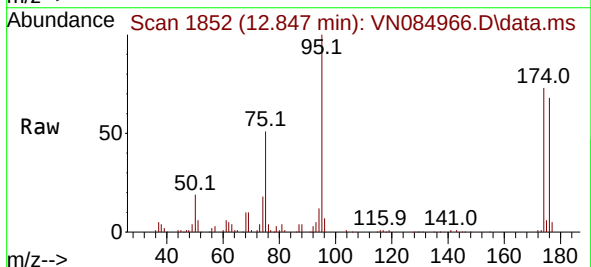




#87
 1,3-Dichlorobenzene
 Concen: 0.215 ug/l
 RT: 13.729 min Scan# 2002
 Delta R.T. 0.000 min
 Lab File: VN084966.D
 Acq: 20 Nov 2024 14:08




Instrument :
 MSVOA_N
 ClientSampleId :
 PB165108TB


Tgt Ion:	146	Resp:	948
Ion	Ratio	Lower	Upper
146	100		
111	29.3	21.8	65.3
148	69.4	31.9	95.7

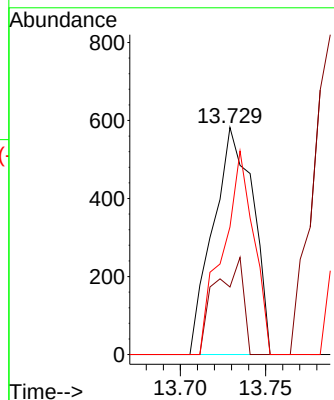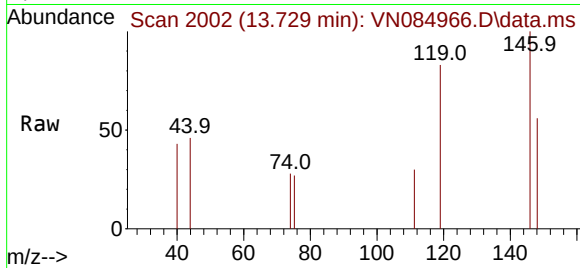

#88
 1,4-Dichlorobenzene
 Concen: Below Cal
 RT: 13.729 min Scan# 2002
 Delta R.T. -0.083 min
 Lab File: VN084966.D
 Acq: 20 Nov 2024 14:08

Tgt Ion:	146	Resp:	948
Ion	Ratio	Lower	Upper
146	100		
111	29.3	21.2	63.6
148	69.4	31.9	95.9



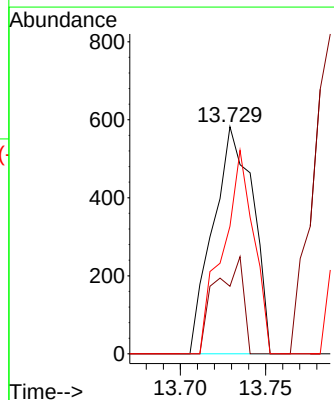
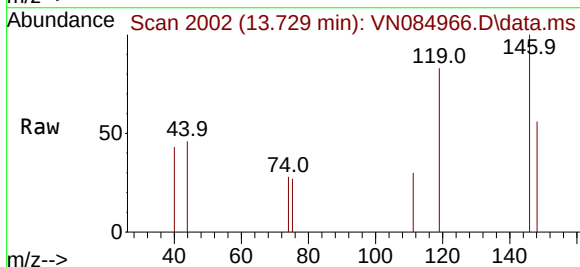


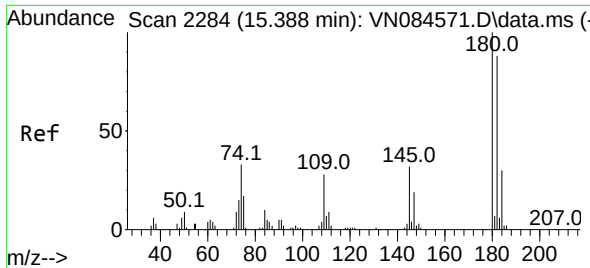

#93
 1,2,4-Trichlorobenzene
 Concen: 0.300 ug/l
 RT: 15.394 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN084966.D
 Acq: 20 Nov 2024 14:08




Instrument :
 MSVOA_N
 ClientSampleId :
 PB165108TB


Tgt Ion:180 Resp: 696
 Ion Ratio Lower Upper
 180 100
 182 111.4 47.0 141.0
 145 11.1 16.4 49.4#

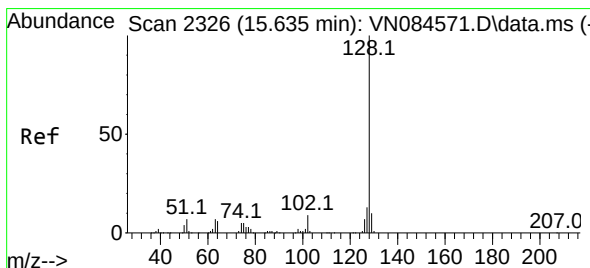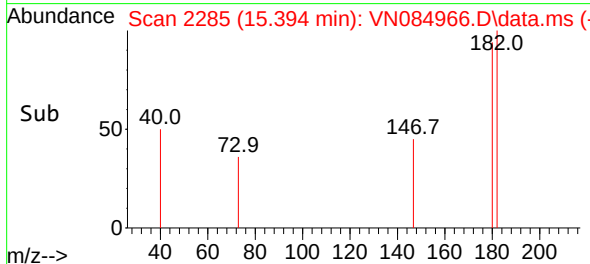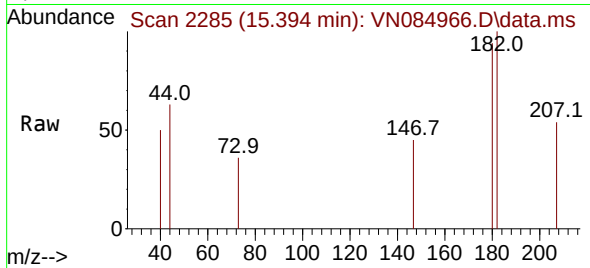

#95
 Naphthalene
 Concen: 0.301 ug/l
 RT: 15.641 min Scan# 2327
 Delta R.T. 0.006 min
 Lab File: VN084966.D
 Acq: 20 Nov 2024 14:08


Tgt Ion:128 Resp: 2092
 Ion Ratio Lower Upper
 128 100
 127 2.7 10.5 15.7#
 129 0.0 8.7 13.1#

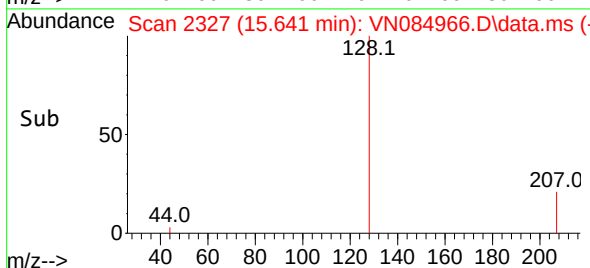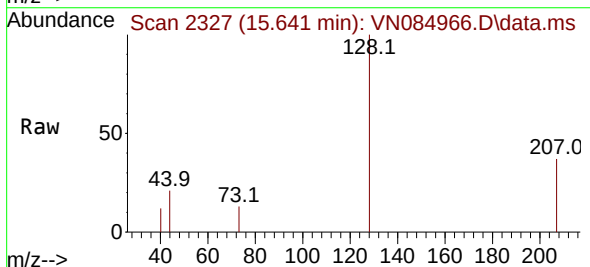



#96
 1,2,3-Trichlorobenzene
 Concen: 0.253 ug/l
 RT: 15.841 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN084966.D
 Acq: 20 Nov 2024 14:08

Instrument :
 MSVOA_N
 ClientSampleId :
 PB165108TB



Tgt Ion:180 Resp: 571
 Ion Ratio Lower Upper
 180 100
 182 79.2 48.2 144.6
 145 0.0 17.3 51.9#

