
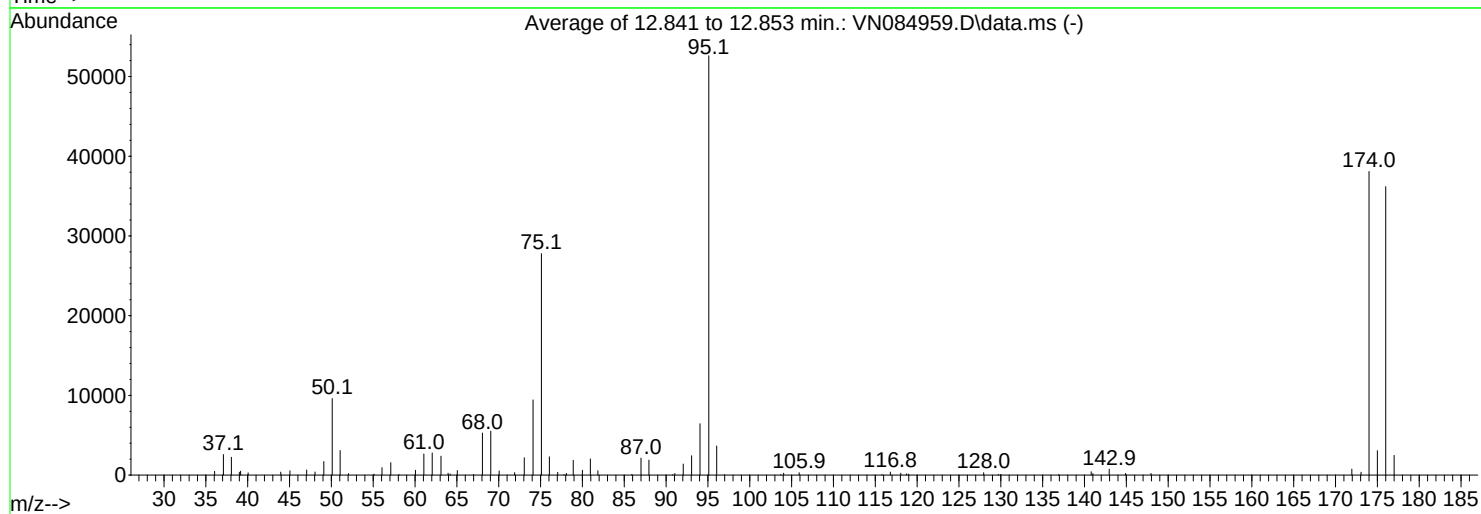


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112024\
Data File : VN084959.D
Acq On : 20 Nov 2024 09:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

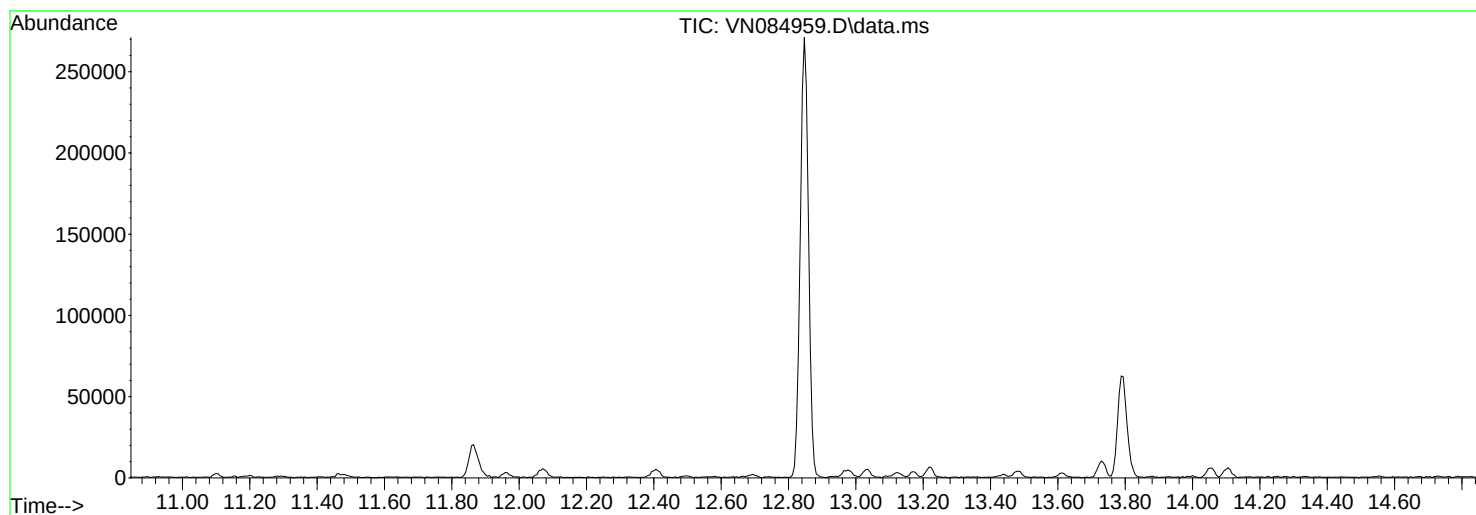

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	9603	PASS
75	95	30	60	52.8	27779	PASS
95	95	100	100	100.0	52611	PASS
96	95	5	9	6.9	3649	PASS
173	174	0.00	2	0.9	361	PASS
174	95	50	100	72.4	38096	PASS
175	174	5	9	8.0	3061	PASS
176	174	95	101	95.0	36195	PASS
177	176	5	9	6.9	2485	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	462	50.10	9603	63.95	245	76.05	2292
37.10	2574	51.05	3083	64.20	136	77.05	349
38.05	2230	52.05	179	65.05	566	77.80	61
39.00	357	55.10	123	67.00	73	78.10	204
39.15	489	56.05	935	68.05	5275	78.90	1859
40.05	285	57.10	1561	69.05	5496	80.00	607
43.95	376	58.10	57	70.05	524	80.95	2029
45.05	537	60.05	607	71.90	314	81.85	551
47.05	633	61.05	2652	73.05	2179	85.90	70
48.05	394	62.05	2768	74.10	9434	87.00	2133
49.10	1701	63.10	2374	75.10	27779	87.95	1883

Average of 12.841 to 12.853 min.: VN084959.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.80	56	115.80	58	142.95	744		
91.05	200	116.80	382	144.90	202		
92.05	1389	118.05	245	147.95	202		
93.05	2427	118.75	167	171.95	747		
94.05	6446	119.00	115	173.05	361		
95.10	52611	127.95	301	174.00	38096		
96.05	3649	129.70	75	175.00	3061		
97.00	52	130.00	76	176.00	36195		
103.70	56	136.90	54	177.00	2485		
104.05	241	140.80	424				
105.90	304	141.00	188				

Instrument :

MSVOA_N

ClientSampleId :

BFB