

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN112118\
 Data File : VN052442.D
 Acq On : 21 Nov 2018 16:57
 Operator : MD\SY
 Sample : J6024-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 18 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 21 23:59:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 15 03:02:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	299749	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	511162	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	437711	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	154709	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	233318	55.11	ug/l	0.00
Spiked Amount			Recovery	=	110.22%	
35) Dibromofluoromethane	7.59	113	168603	51.14	ug/l	0.00
Spiked Amount			Recovery	=	102.28%	
50) Toluene-d8	10.09	98	648587	50.01	ug/l	0.00
Spiked Amount			Recovery	=	100.02%	
62) 4-Bromofluorobenzene	12.40	95	197449	46.28	ug/l	0.00
Spiked Amount			Recovery	=	92.56%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acrolein	3.87	56	64	21.944	ug/l #	14
16) Acetone	3.82	43	6864	5.889	ug/l	99
18) Methyl Acetate	4.33	43	2003	1.040	ug/l #	68
20) Methylene Chloride	4.56	84	117075	32.773	ug/l	96
25) 2-Butanone	6.84	43	988	0.602	ug/l #	52
29) Tetrahydrofuran	7.21	42	341	0.316	ug/l #	65
30) Chloroform	7.37	83	2673	0.405	ug/l	100
31) Cyclohexane	7.67	56	9463	0.419	ug/l #	17
36) 1,1-Dichloropropene	7.66	75	28483	5.559	ug/l #	51
38) Carbon Tetrachloride	7.67	117	32082	6.816	ug/l #	16
41) Methacrylonitrile	7.18	41	29	3.708	ug/l #	100
43) Isopropyl Acetate	8.17	43	19922	2.777	ug/l #	94
45) 1,2-Dichloropropane	9.27	63	920	0.221	ug/l #	44
48) Methyl methacrylate	9.18	41	4801	1.319	ug/l #	16
51) 4-Methyl-2-Pentanone	10.02	43	5295	1.466	ug/l #	41
52) Toluene	10.16	92	2367	0.270	ug/l	98
54) cis-1,3-Dichloropropene	9.90	75	27719	4.886	ug/l #	79
57) 1,3-Dichloropropane	10.77	76	5787	1.029	ug/l #	43
59) 2-Hexanone	10.76	43	101556	40.880	ug/l #	53
68) m/p-Xylenes	11.62	106	1249	0.213	ug/l	94
74) N-amyl acetate	11.88	43	9080	2.050	ug/l #	59
76) 1,2,3-Trichloropropane	12.40	75	114573	43.645	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.73	105	4456	0.450	ug/l	96
81) trans-1,4-Dichloro-2-buten	12.40	75	114573	141.557	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.04	105	4818	0.485	ug/l	96
95) Naphthalene	15.14	128	2643	3.062	ug/l #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN112118\
Data File : VN052442.D
Acq On : 21 Nov 2018 16:57
Operator : MD\SY
Sample : J6024-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 18 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 21 23:59:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 15 03:02:37 2018
Response via : Initial Calibration

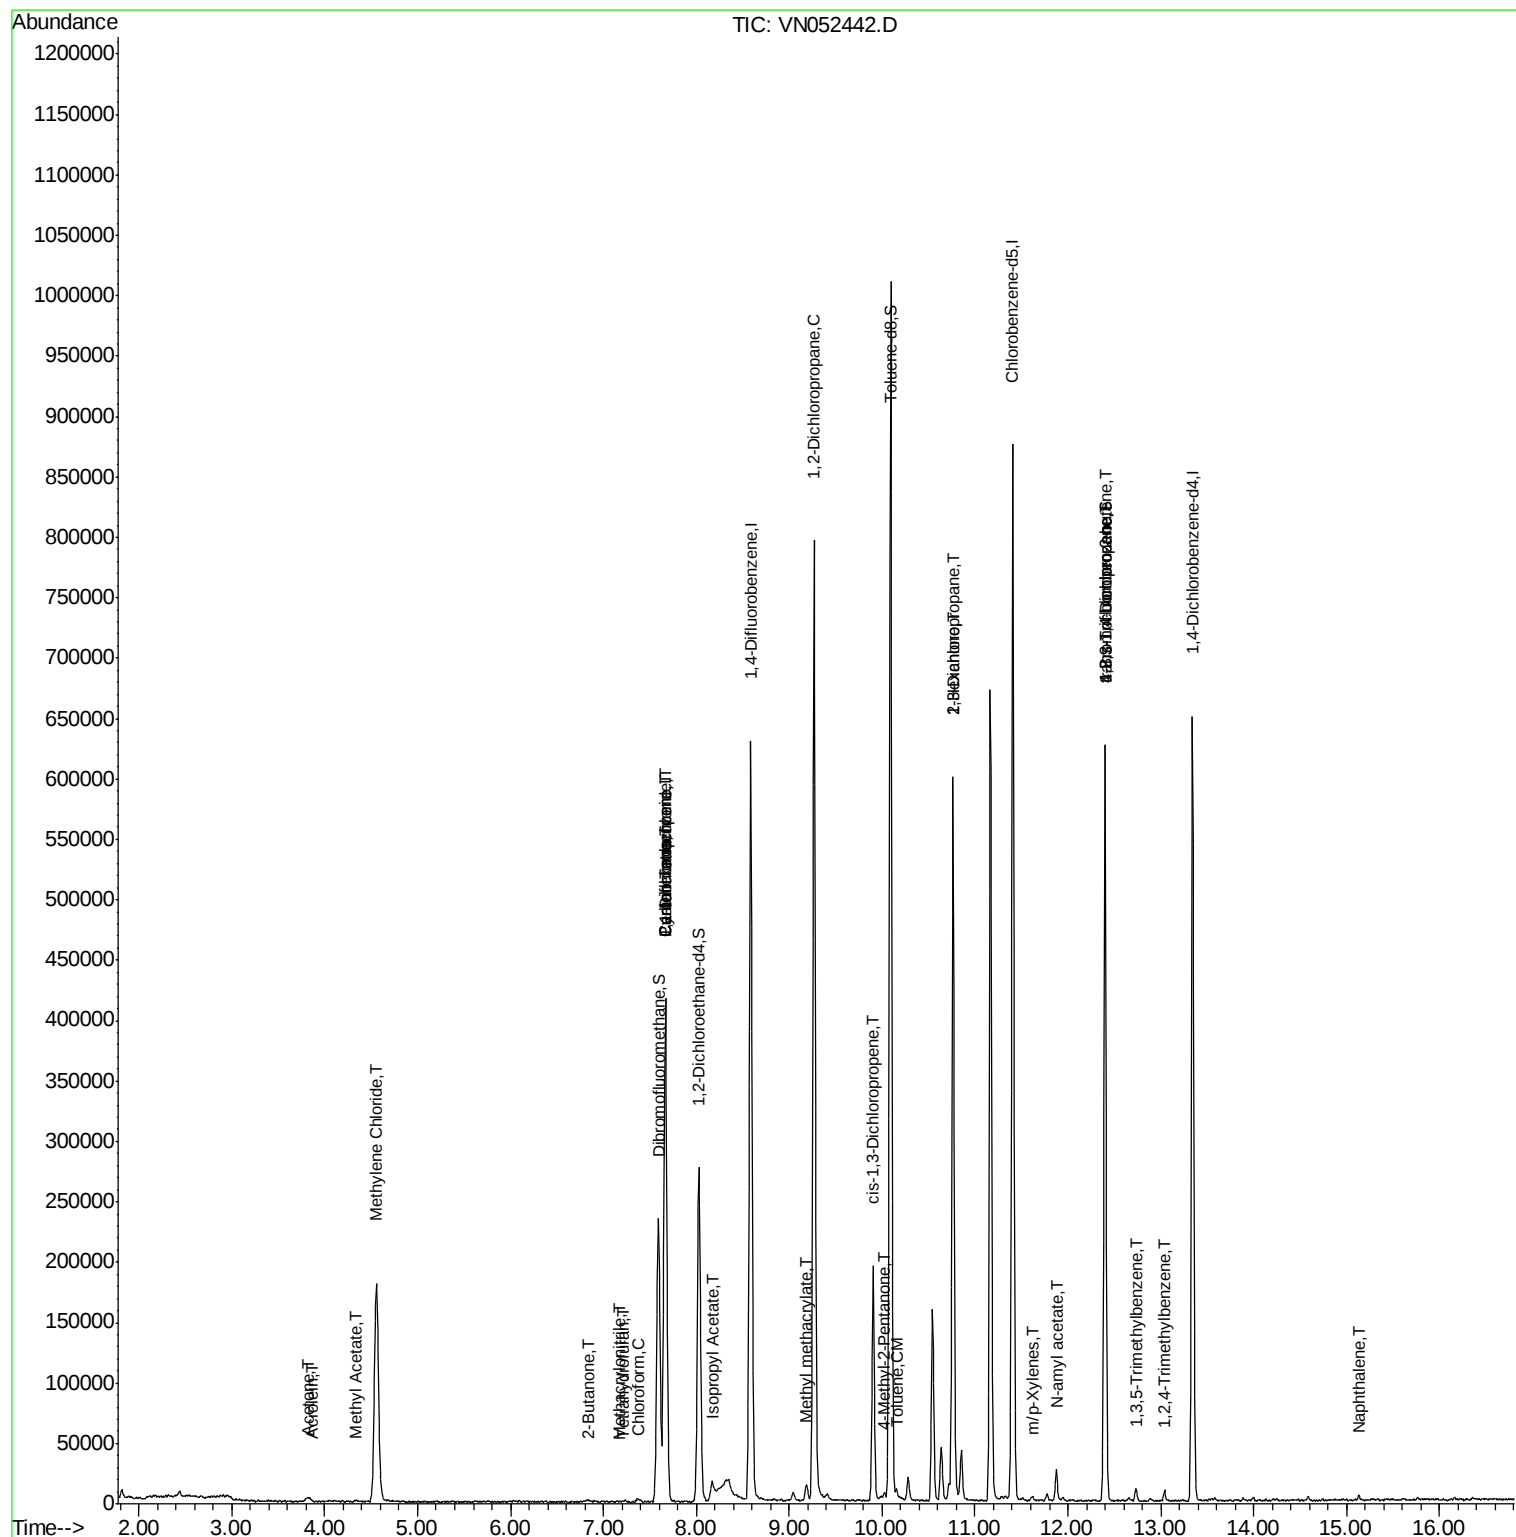



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57


Instrument :
MSVOA_N
ClientSampled :

Tot Ion:168 Resp: 299749




Ion Ratio Lower Upper

168 100

99 63.6 47.9 71.9

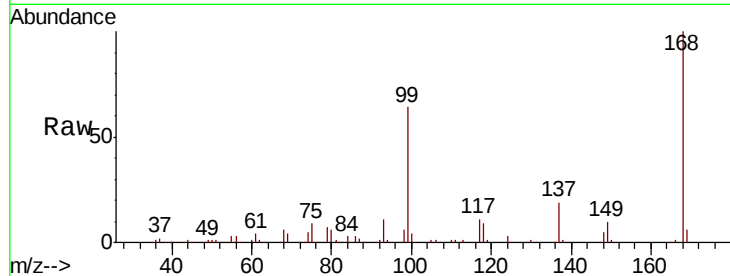

Abundance Ion 167.90 (167.60 to 168.60): V
Ion 98.90 (98.60 to 99.60): VN

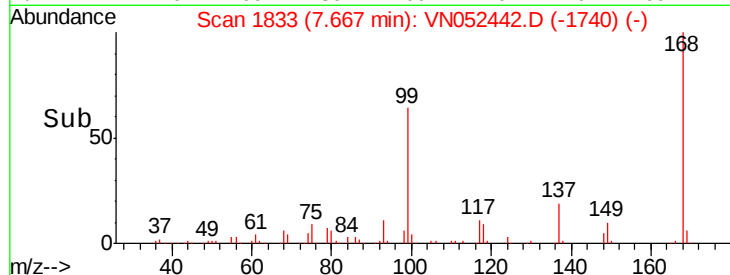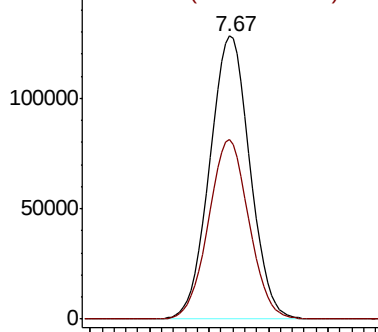

#13

Acrolein

Concen: 21.944 ug/l

RT: 3.87 min Scan# 651

Delta R.T. 0.26 min

Lab File: VN052442.D


Acq: 21 Nov 2018 16:57

Tgt Ion: 56 Resp: 64



Ion Ratio Lower Upper

56 100

55 0.0 57.6 86.4#



Abundance Ion 56.00 (55.70 to 56.70): VN
Ion 55.00 (54.70 to 55.70): VN

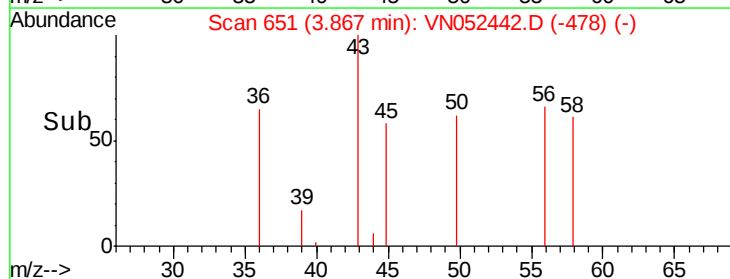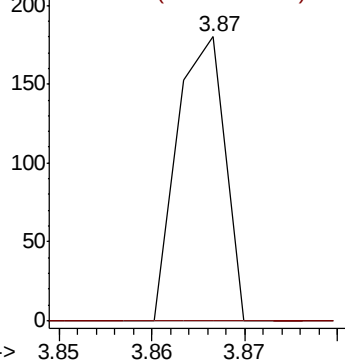



#16

Acetone

Concen: 5.889 ug/l

RT: 3.82 min Scan# 636

Delta R.T. 0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion: 43 Resp: 6864




Ion Ratio Lower Upper

43 100

58 30.9 24.2 36.4



Abundance Ion 43.00 (42.70 to 43.70): VN052307.D (-599) (-)

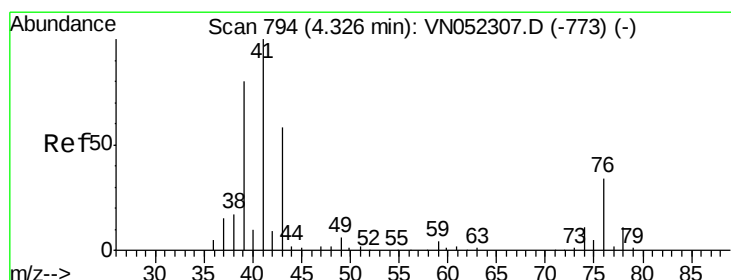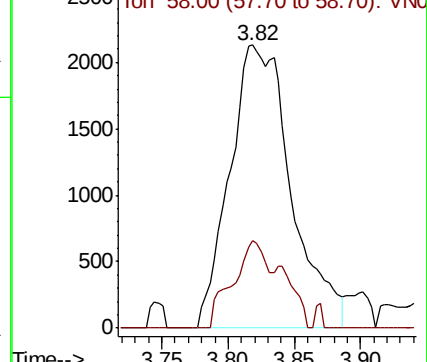

#18

Methyl Acetate

Concen: 1.040 ug/l

RT: 4.33 min Scan# 795

Delta R.T. 0.00 min

Lab File: VN052442.D


Acq: 21 Nov 2018 16:57

Tgt Ion: 43 Resp: 2003



Ion Ratio Lower Upper


43 100

74 5.2 15.9 23.9#

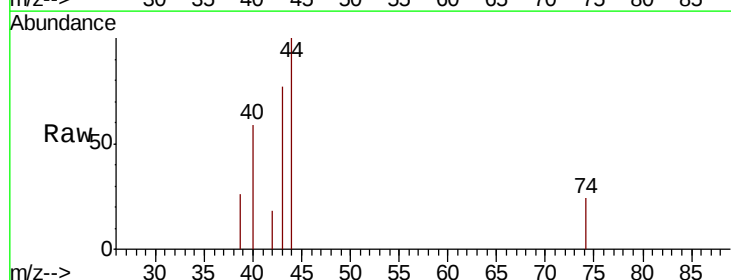

Abundance Ion 43.00 (42.70 to 43.70): VN052307.D (-773) (-)



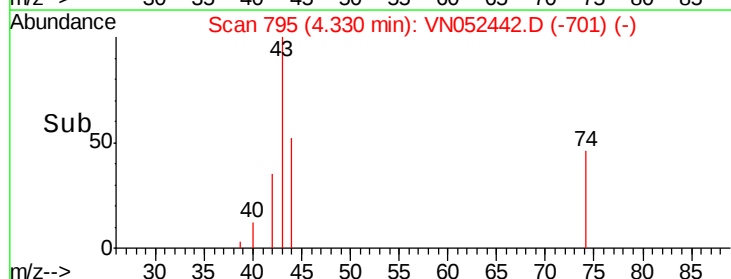
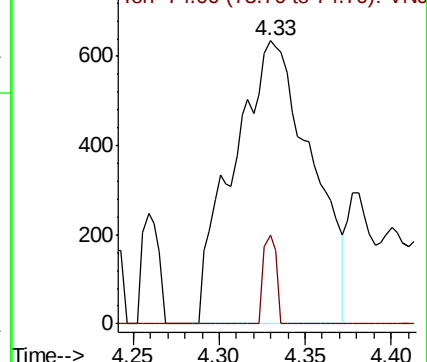




#20
Methvlene Chloride
Concen: 32.773 ug/l
RT: 4.56 min Scan# 866
Delta R.T. 0.00 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57




Instrument :
MSVOA_N
ClientSampled :


Tot Ion: 84 Resp: 117075
Ion Ratio Lower Upper
84 100
49 153.5 118.2 177.2
51 46.7 36.1 54.1
86 63.1 51.6 77.4

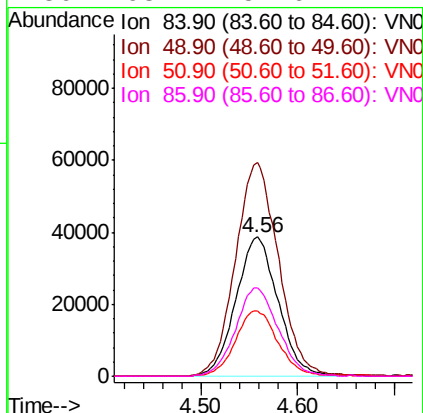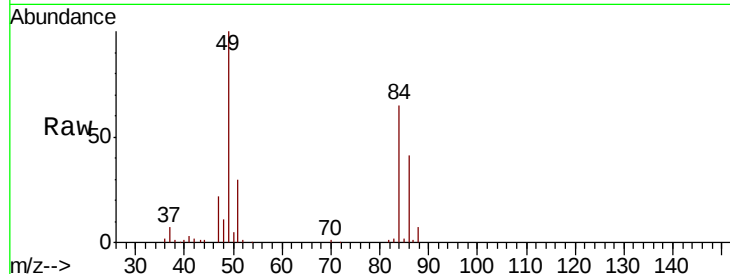

#25
2-Butanone
Concen: 0.602 ug/l
RT: 6.84 min Scan# 1577
Delta R.T. 0.01 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57

Tgt Ion: 43 Resp: 988
Ion Ratio Lower Upper
43 100
72 0.0 18.6 27.8#

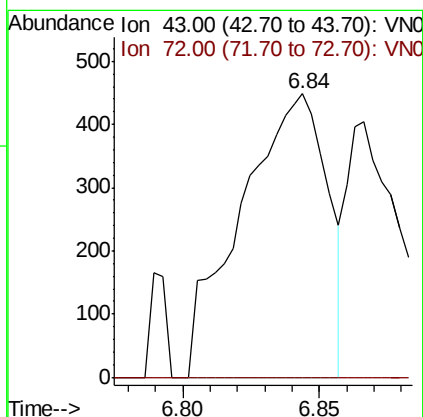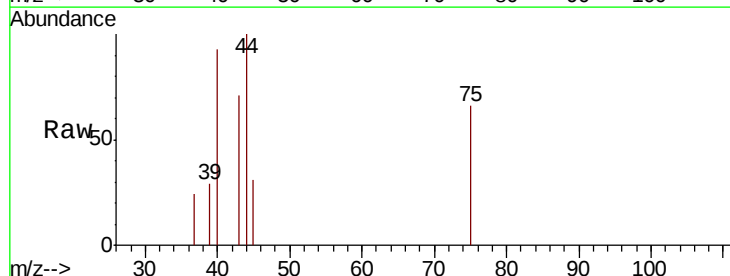



#29

Tetrahydrofuran

Concen: 0.316 ug/l

RT: 7.21 min Scan# 1690

Delta R.T. -0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57

Instrument :

MSVOA_N

ClientSampled :





Tot Ion: 42 Resp: 341

Ion Ratio Lower Upper

42 100

72 9.4 28.6 42.8#

71 19.1 26.7 40.1#

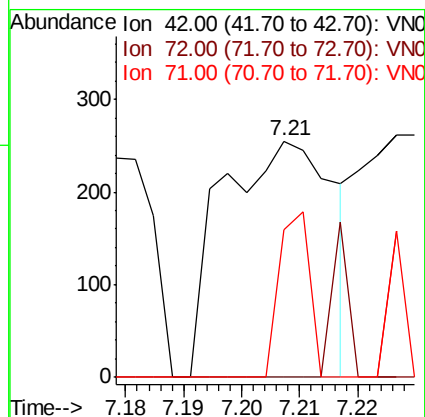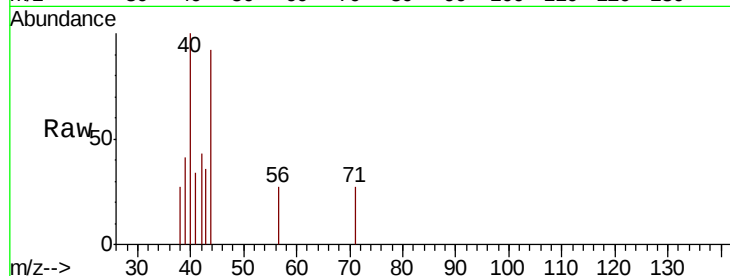

#30

Chloroform

Concen: 0.405 ug/l

RT: 7.37 min Scan# 1742

Delta R.T. 0.00 min

Lab File: VN052442.D




Acq: 21 Nov 2018 16:57


Tgt Ion: 83 Resp: 2673

Ion Ratio Lower Upper

83 100

85 61.5 49.4 74.2

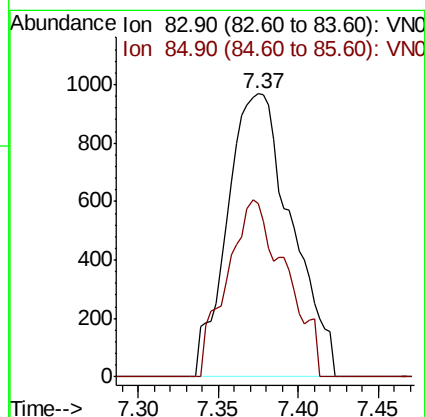


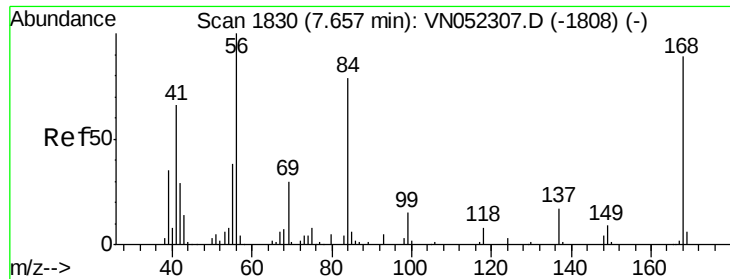




#31
Cyclohexane
Concen: 0.419 ug/l
RT: 7.67 min Scan# 1833
Delta R.T. 0.01 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57

Instrument :
MSVOA_N
ClientSampleId :

Tot Ion: 56 Resp: 9463
Ion Ratio Lower Upper
56 100
69 142.4 23.8 35.8#
84 109.9 63.0 94.6#

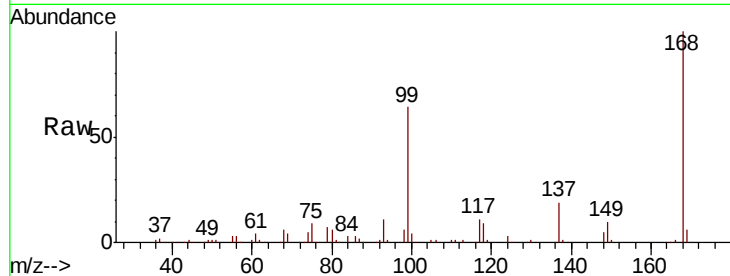


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0


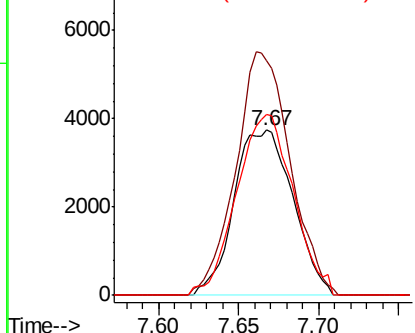



#33
1,2-Dichloroethane-d4
Concen: Below ug/l
RT: 8.03 min Scan# 1945
Delta R.T. 0.00 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57

Tgt Ion: 65 Resp: 233318
Ion Ratio Lower Upper
65 100
67 50.5 0.0 105.2



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

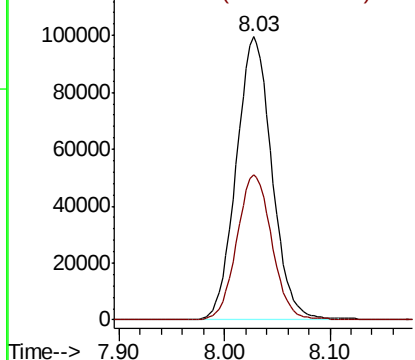

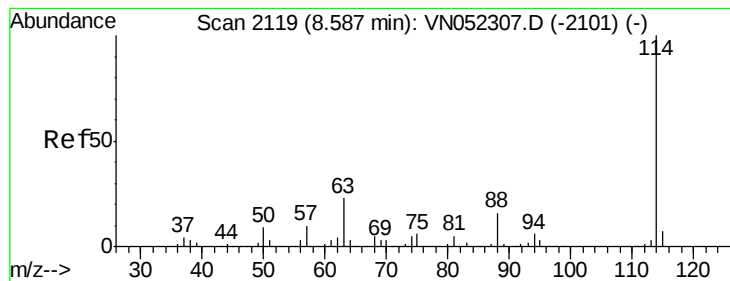

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. 0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:114 Resp: 511162

Ion Ratio Lower Upper

114 100

63 23.9 0.0 45.4

88 15.8 0.0 31.2




Abundance Ion 113.90 (113.60 to 114.60): V


Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

Time-->



Time-->

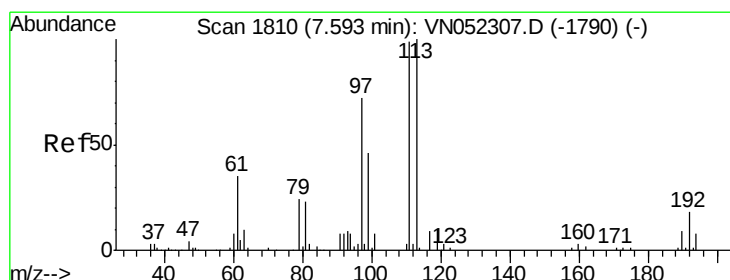

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. 0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57


Tgt Ion:113 Resp: 168603

Ion Ratio Lower Upper

113 100

111 103.2 81.0 121.6

192 17.2 13.8 20.6

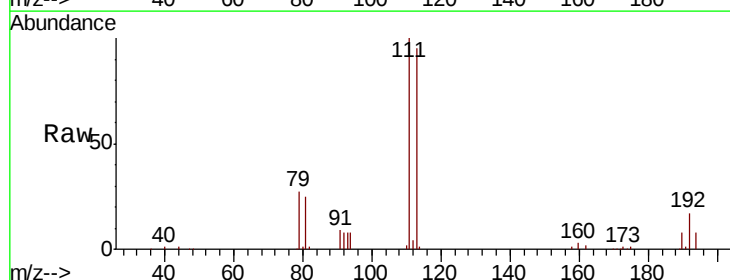


Abundance Ion 112.80 (112.50 to 113.50): V


Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

Time-->

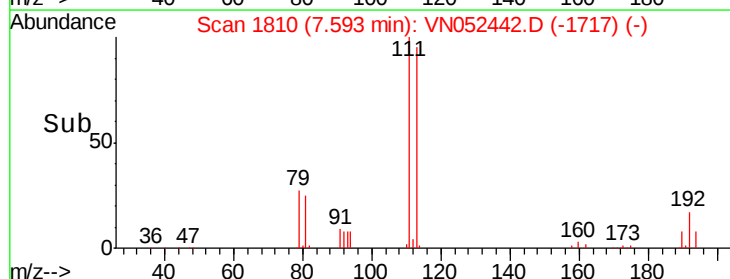





Time-->

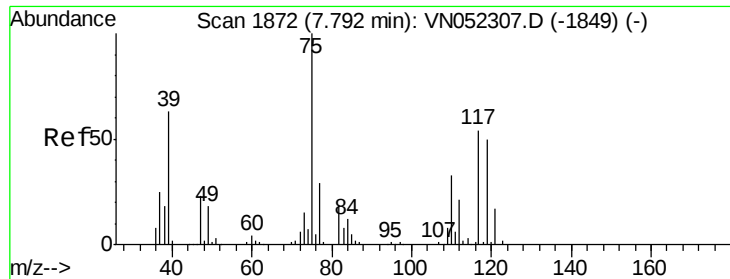

#36
 1,1-Dichloropropene
 Concen: 5.559 ug/l
 RT: 7.66 min Scan# 1832
 Delta R.T. -0.13 min
 Lab File: VN052442.D
 Acq: 21 Nov 2018 16:57




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion: 75 Resp: 28483
 Ion Ratio Lower Upper
 75 100
 110 8.4 16.5 49.5#
 77 0.0 24.2 36.2#

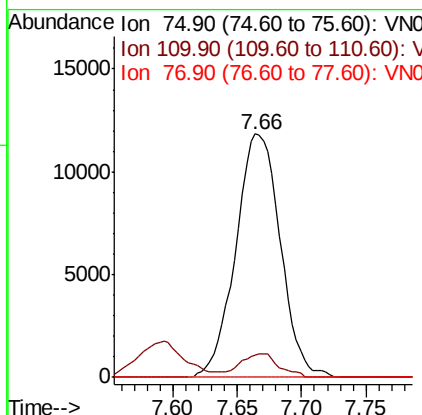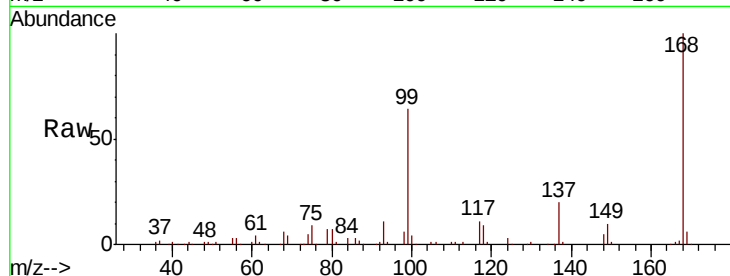

#38
 Carbon Tetrachloride
 Concen: 6.816 ug/l
 RT: 7.67 min Scan# 1833
 Delta R.T. -0.11 min
 Lab File: VN052442.D
 Acq: 21 Nov 2018 16:57

Tgt Ion: 117 Resp: 32082
 Ion Ratio Lower Upper
 117 100
 119 5.2 77.4 116.0#
 121 0.0 24.0 36.0#


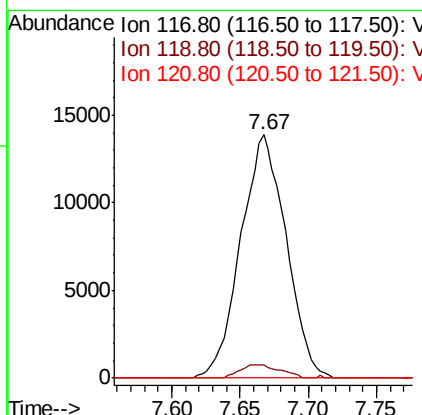






#41
Methacrylonitrile
Concen: 3.708 ug/l
RT: 7.18 min Scan# 1681
Delta R.T. 0.00 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion:	41	Resp:	29
Ion	Ratio	Lower	Upper
41	100		
39	134.5	0.0	0.0#
67	0.0	0.0	0.0
52	0.0	0.0	0.0

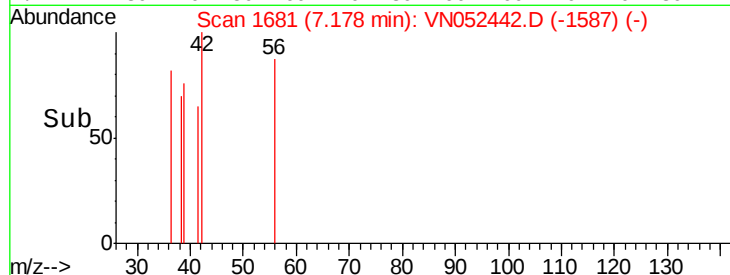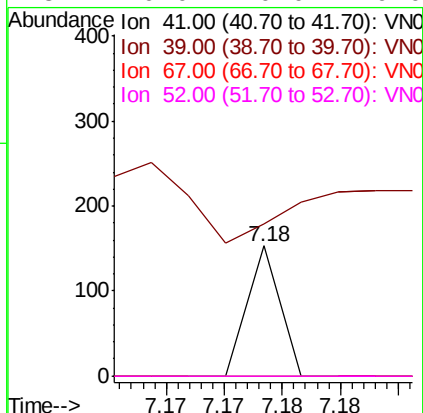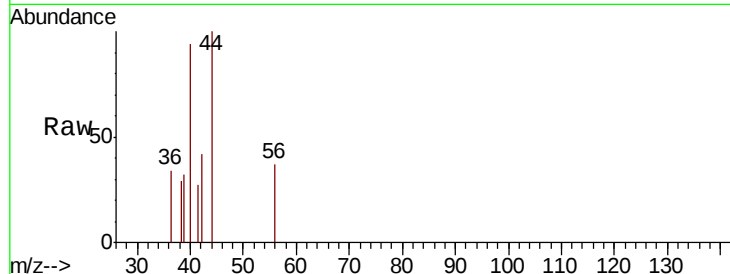

#43
Isopropyl Acetate
Concen: 2.777 ug/l
RT: 8.17 min Scan# 1989
Delta R.T. 0.01 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57

Tgt Ion:	43	Resp:	19922
Ion	Ratio	Lower	Upper
43	100		
61	14.3	12.0	18.0
87	5.7	8.3	12.5#



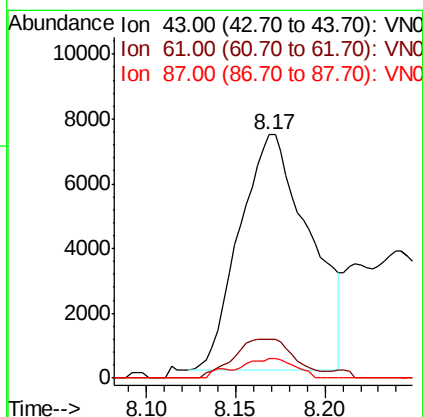
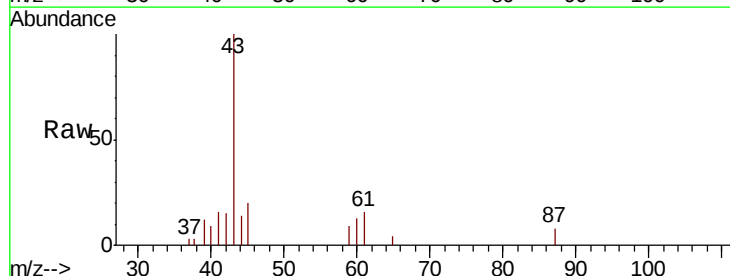


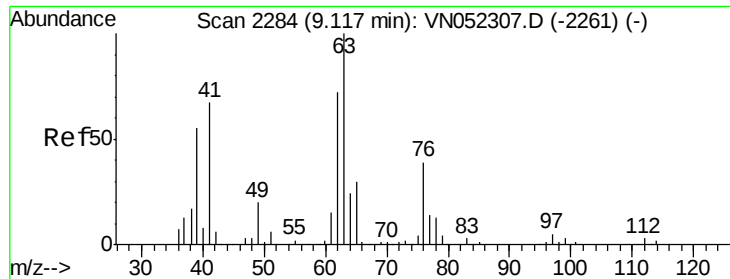

#45
 1,2-Dichloropropane
 Concen: 0.221 ug/l
 RT: 9.27 min Scan# 2332
 Delta R.T. 0.15 min
 Lab File: VN052442.D
 Acq: 21 Nov 2018 16:57




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion: 63 Resp: 920
 Ion Ratio Lower Upper
 63 100
 65 0.0 24.2 36.4#

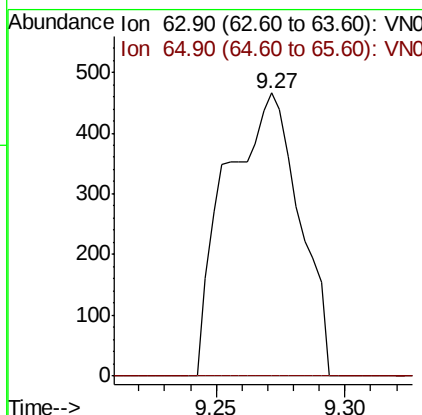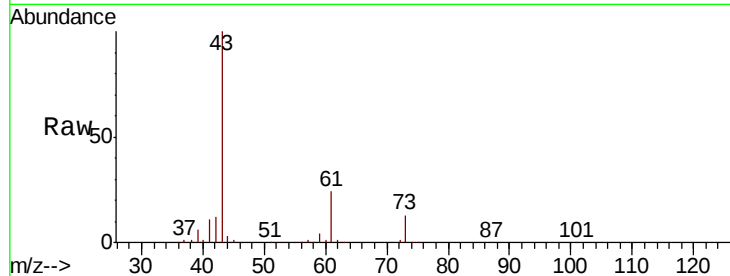

#48
 Methyl methacrylate
 Concen: 1.319 ug/l
 RT: 9.18 min Scan# 2303
 Delta R.T. -0.02 min
 Lab File: VN052442.D
 Acq: 21 Nov 2018 16:57

Tgt Ion: 41 Resp: 4801
 Ion Ratio Lower Upper
 41 100
 69 0.0 57.1 85.7#
 39 0.0 52.5 78.7#

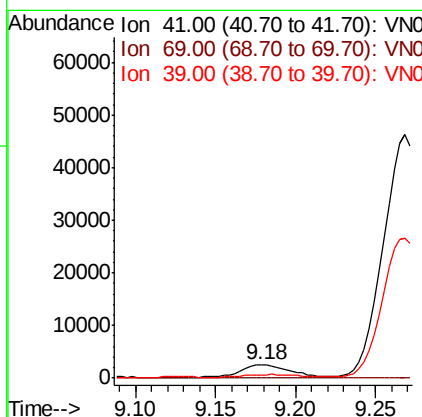

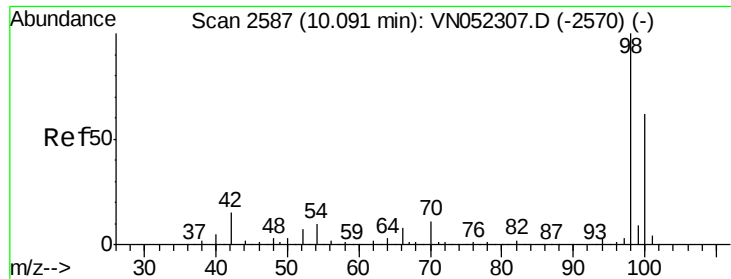

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion: 98 Resp: 648587


Ion Ratio Lower Upper

98 100



100 62.2 49.5 74.3

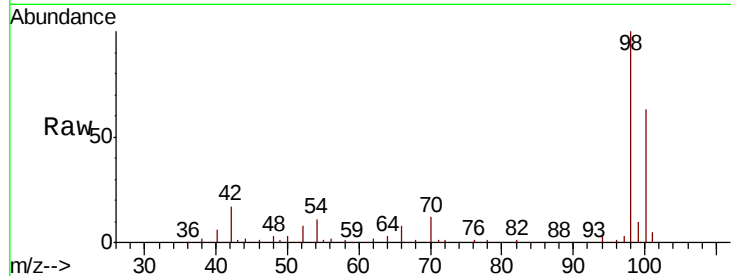

Abundance Ion 98.00 (97.70 to 98.70): VN052307.D (-2570) (-)

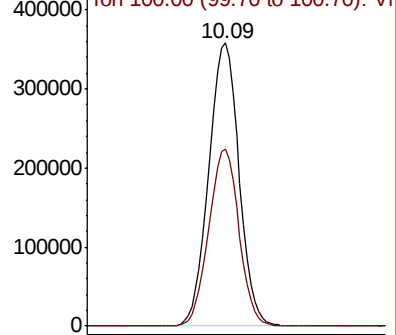

Time-->



#51

4-Methyl-2-Pentanone

Concen: 1.466 ug/l

RT: 10.02 min Scan# 2566

Delta R.T. 0.04 min

Lab File: VN052442.D


Acq: 21 Nov 2018 16:57

Tgt Ion: 43 Resp: 5295


Ion Ratio Lower Upper

43 100


58 0.0 27.0 40.6#




Abundance Ion 43.00 (42.70 to 43.70): VN052307.D (-2535) (-)

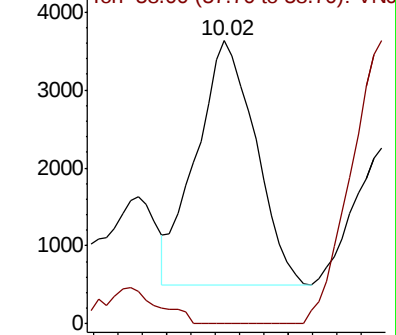

Time-->



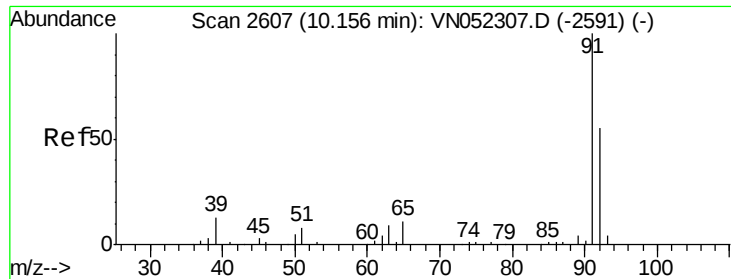

#52

Toluene

Concen: 0.270 ug/l

RT: 10.16 min Scan# 2607

Delta R.T. 0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 92 Resp: 2367

Ion Ratio Lower Upper




92 100

91 176.0 143.6 215.4

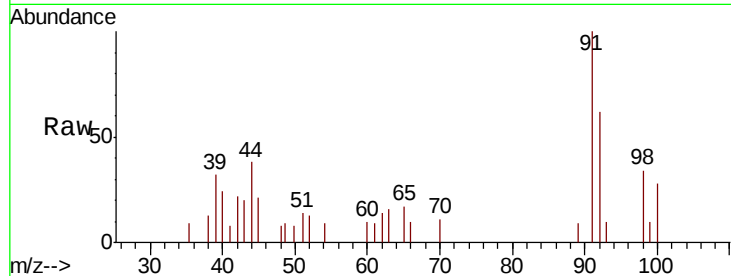

Abundance Ion 92.00 (91.70 to 92.70): VN0

Ion 91.00 (90.70 to 91.70): VN0

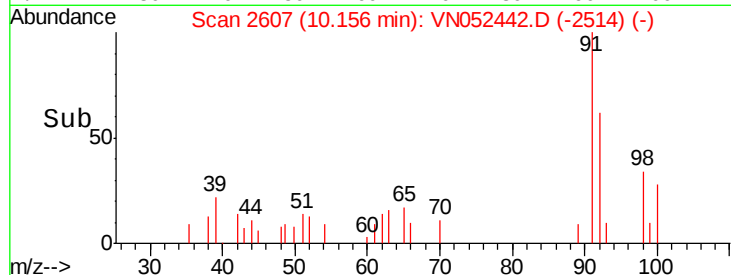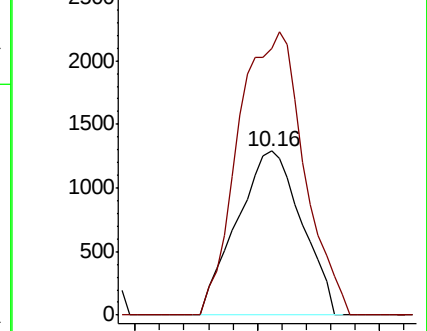

#54

cis-1,3-Dichloropropene

Concen: 4.886 ug/l

RT: 9.90 min Scan# 2529

Delta R.T. 0.07 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57


Tgt Ion: 75 Resp: 27719

Ion Ratio Lower Upper

75 100

77 0.0 24.6 36.8#



39 59.3 49.9 74.9




Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 76.90 (76.60 to 77.60): VN0

Ion 39.00 (38.70 to 39.70): VN0

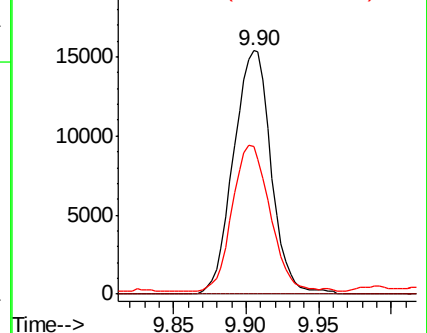



#57

1,3-Dichloropropane

Concen: 1.029 ug/l

RT: 10.77 min Scan# 2797

Delta R.T. 0.06 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion: 76 Resp: 5787

Ion Ratio Lower Upper




76 100

78 0.0 25.7 38.5#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

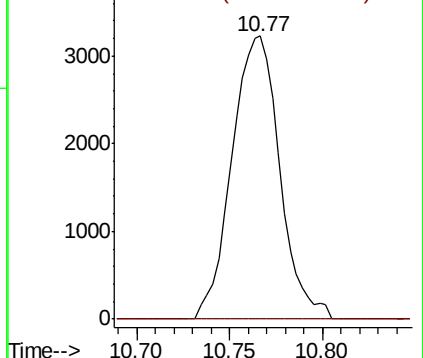

#59

2-Hexanone

Concen: 40.880 ug/l

RT: 10.76 min Scan# 2796

Delta R.T. 0.01 min

Lab File: VN052442.D


Acq: 21 Nov 2018 16:57

Tgt Ion: 43 Resp: 101556

Ion Ratio Lower Upper



43 100


58 16.0 23.5 70.6#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0




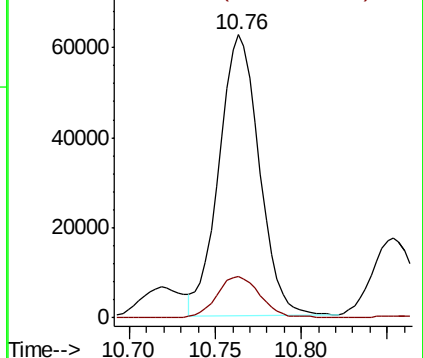




#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.00 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 95 Resp: 197449
Ion Ratio Lower Upper
95 100
174 73.4 0.0 156.0
176 70.9 0.0 148.4

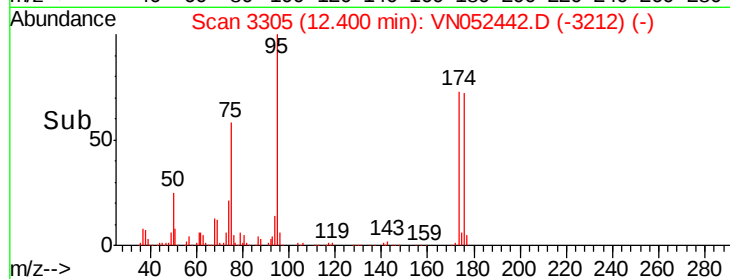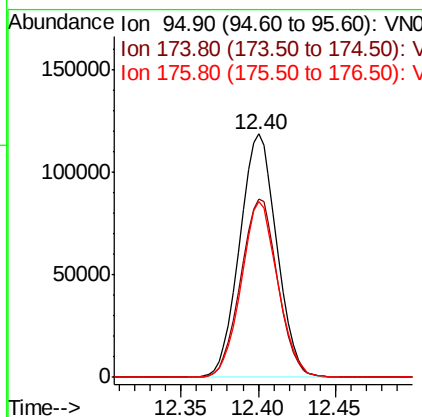

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57

Tgt Ion: 117 Resp: 437711
Ion Ratio Lower Upper
117 100
82 60.9 46.5 69.7
119 32.1 25.7 38.5



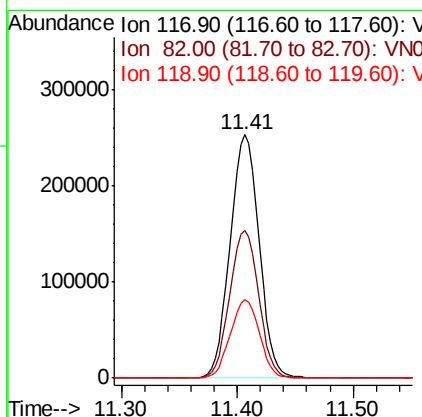





#68
m/p-Xvlenes
Concen: 0.213 ug/l
RT: 11.62 min Scan# 3063
Delta R.T. 0.00 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57




Instrument :
MSVOA_N
ClientSampled :


Tot Ion:106 Resp: 1249
Ion Ratio Lower Upper
106 100
91 197.5 165.5 248.3

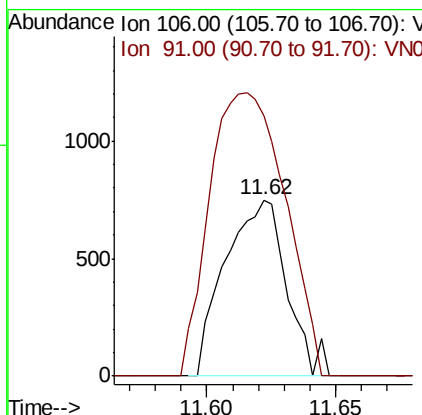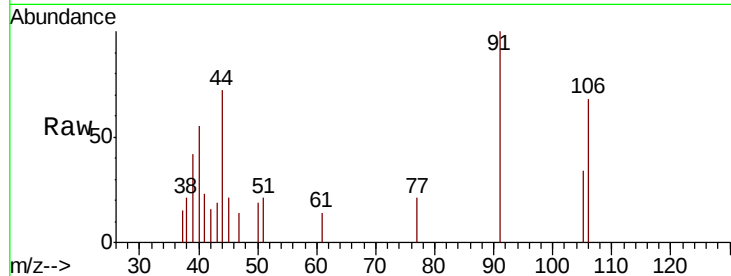

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN052442.D
Acq: 21 Nov 2018 16:57

Tgt Ion:152 Resp: 154709
Ion Ratio Lower Upper
152 100
115 61.8 30.3 91.0
150 158.4 0.0 348.2

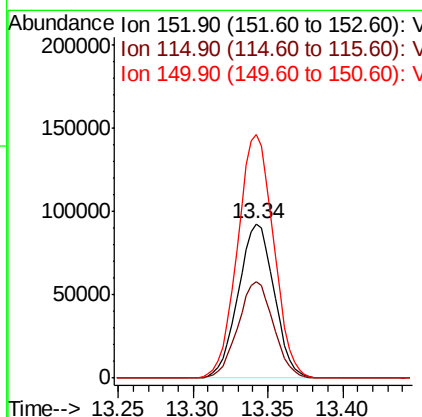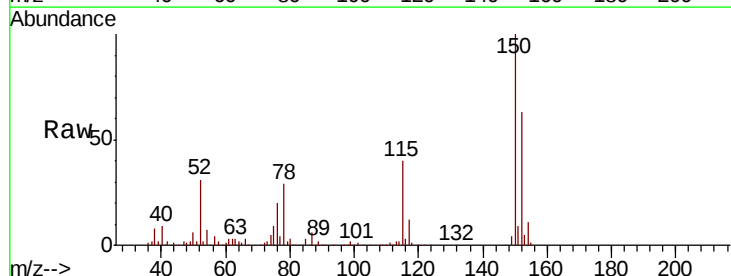



#74

N-amvl acetate

Concen: 2.050 ug/l

RT: 11.88 min Scan# 3142

Delta R.T. -0.19 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57

Instrument :

MSVOA_N

ClientSampleId :

Tot Ion: 43 Resp: 9080



Ion Ratio Lower Upper

43 100

70 0.0 27.1 40.7#

55 8.1 17.4 26.0#

61 9.0 16.1 24.1#


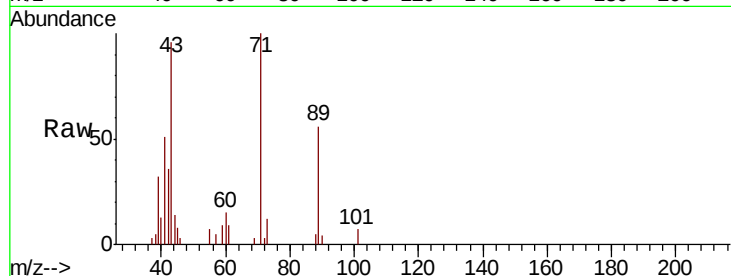


Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

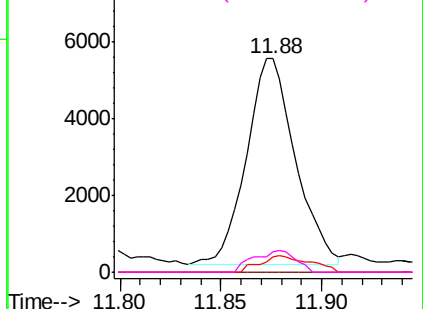

#76

1,2,3-Trichloropropane

Concen: 43.645 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.15 min

Lab File: VN052442.D



Acq: 21 Nov 2018 16:57

Tgt Ion: 75 Resp: 114573

Ion Ratio Lower Upper


75 100


77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

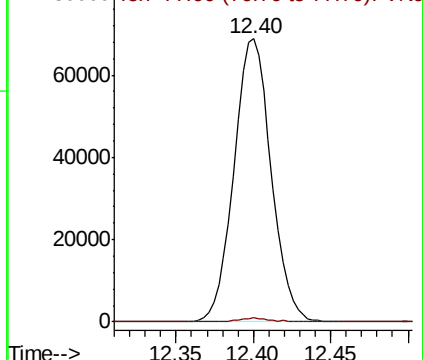



#80

1,3,5-Trimethylbenzene

Concen: 0.450 ug/l

RT: 12.73 min Scan# 3408

Delta R.T. 0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57

Instrument :

MSVOA_N


ClientSampled :

Tot Ion:105 Resp: 4456

Ion Ratio Lower Upper




105 100

120 44.4 23.7 71.1



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

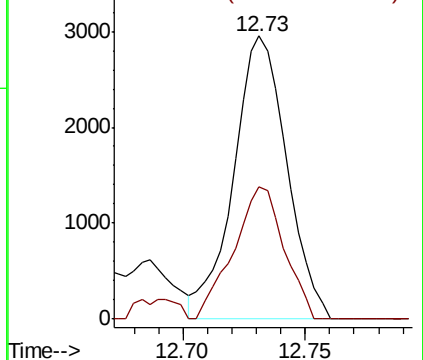

#81

trans-1,4-Dichloro-2-butene

Concen: 141.557 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.10 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57


Tgt Ion: 75 Resp: 114573

Ion Ratio Lower Upper

75 100

53 0.0 90.2 135.2#



89 0.0 35.4 53.0#




Abundance Ion 74.90 (74.60 to 75.60): VNO

Ion 53.00 (52.70 to 53.70): VNO

Ion 88.90 (88.60 to 89.60): VNO

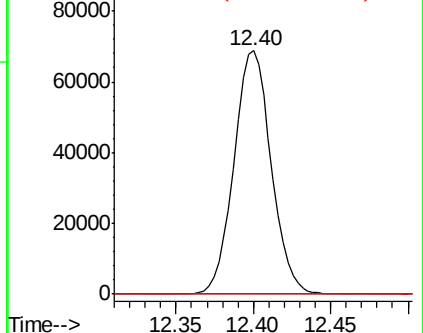

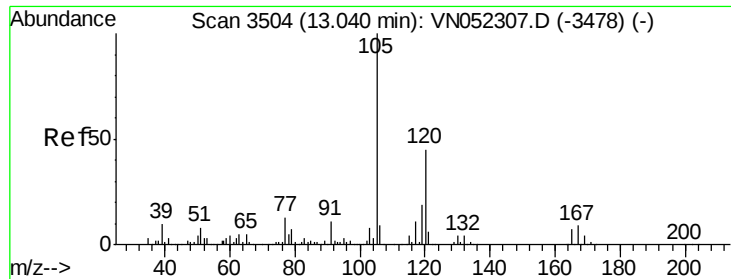

#84

1,2,4-Trimethylbenzene

Concen: 0.485 ug/l

RT: 13.04 min Scan# 3504

Delta R.T. 0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion:105 Resp: 4818

Ion Ratio Lower Upper

105 100

120 42.1 22.5 67.5

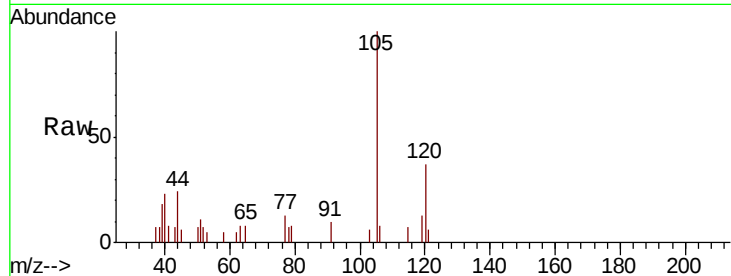

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

3000



2000

1000

0

13.00 13.05

Time-->



#95

Naphthalene

Concen: 3.062 ug/l

RT: 15.14 min Scan# 4156

Delta R.T. 0.00 min

Lab File: VN052442.D

Acq: 21 Nov 2018 16:57


Tgt Ion:128 Resp: 2643

Ion Ratio Lower Upper

128 100

127 8.1 10.4 15.6#

129 8.8 8.6 13.0



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

2000

1500

1000

500

0

15.10 15.15

Time-->

