


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN112118\
 Data File : VN052425.D
 Acq On : 21 Nov 2018 9:11
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
 Title : SW846 8260
 Last Update : Thu Nov 15 03:02:37 2018

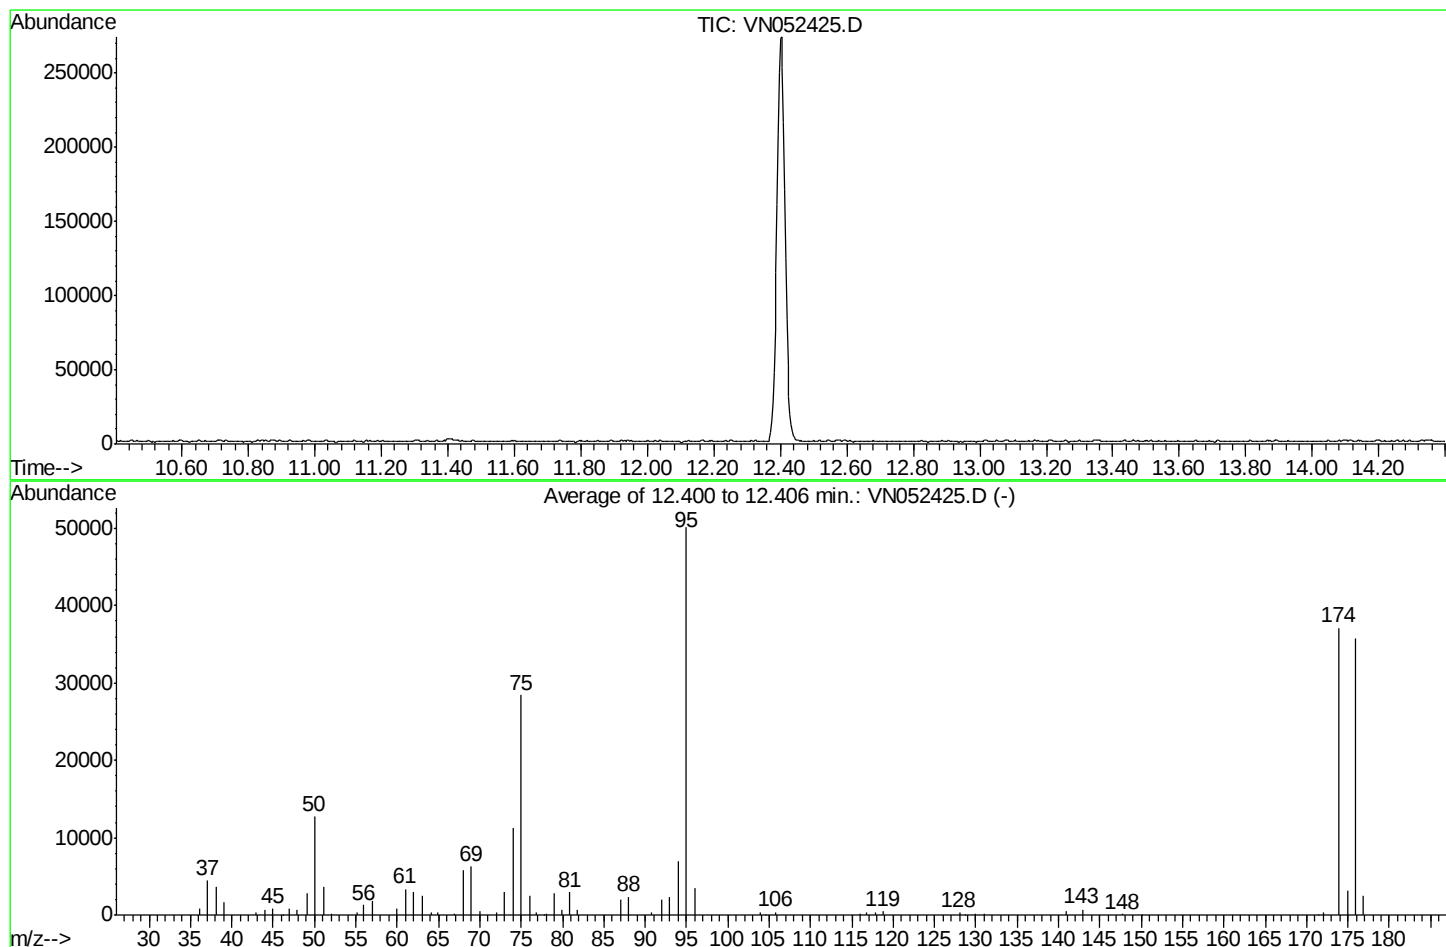

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.4	12746	PASS
75	95	30	60	56.8	28469	PASS
95	95	100	100	100.0	50136	PASS
96	95	5	9	6.8	3410	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.1	37152	PASS
175	174	5	9	8.6	3199	PASS
176	174	95	101	96.0	35682	PASS
177	176	5	9	7.1	2547	PASS