


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN112119\
Data File : VN059327.D
Acq On : 21 Nov 2019 9:25
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112019W.M
Title : SW846 8260
Last Update : Thu Nov 21 08:44:45 2019

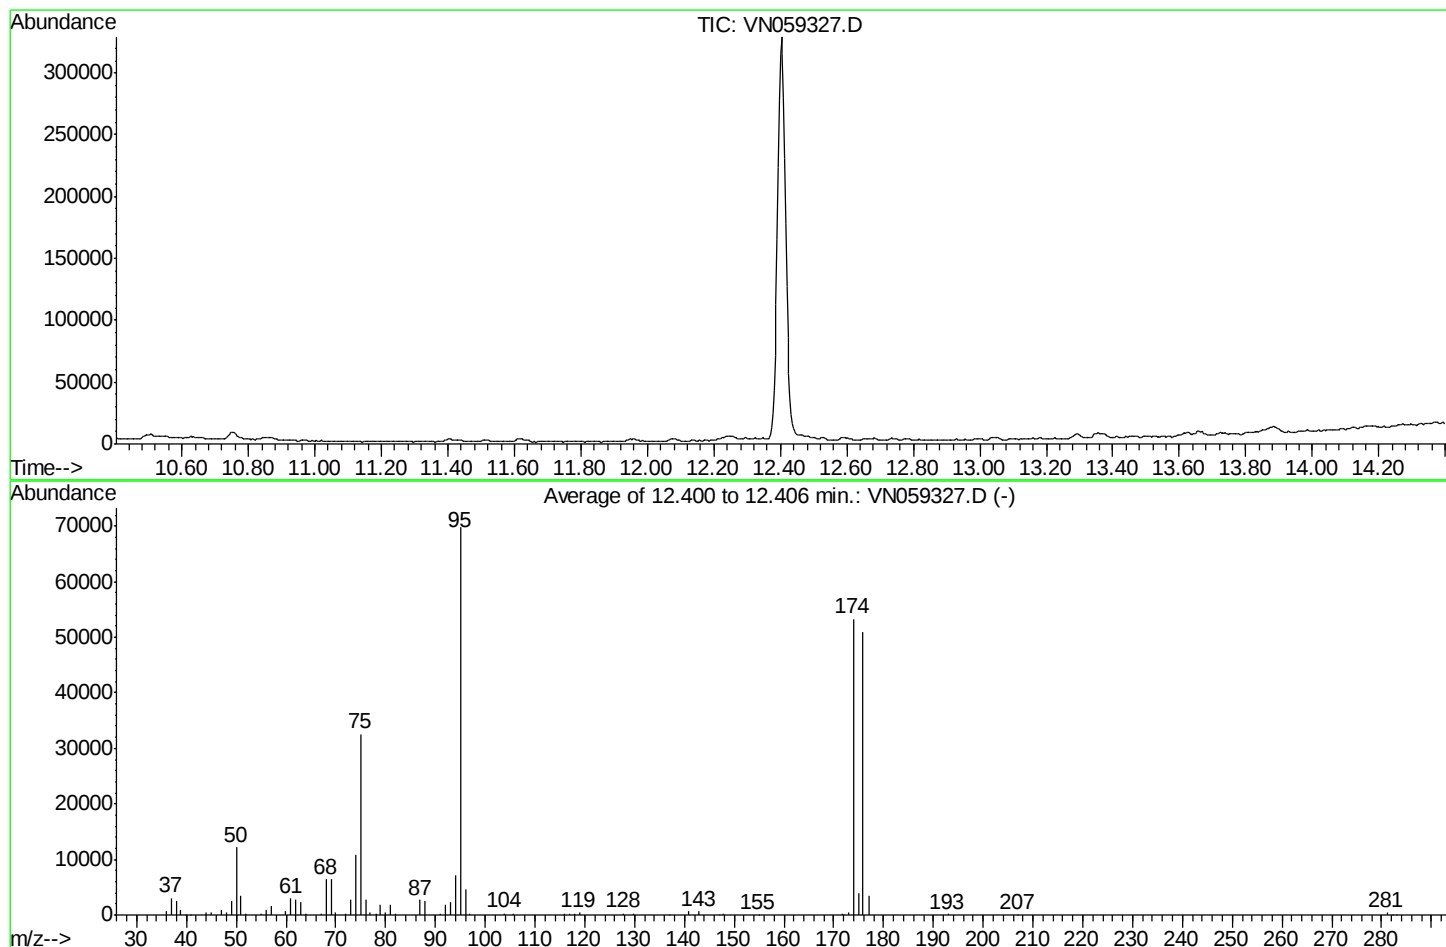

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	12141	PASS
75	95	30	60	46.6	32493	PASS
95	95	100	100	100.0	69781	PASS
96	95	5	9	6.6	4601	PASS
173	174	0.00	2	0.9	467	PASS
174	95	50	100	76.4	53344	PASS
175	174	5	9	7.5	3980	PASS
176	174	95	101	95.6	51018	PASS
177	176	5	9	6.6	3361	PASS