
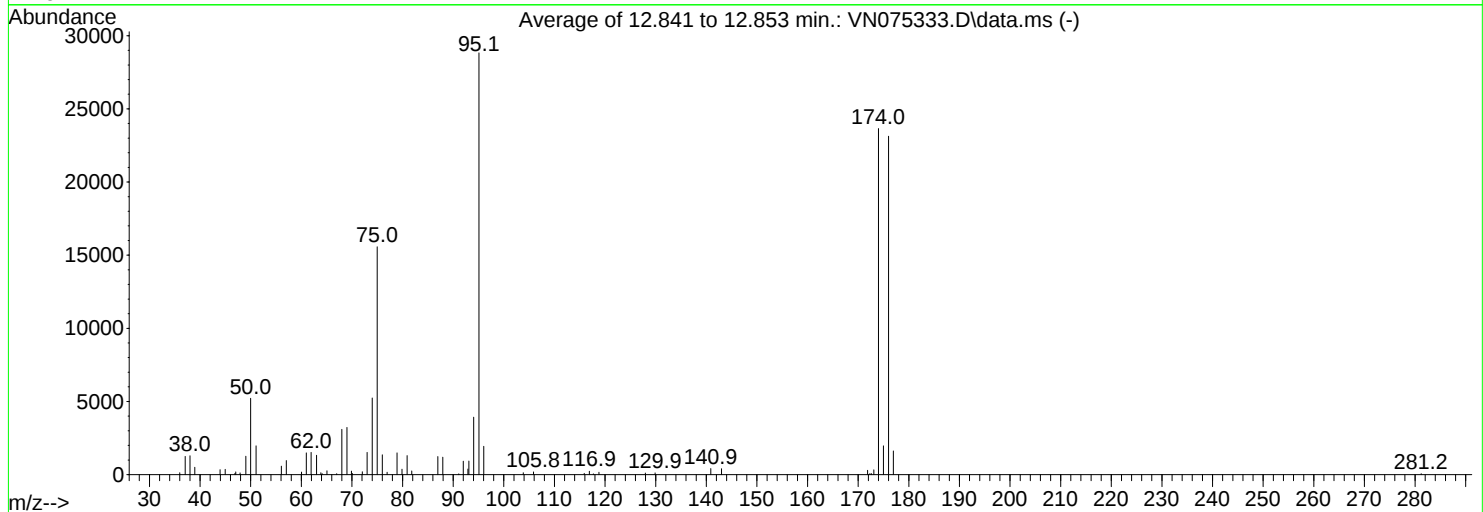


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112122\
 Data File : VN075333.D
 Acq On : 21 Nov 2022 09:19
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Title : SW846 8260
 Last Update : Wed Nov 23 00:18:03 2022

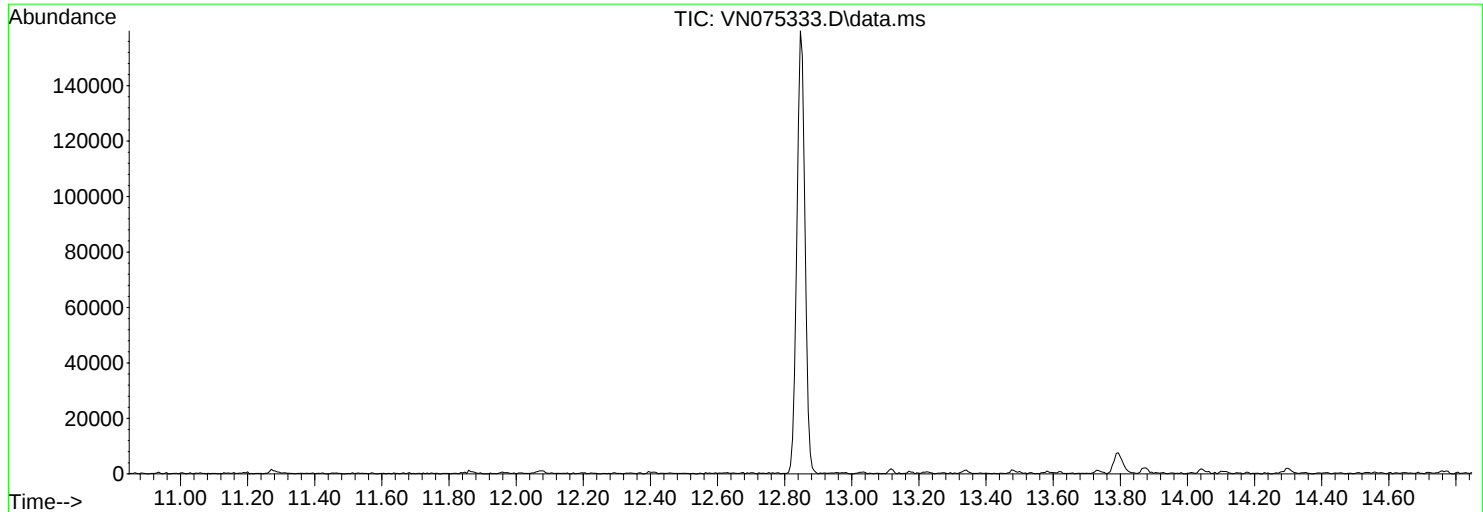

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	5212	PASS
75	95	30	60	54.0	15570	PASS
95	95	100	100	100.0	28829	PASS
96	95	5	9	6.7	1935	PASS
173	174	0.00	2	1.4	328	PASS
174	95	50	100	82.0	23651	PASS
175	174	5	9	8.3	1972	PASS
176	174	95	101	97.8	23131	PASS
177	176	5	9	7.0	1615	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	131	51.05	1974	68.00	3099	79.90	361
37.05	1247	56.05	578	69.00	3221	80.90	1307
38.00	1292	57.05	959	69.90	242	81.80	24
38.95	507	60.05	177	70.10	79	86.95	123
43.95	342	61.00	1491	72.05	197	87.95	1195
44.95	361	61.95	1519	73.00	1518	91.10	55
46.90	85	63.00	1324	74.00	5239	92.00	922
47.05	184	63.85	129	75.00	15570	92.90	384
47.90	123	64.10	65	76.00	1358	93.10	935
49.05	1256	65.05	261	76.95	164	94.05	3923
50.00	5212	67.00	62	78.90	1487	95.10	28829

Average of 12.841 to 12.853 min.: VN075333.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	1935	171.85	295				
103.85	133	172.30	64				
105.85	186	172.60	79				
115.90	86	173.10	328				
116.90	232	174.00	23651				
117.70	53	175.00	1972				
118.80	159	176.00	23131				
127.95	115	176.95	1615				
129.90	120	281.20	69				
140.90	412						
143.00	410						

Instrument :

MSVOA_N

ClientSampleId :

BFB