
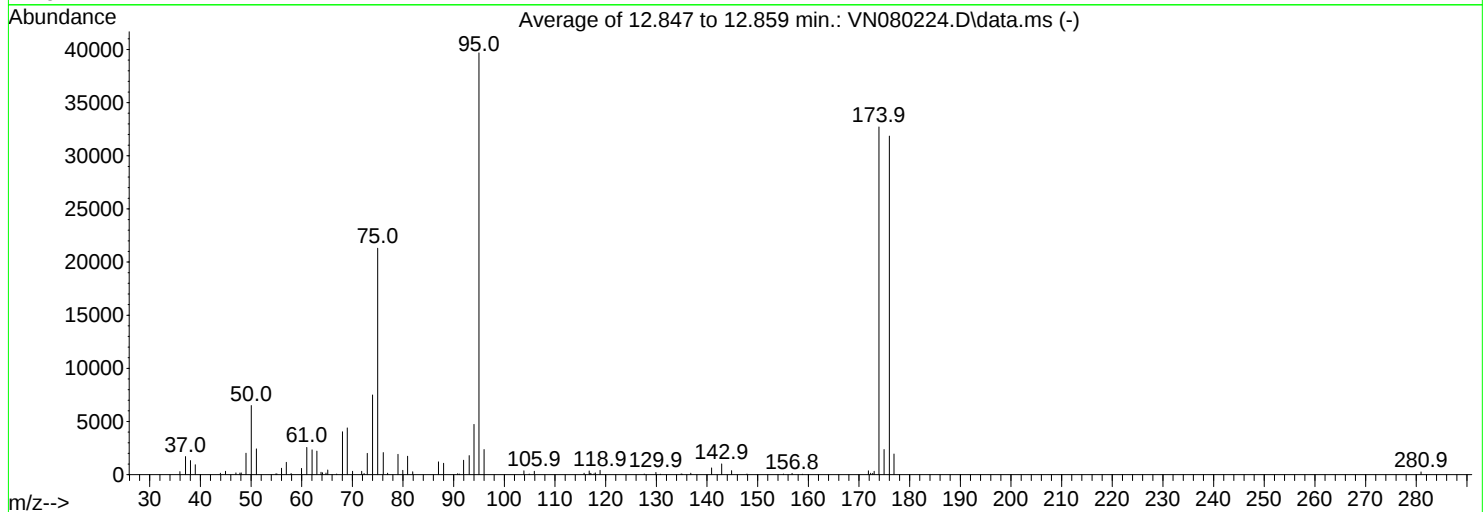


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112123\
Data File : VN080224.D
Acq On : 21 Nov 2023 09:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

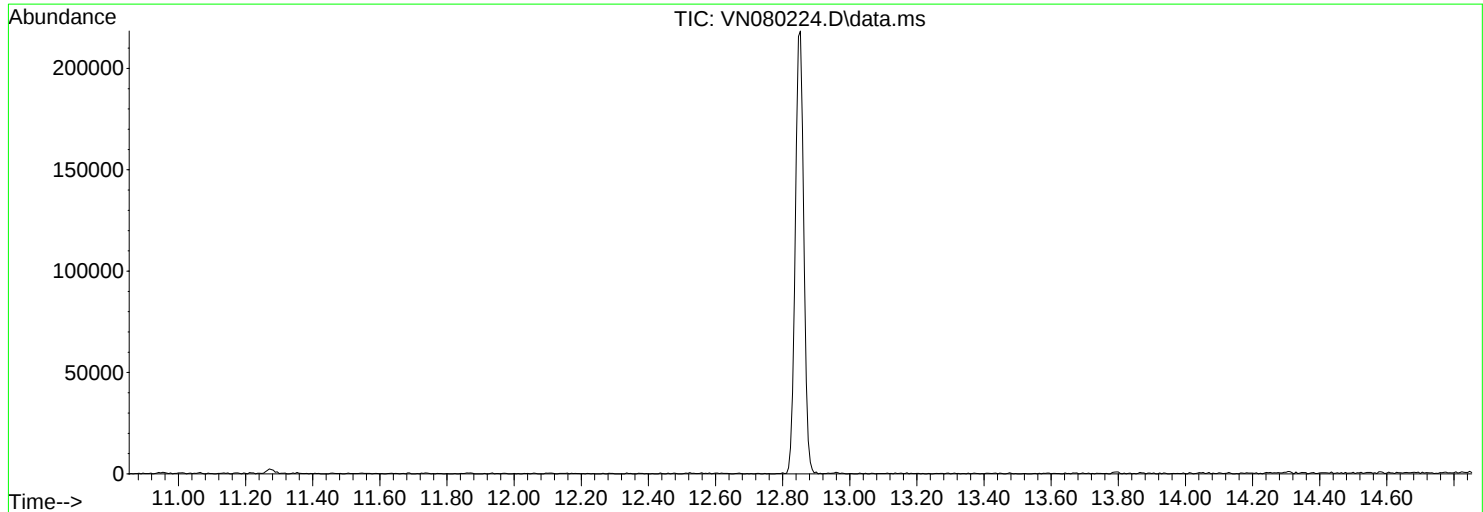

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	6499	PASS
75	95	30	60	53.7	21301	PASS
95	95	100	100	100.0	39685	PASS
96	95	5	9	6.0	2368	PASS
173	174	0.00	2	1.0	314	PASS
174	95	50	100	82.4	32707	PASS
175	174	5	9	7.2	2364	PASS
176	174	95	101	97.4	31856	PASS
177	176	5	9	6.1	1939	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	293	50.05	6499	63.80	220	74.00	750
37.05	1694	51.05	2427	64.10	182	75.00	2130
38.05	1329	54.90	79	64.80	147	76.10	208
39.00	935	55.10	82	65.15	432	76.95	13
40.00	15	56.00	609	66.90	58	79.00	1913
43.95	137	56.95	1159	68.05	4032	79.95	400
44.95	314	57.90	106	69.00	4403	80.90	1736
47.00	166	59.95	589	70.05	319	81.90	268
47.80	149	61.00	2565	71.85	310	87.00	1211
48.05	164	62.05	2328	72.30	101	88.00	1064
49.00	2014	63.00	2212	72.95	1999	90.80	94

Average of 12.847 to 12.859 min.: VN080224.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.10	63	116.90	130	140.90	636	173.95	32707
91.95	1354	117.10	103	142.90	1008	174.95	2364
93.05	1786	117.70	82	144.85	379	176.00	31856
94.00	4729	117.95	160	147.90	56	176.90	1939
95.00	39685	118.90	404	155.10	55	280.95	253
96.00	2368	127.60	59	156.80	114		
103.85	362	129.90	212	158.80	53		
104.90	60	130.80	53	171.85	369		
105.90	314	134.90	71	172.30	136		
115.75	142	135.10	52	172.70	114		
116.75	341	136.80	131	173.00	314		

Instrument :

MSVOA_N

ClientSampleId :

BFB