


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112219\
Data File : VN059350.D
Acq On : 22 Nov 2019 9:02
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112019W.M
Title : SW846 8260
Last Update : Thu Nov 21 08:44:45 2019

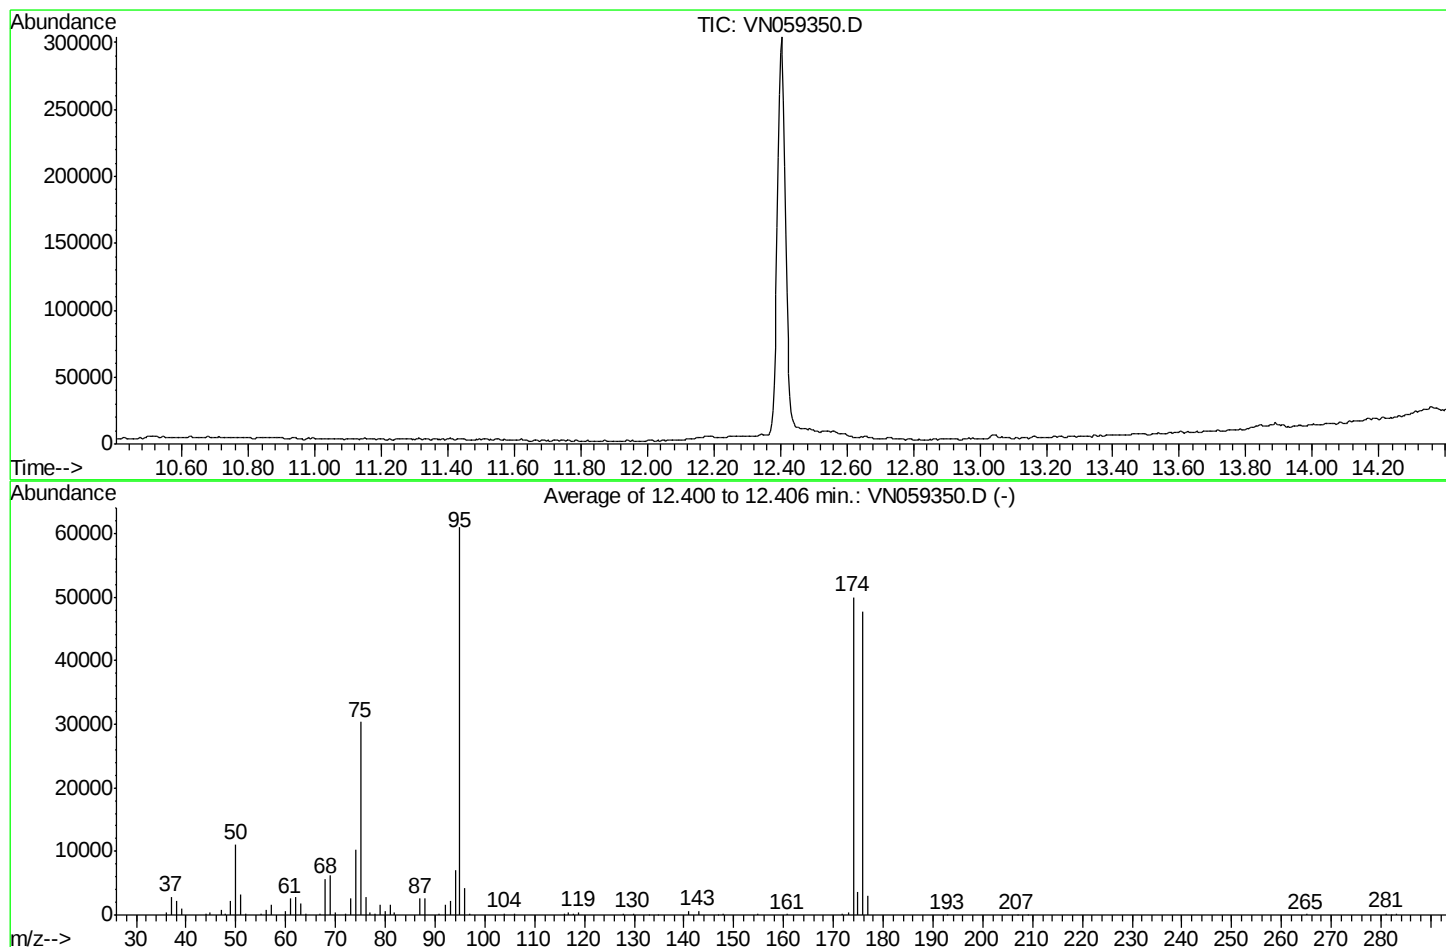

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	11017	PASS
75	95	30	60	49.8	30330	PASS
95	95	100	100	100.0	60954	PASS
96	95	5	9	6.9	4193	PASS
173	174	0.00	2	0.8	408	PASS
174	95	50	100	82.0	49981	PASS
175	174	5	9	7.1	3559	PASS
176	174	95	101	95.4	47669	PASS
177	176	5	9	6.5	3107	PASS