

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112222\
 Data File : VN075358.D
 Acq On : 22 Nov 2022 11:19
 Operator : JC\MD
 Sample : VN1122WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1122WBL01

Quant Time: Nov 23 07:04:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	136397	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	237134	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	207478	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	88609	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	40154	54.843	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	109.680%
35) Dibromofluoromethane	8.171	113	48436	51.996	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.000%
50) Toluene-d8	10.571	98	103257	49.215	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.420%
62) 4-Bromofluorobenzene	12.847	95	72276	46.671	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112222\
Data File : VN075358.D
Acq On : 22 Nov 2022 11:19
Operator : JC\MD
Sample : VN1122WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1122WBL01

Quant Time: Nov 23 07:04:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration




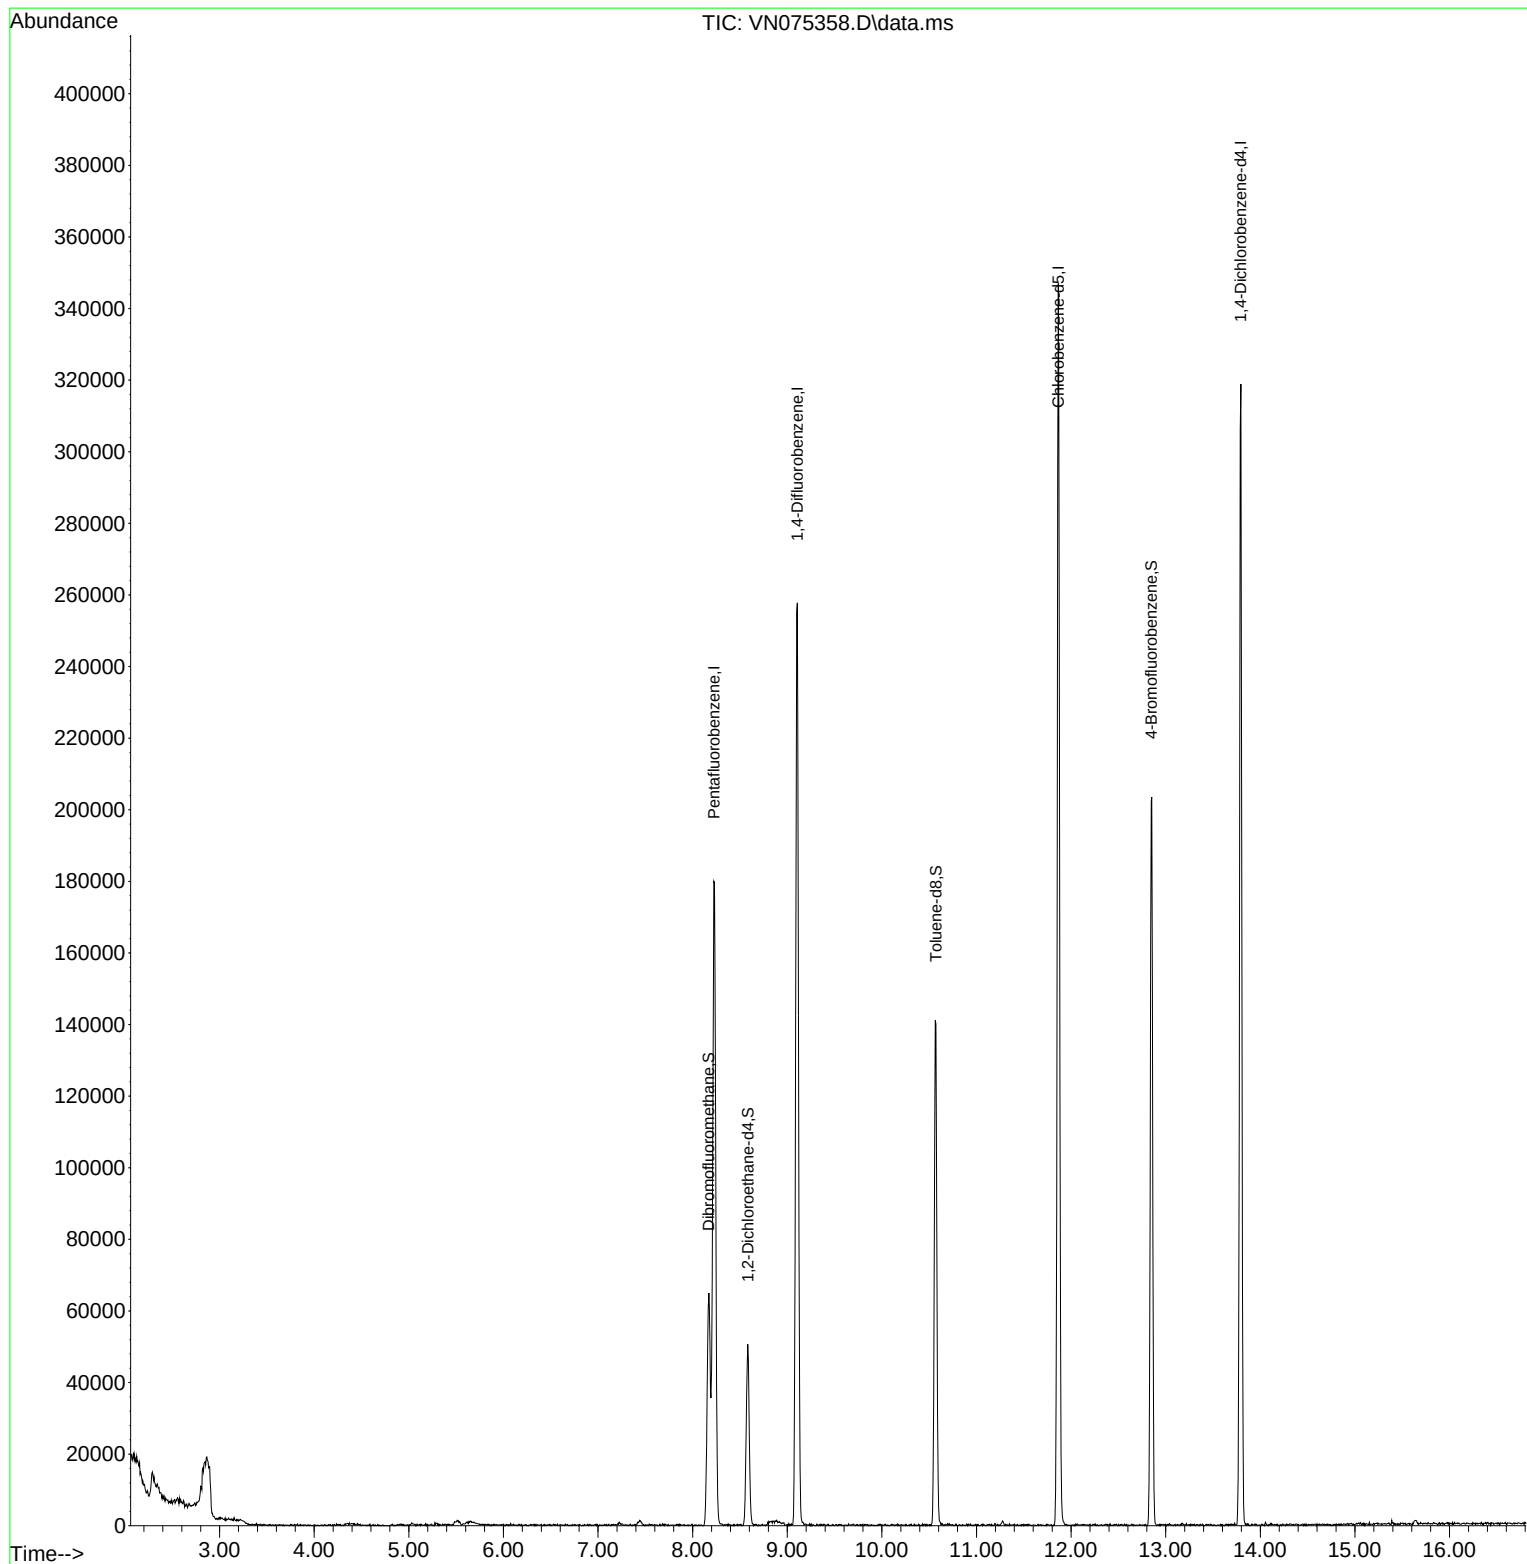


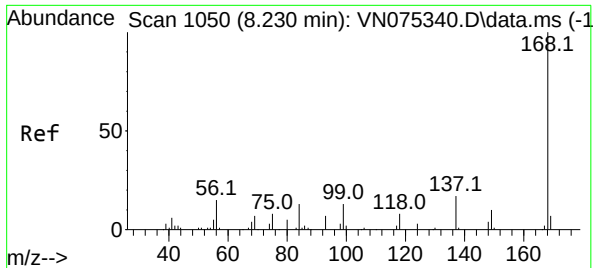

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1049
Delta R.T. -0.006 min
Lab File: VN075358.D
Acq: 22 Nov 2022 11:19




Instrument :
MSVOA_N
ClientSampleId :
VN1122WBL01


Tgt Ion:168 Resp: 136397
Ion Ratio Lower Upper
168 100
99 58.4 51.6 77.4

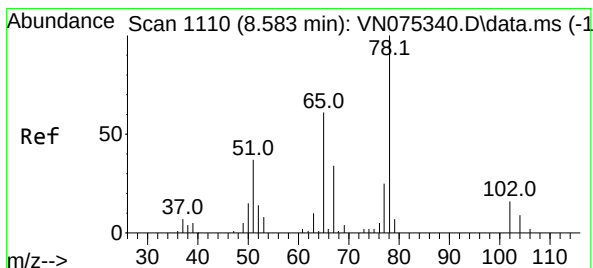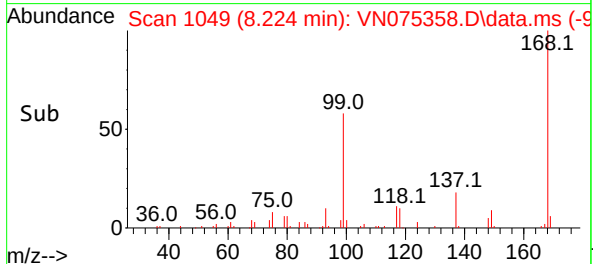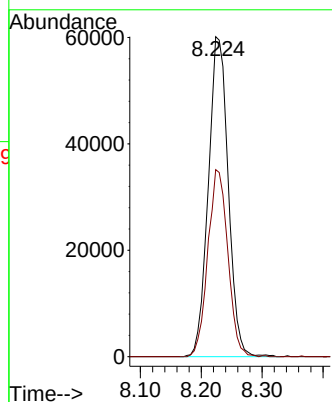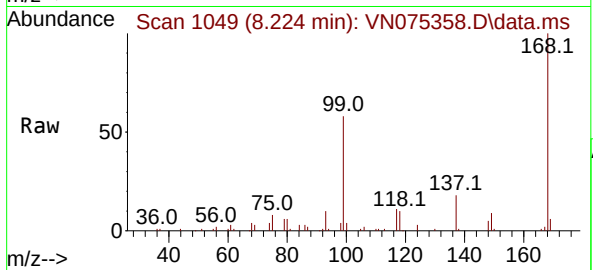

#33
1,2-Dichloroethane-d4
Concen: 54.843 ug/l
RT: 8.582 min Scan# 1110
Delta R.T. -0.001 min
Lab File: VN075358.D
Acq: 22 Nov 2022 11:19

Tgt Ion: 65 Resp: 40154
Ion Ratio Lower Upper
65 100
67 52.9 0.0 102.0

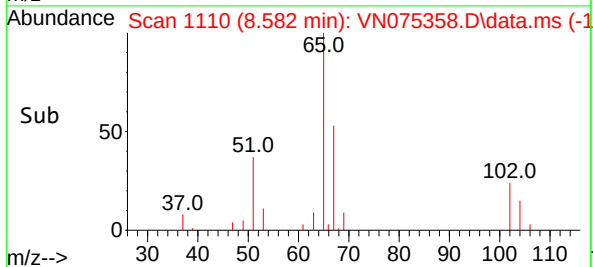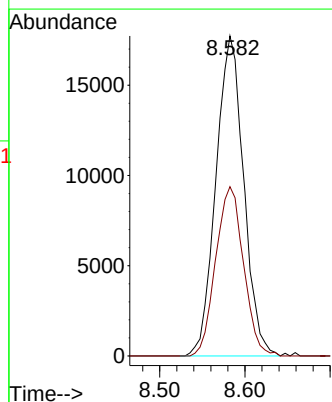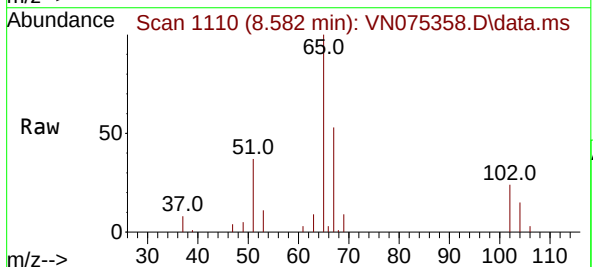

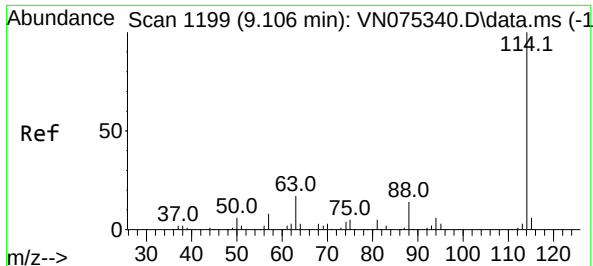

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075358.D

Acq: 22 Nov 2022 11:19

Instrument :

MSVOA_N

ClientSampleId :

VN1122WBL01





Tgt Ion:114 Resp: 237134

Ion Ratio Lower Upper

114 100

63 18.6 0.0 39.6

88 14.7 0.0 29.0

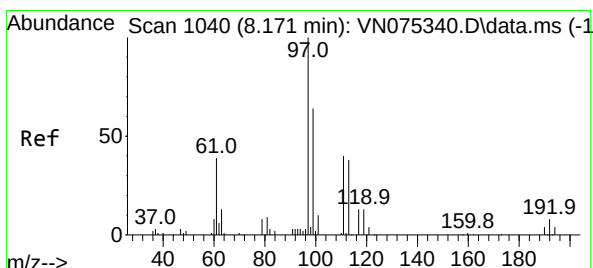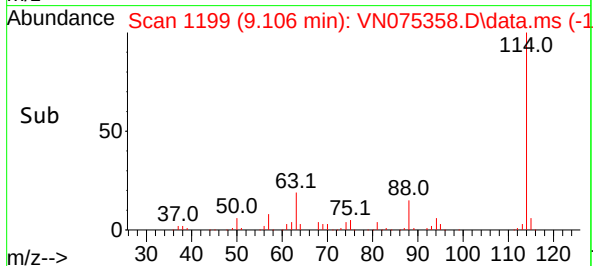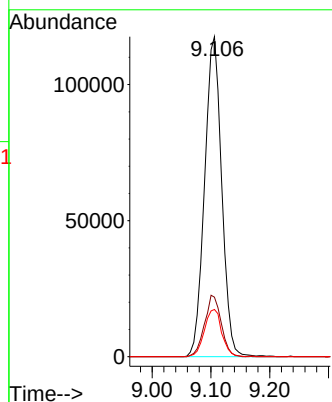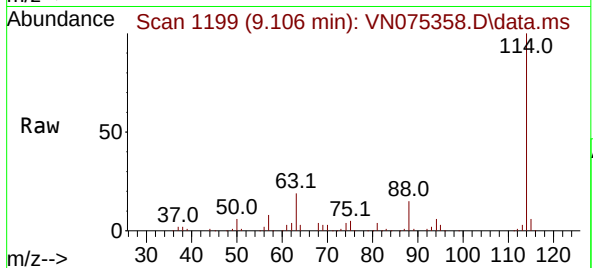

#35

Dibromofluoromethane

Concen: 51.996 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN075358.D

Acq: 22 Nov 2022 11:19




Tgt Ion:113 Resp: 48436


Ion Ratio Lower Upper

113 100

111 101.2 80.5 120.7

192 17.3 13.2 19.8


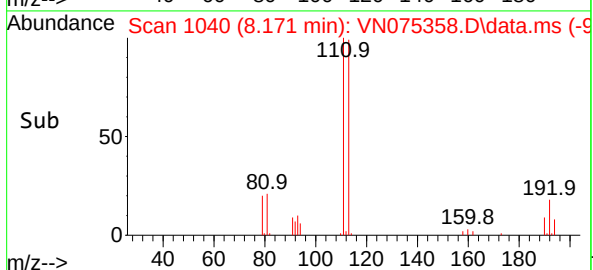
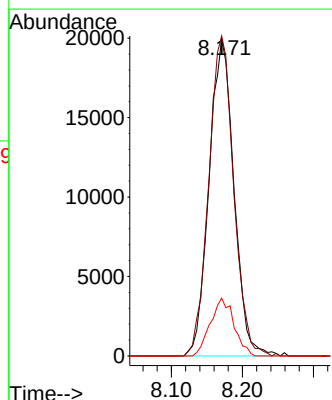
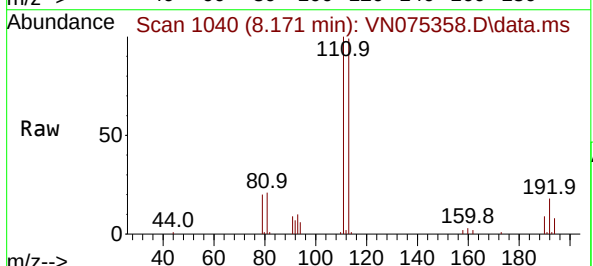


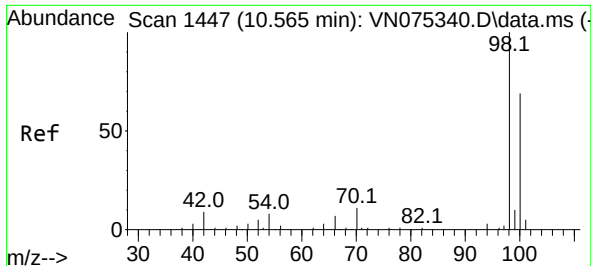

#50
Toluene-d8
Concen: 49.215 ug/l
RT: 10.571 min Scan# 1447
Delta R.T. 0.006 min
Lab File: VN075358.D
Acq: 22 Nov 2022 11:19




Instrument :
MSVOA_N
ClientSampleId :
VN1122WBL01


Tgt Ion: 98 Resp: 103257
Ion Ratio Lower Upper
98 100
100 65.7 53.0 79.6

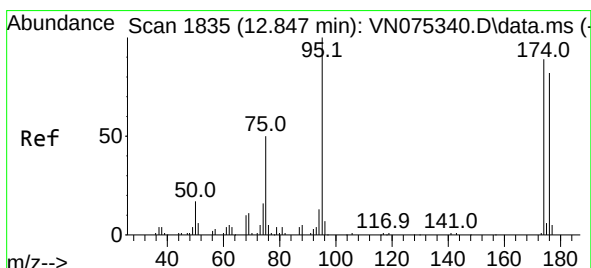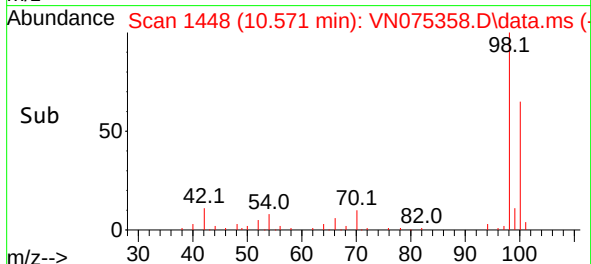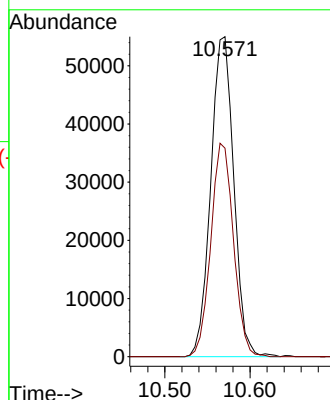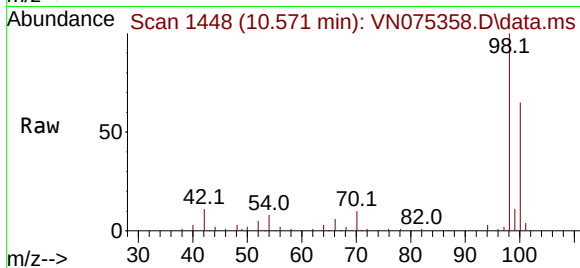

#62
4-Bromofluorobenzene
Concen: 46.671 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.000 min
Lab File: VN075358.D
Acq: 22 Nov 2022 11:19

Tgt Ion: 95 Resp: 72276
Ion Ratio Lower Upper
95 100
174 80.4 0.0 147.4
176 77.7 0.0 142.2


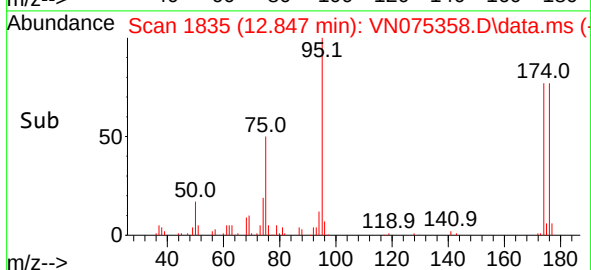
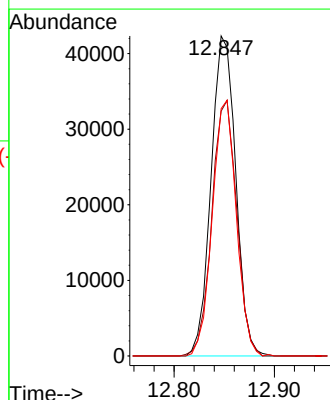
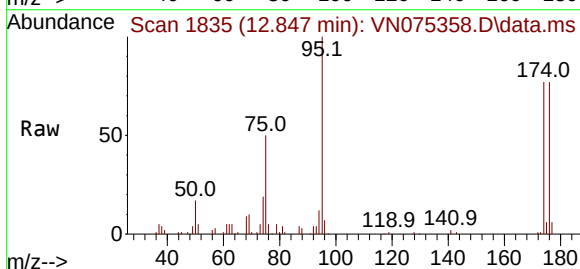


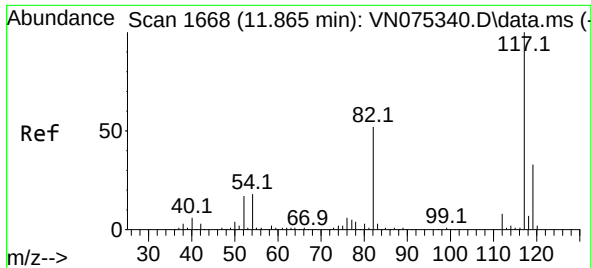

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN075358.D
Acq: 22 Nov 2022 11:19

Instrument :
MSVOA_N
ClientSampleId :
VN1122WBL01

Tgt Ion:117 Resp: 207478
Ion Ratio Lower Upper
117 100
82 51.8 43.1 64.7
119 31.9 25.5 38.3

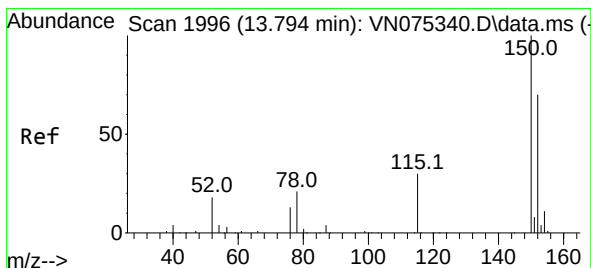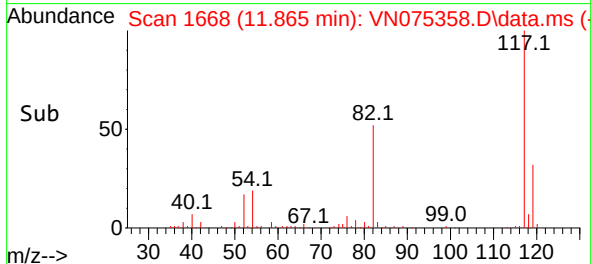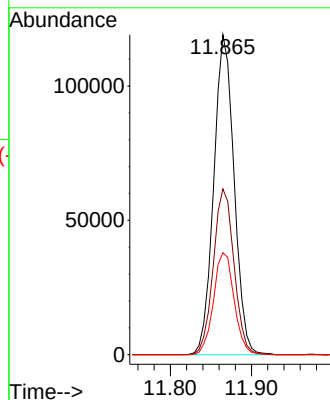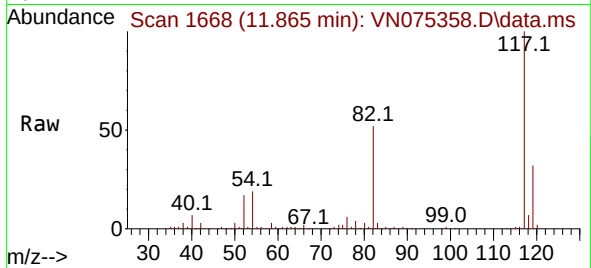

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075358.D
Acq: 22 Nov 2022 11:19

Tgt Ion:152 Resp: 88609
Ion Ratio Lower Upper
152 100
115 61.3 30.2 90.6
150 157.7 0.0 348.4

