
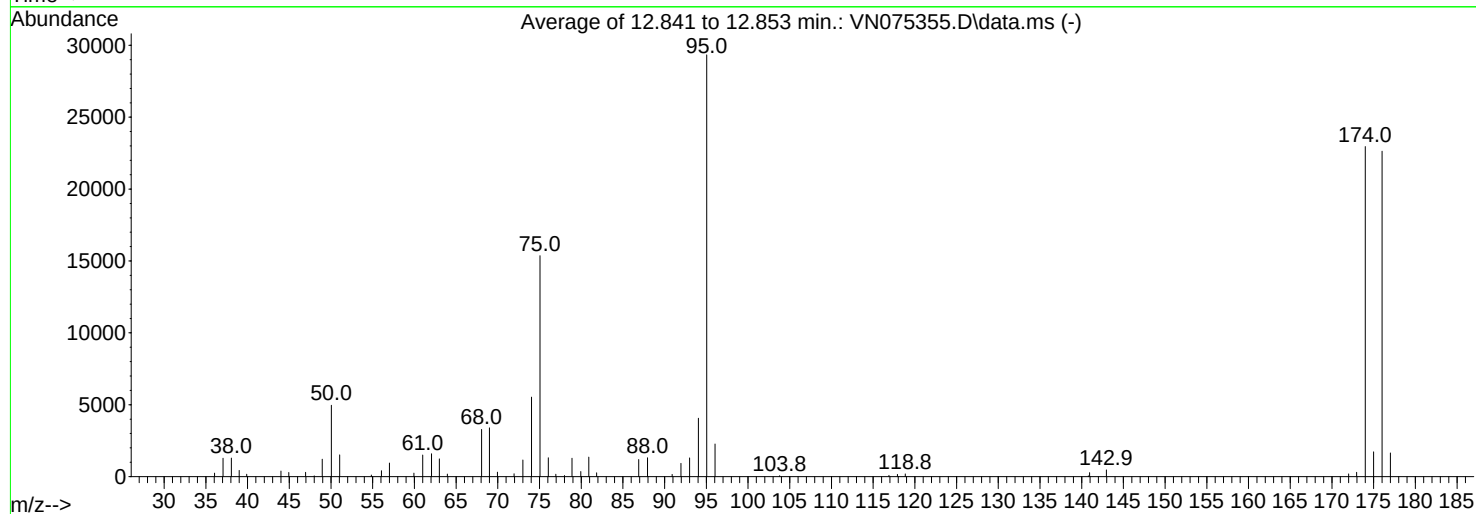


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112222\
Data File : VN075355.D
Acq On : 22 Nov 2022 09:45
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Title : SW846 8260
Last Update : Wed Nov 23 00:18:03 2022

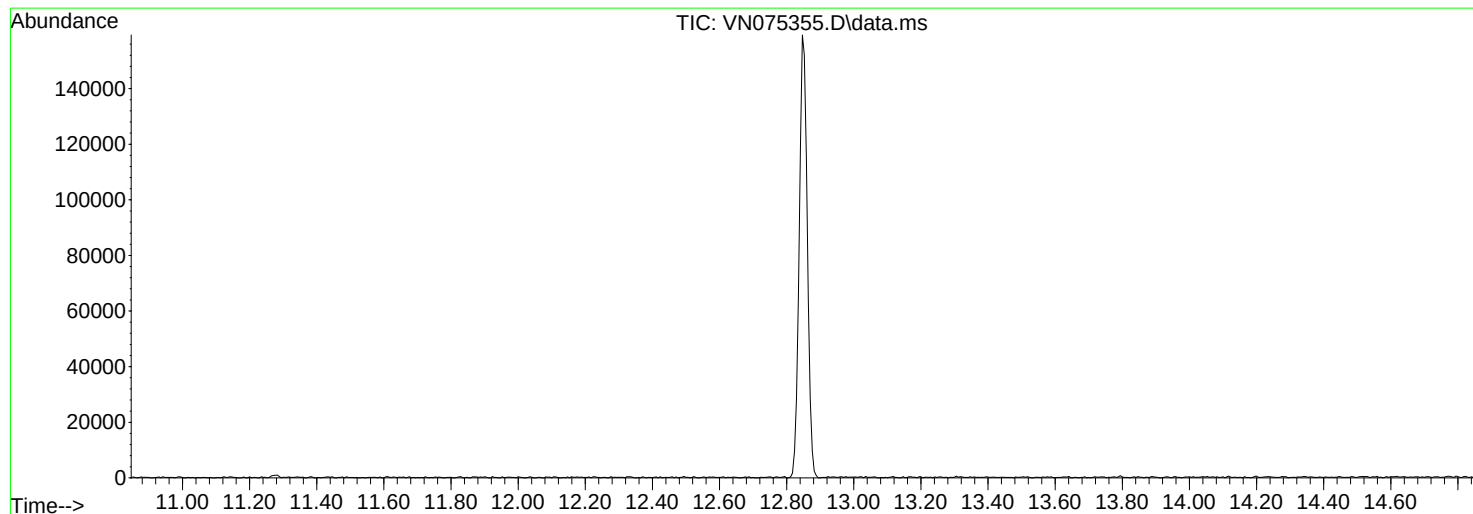

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	4958	PASS
75	95	30	60	52.4	15367	PASS
95	95	100	100	100.0	29336	PASS
96	95	5	9	7.7	2267	PASS
173	174	0.00	2	1.3	304	PASS
174	95	50	100	78.3	22960	PASS
175	174	5	9	7.5	1727	PASS
176	174	95	101	98.6	22640	PASS
177	176	5	9	7.3	1647	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	242	51.05	1513	69.95	317	81.85	261
37.05	1275	54.85	114	71.95	198	86.90	119
38.05	1296	56.05	411	73.00	1157	87.95	130
39.00	434	57.00	941	74.05	5532	90.90	15
39.90	169	59.95	242	75.05	15367	91.95	926
44.00	385	61.00	1499	76.05	1315	93.00	1303
44.95	294	62.05	1593	76.95	162	94.05	4063
46.95	299	63.00	1236	78.00	73	95.05	29336
48.00	56	63.95	175	78.90	1277	96.05	2267
48.95	1210	68.05	3284	79.95	357	103.80	69
50.05	4958	69.00	3389	80.90	1353	116.90	92

Average of 12.841 to 12.853 min.: VN075355.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.90	161						
118.85	190						
140.80	53						
140.95	281						
142.95	471						
172.00	184						
172.95	304						
174.00	22960						
175.00	1727						
176.00	22640						
177.00	1647						

Instrument :

MSVOA_N

ClientSampleId :

BFB