
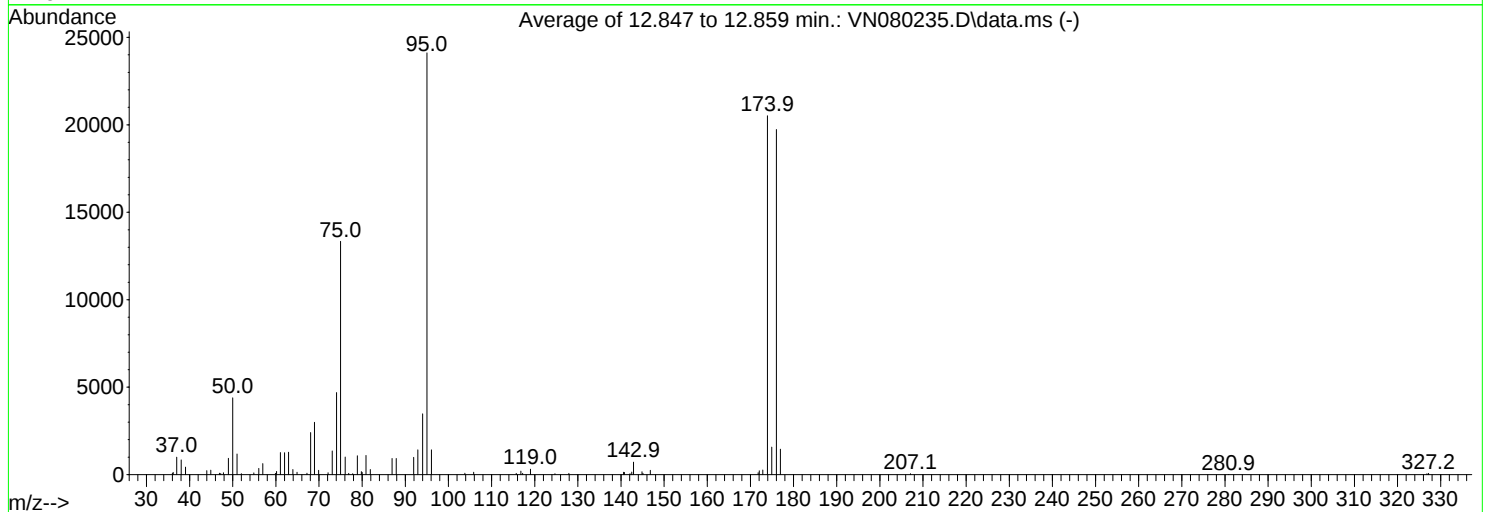


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112223\
Data File : VN080235.D
Acq On : 22 Nov 2023 09:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

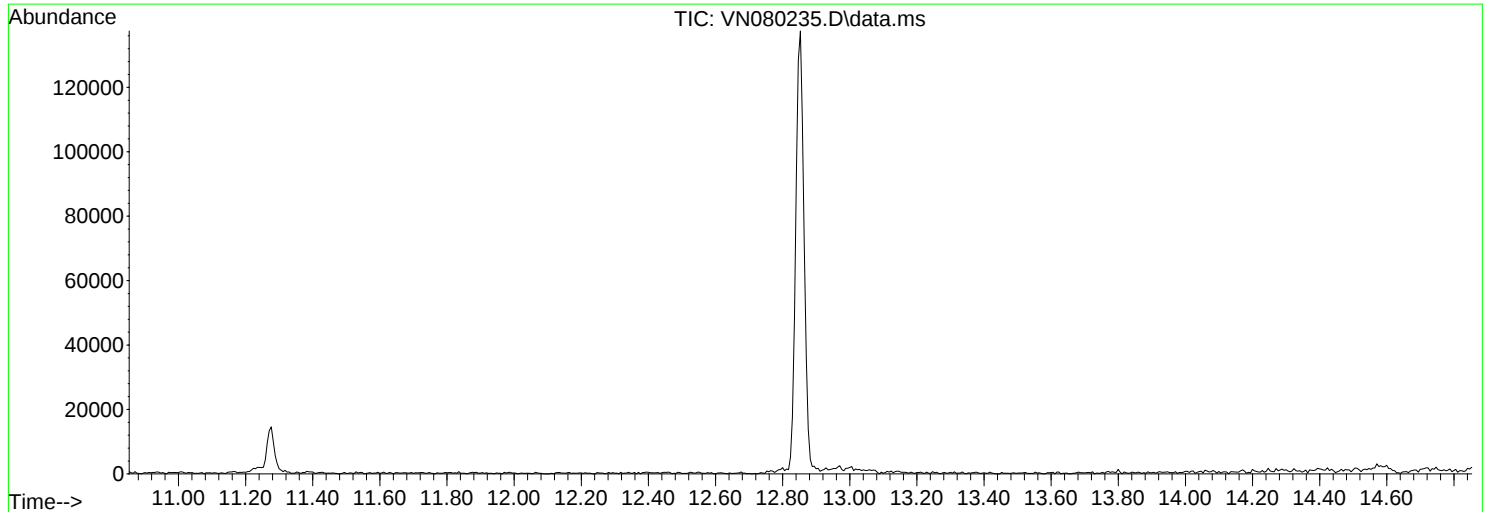

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	4394	PASS
75	95	30	60	55.3	13335	PASS
95	95	100	100	100.0	24115	PASS
96	95	5	9	5.9	1417	PASS
173	174	0.00	2	1.3	262	PASS
174	95	50	100	85.1	20523	PASS
175	174	5	9	7.7	1578	PASS
176	174	95	101	96.2	19733	PASS
177	176	5	9	7.4	1453	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	87	50.00	4394	63.95	295	76.90	7
36.20	131	51.00	1184	64.90	138	77.80	5
37.00	993	52.00	53	67.20	80	78.90	108
38.05	838	54.90	104	68.05	2407	79.80	17
39.05	427	56.05	360	68.95	2996	80.00	124
44.00	231	56.95	631	69.90	243	80.90	1094
44.90	254	59.90	78	72.10	109	81.90	296
46.90	82	60.15	186	73.05	1352	86.95	926
47.20	62	61.05	1263	74.05	4690	87.90	928
47.85	109	62.00	1252	75.00	13335	91.95	988
49.00	929	62.95	1278	76.05	1009	92.90	1416

Average of 12.847 to 12.859 min.: VN080235.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	3480	140.60	139	173.95	20523		
95.00	24115	140.80	124	174.95	1578		
96.05	1417	142.10	54	176.00	19733		
103.80	81	142.50	143	176.95	1453		
105.85	137	142.90	710	207.10	59		
115.70	72	144.85	164	280.85	7		
116.80	206	145.10	71	326.80	51		
117.20	74	146.80	248	327.20	71		
119.00	314	171.80	107				
124.70	52	172.05	217				
127.90	73	172.85	262				

Instrument :

MSVOA_N

ClientSampleId :

BFB