
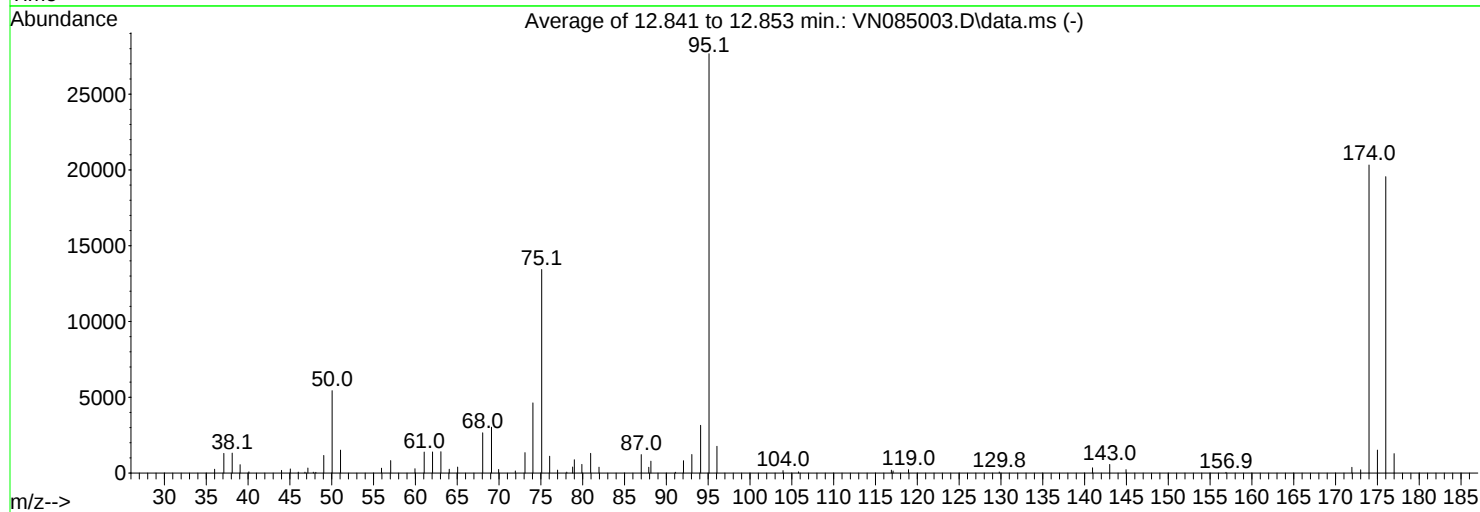


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112224\
Data File : VN085003.D
Acq On : 22 Nov 2024 09:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

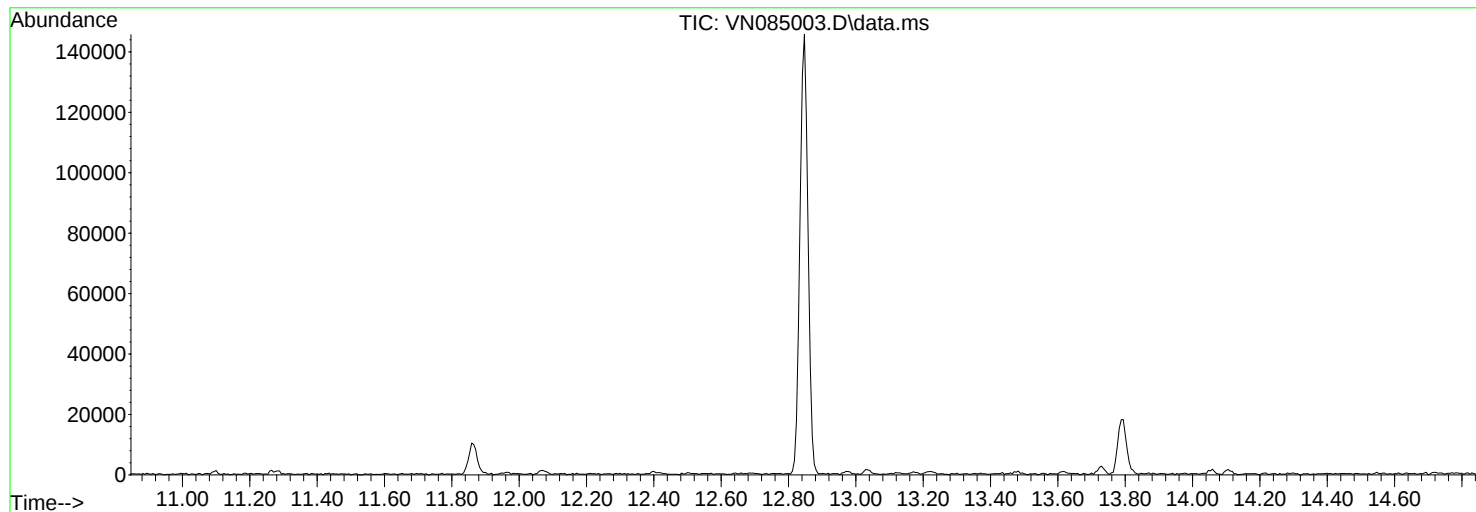

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	5439	PASS
75	95	30	60	48.5	13431	PASS
95	95	100	100	100.0	27667	PASS
96	95	5	9	6.4	1766	PASS
173	174	0.00	2	1.1	216	PASS
174	95	50	100	73.5	20325	PASS
175	174	5	9	7.5	1518	PASS
176	174	95	101	96.2	19555	PASS
177	176	5	9	6.6	1282	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	254	48.10	51	65.05	396	78.80	399
37.10	1298	49.05	1163	68.05	2657	79.00	882
38.10	1317	50.05	5439	69.10	3028	79.90	572
39.05	554	51.05	1513	69.95	237	80.95	1301
40.10	84	55.95	322	71.95	141	81.95	389
44.00	176	57.05	824	73.10	1348	87.00	1219
45.05	272	59.95	289	74.05	4631	87.90	383
46.00	62	61.05	1386	75.10	13431	88.15	786
46.80	61	62.05	1393	76.05	1113	91.10	54
47.15	333	63.05	1409	77.00	195	92.05	818
47.80	59	64.05	255	78.10	63	93.05	1225

Average of 12.841 to 12.853 min.: VN085003.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.10	3150	144.95	229				
95.10	27667	156.90	50				
96.05	1766	171.95	381				
103.95	166	173.00	216				
105.80	83	174.00	20325				
116.90	194	175.00	1518				
117.10	139	176.00	19555				
118.95	227	177.00	1282				
129.80	74						
140.95	348						
143.00	571						

Instrument :

MSVOA_N

ClientSampleId :

BFB