


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN112320\  
Data File : VN064774.D  
Acq On : 23 Nov 2020 8:52  
Operator : JC/MD  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N112320W.M  
Title : SW846 8260  
Last Update : Mon Nov 23 13:54:12 2020

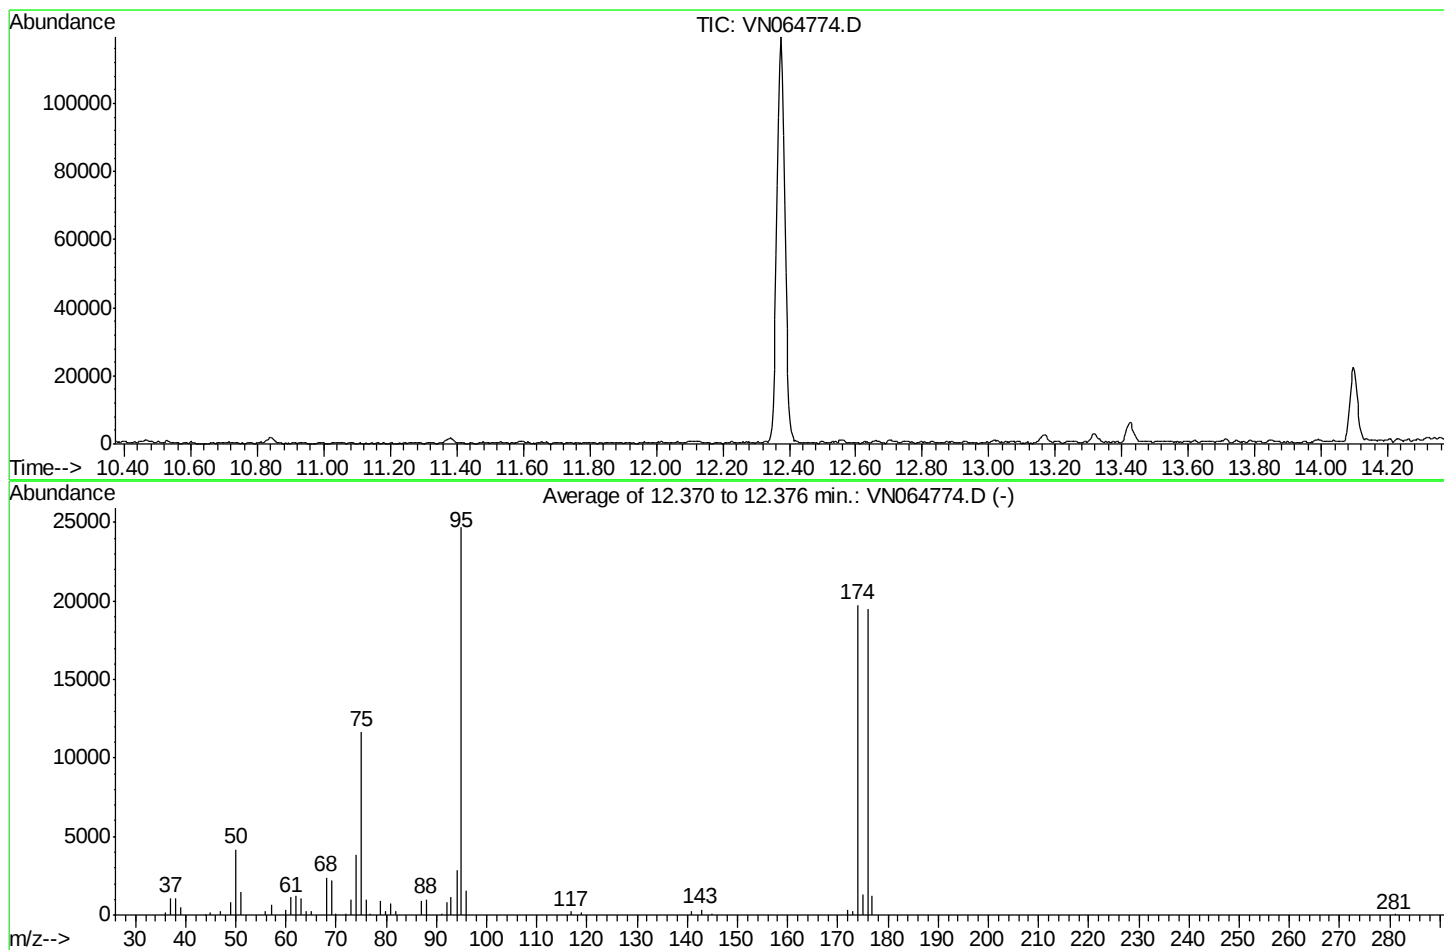

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.9      | 4178    | PASS             |
| 75          | 95           | 30           | 60           | 47.4      | 11702   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 24696   | PASS             |
| 96          | 95           | 5            | 9            | 6.3       | 1564    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.4       | 277     | PASS             |
| 174         | 95           | 50           | 100          | 80.0      | 19757   | PASS             |
| 175         | 174          | 5            | 9            | 6.8       | 1337    | PASS             |
| 176         | 174          | 95           | 101          | 98.8      | 19525   | PASS             |
| 177         | 176          | 5            | 9            | 6.1       | 1195    | PASS             |