
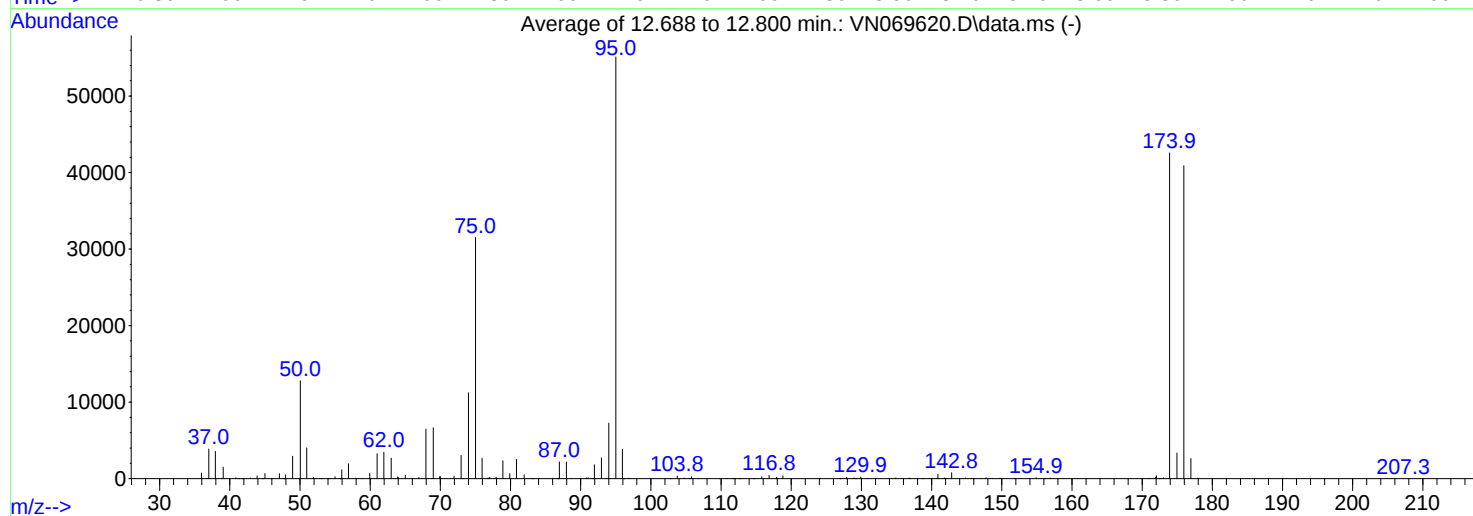


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112321\
 Data File : VN069620.D
 Acq On : 23 Nov 2021 10:24
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N111021W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Nov 10 14:36:17 2021

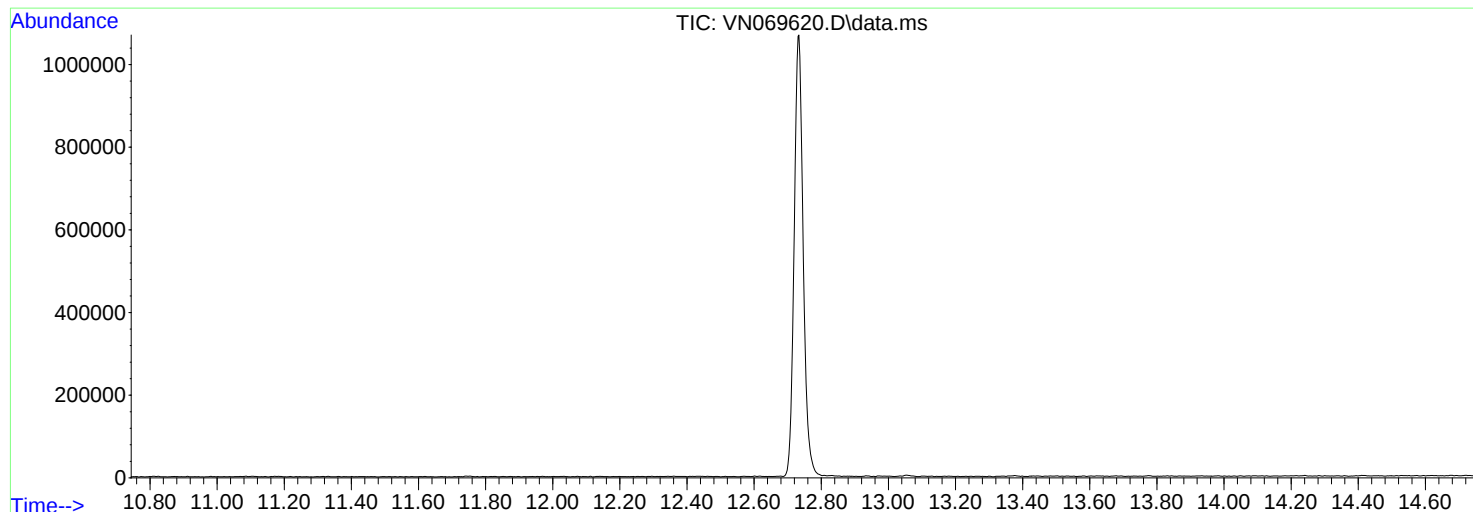

AutoFind: Averaged scan 3989 to 4031; Bkg corrected with scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	12803	PASS
75	95	30	60	57.2	31523	PASS
95	95	100	100	100.0	55128	PASS
96	95	5	9	6.9	3820	PASS
173	174	0.00	2	0.2	101	PASS
174	95	50	100	77.2	42582	PASS
175	174	5	9	7.9	3343	PASS
176	174	95	101	96.1	40901	PASS
177	176	5	9	6.4	2627	PASS