

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112322\
 Data File : VN075397.D
 Acq On : 23 Nov 2022 15:35
 Operator : JC\MD
 Sample : PB149245TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB149245TB

Quant Time: Nov 24 06:52:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	176906	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	296795	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	277007	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	125924	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	45795	48.225	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	96.460%		
35) Dibromofluoromethane	8.171	113	56334	48.318	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.640%		
50) Toluene-d8	10.571	98	132516	50.464	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	100.920%		
62) 4-Bromofluorobenzene	12.847	95	95608	49.327	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.660%		
Target Compounds						
					Qvalue	
5) Bromomethane	2.942	94	407	0.218	ug/l #	62
8) Diethyl Ether	3.965	74	4301	4.049	ug/l	94
11) Tert butyl alcohol	5.518	59	3027	7.593	ug/l #	72
16) Acetone	4.442	43	83468	94.234	ug/l	97
18) Methyl Acetate	5.042	43	1450	Below Cal	#	71
20) Methylene Chloride	5.289	84	23596	12.169	ug/l	91
25) 2-Butanone	7.500	43	3753	3.035	ug/l	91
29) Tetrahydrofuran	7.859	42	286	0.380	ug/l #	41
31) Cyclohexane	8.230	56	3285	1.089	ug/l #	1
36) 1,1-Dichloropropene	8.224	75	12629	4.967	ug/l #	50
37) Ethyl Acetate	7.577	43	24161	10.553	ug/l	99
38) Carbon Tetrachloride	8.230	117	16793	6.012	ug/l #	16
42) 1,2-Dichloroethane	8.688	62	661	0.254	ug/l #	75
43) Isopropyl Acetate	8.694	43	109717	29.857	ug/l	92
45) 1,2-Dichloropropane	9.747	63	1357	0.731	ug/l #	42
48) Methyl methacrylate	9.671	41	3198	1.882	ug/l #	34
49) 1,4-Dioxane	9.741	88	61	1.264	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	10009	4.276	ug/l #	73
53) t-1,3-Dichloropropene	10.724	75	766	0.281	ug/l #	70
54) cis-1,3-Dichloropropene	10.359	75	47799	16.133	ug/l #	60
57) 1,3-Dichloropropane	11.206	76	6544	1.964	ug/l #	42
59) 2-Hexanone	11.171	43	91414	52.013	ug/l #	21
74) N-amyl acetate	12.482	43	2047	0.724	ug/l #	47
76) 1,2,3-Trichloropropane	12.847	75	47393	19.906	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	47393	58.896	ug/l #	10
88) 1,4-Dichlorobenzene	13.817	146	1335	0.305	ug/l #	49
89) n-Butylbenzene	14.059	91	1721	0.256	ug/l #	66
91) 1,2-Dichlorobenzene	14.106	146	930	0.222	ug/l	81
93) 1,2,4-Trichlorobenzene	15.394	180	1169	0.544	ug/l	96
95) Naphthalene	15.641	128	7548	1.116	ug/l #	92
96) 1,2,3-Trichlorobenzene	15.835	180	1048	0.496	ug/l	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 24 06:52:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration







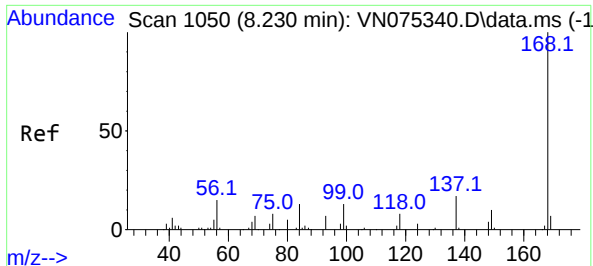

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion:168 Resp: 176906
Ion Ratio Lower Upper
168 100
99 52.8 51.6 77.4

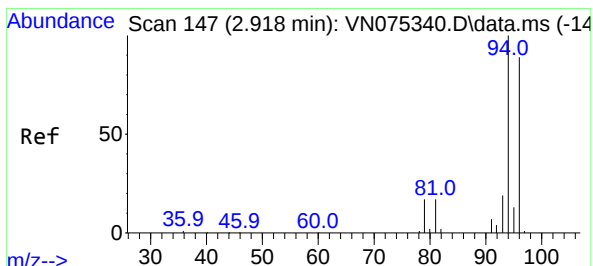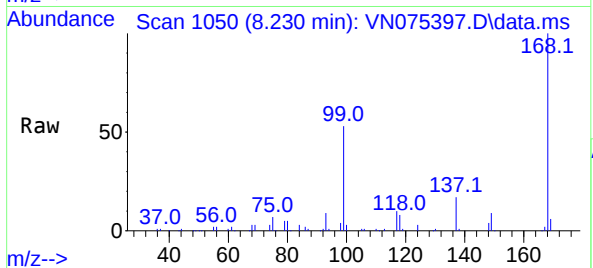

#5
Bromomethane
Concen: 0.218 ug/l
RT: 2.942 min Scan# 151
Delta R.T. 0.024 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 94 Resp: 407
Ion Ratio Lower Upper
94 100
96 53.9 71.8 107.6#


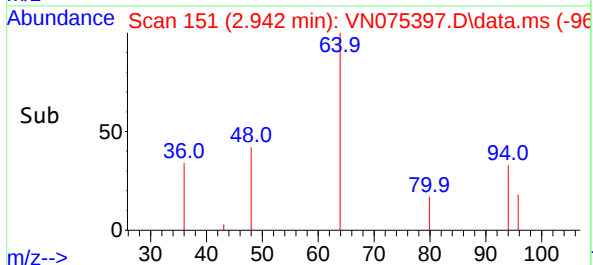
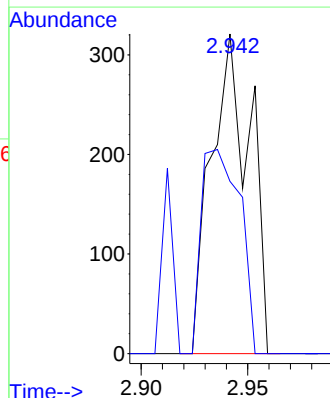
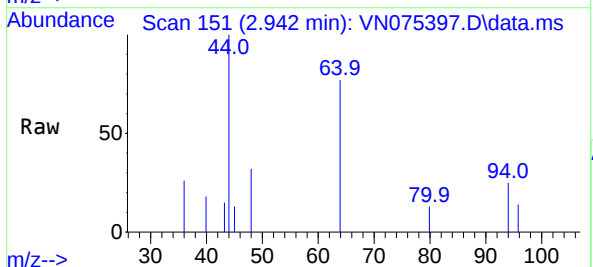




#8
Diethyl Ether
Concen: 4.049 ug/l
RT: 3.965 min Scan# 31
Delta R.T. 0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 74 Resp: 4301
Ion Ratio Lower Upper
74 100
45 83.6 39.3 117.9



#11
Tert butyl alcohol
Concen: 7.593 ug/l
RT: 5.518 min Scan# 589
Delta R.T. -0.024 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 59 Resp: 3027
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#


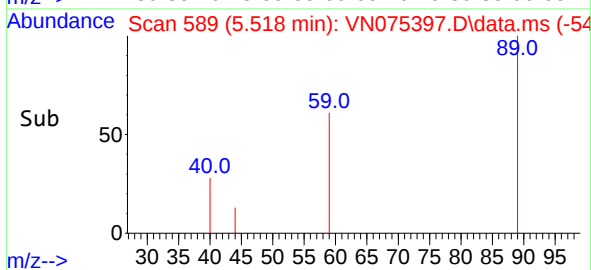






#16
Acetone
Concen: 94.234 ug/l
RT: 4.442 min Scan# 405
Delta R.T. 0.006 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 43 Resp: 83468
Ion Ratio Lower Upper
43 100
58 33.4 25.5 38.3

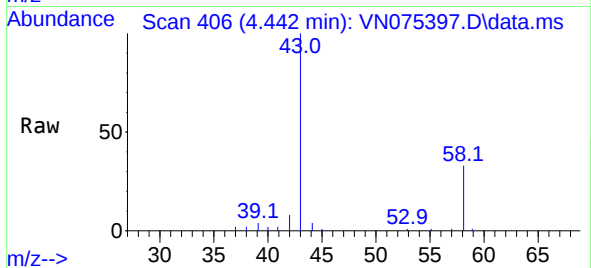

#18
Methyl Acetate
Concen: Below Cal
RT: 5.042 min Scan# 508
Delta R.T. 0.006 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 43 Resp: 1450
Ion Ratio Lower Upper
43 100
74 42.9 22.0 33.0#


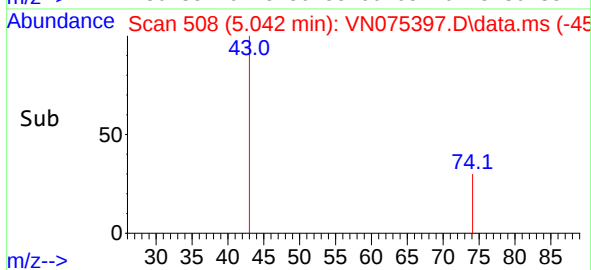






#20
Methylene Chloride
Concen: 12.169 ug/l
RT: 5.289 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion:	84	Resp:	23596
Ion	Ratio	Lower	Upper
84	100		
49	106.6	94.9	142.3
51	30.6	26.8	40.2
86	73.8	53.7	80.5

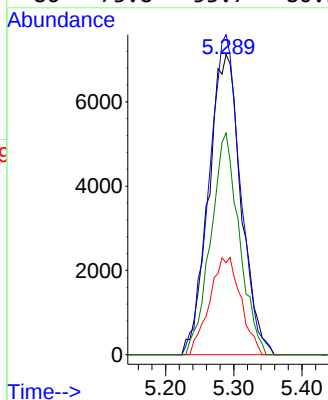

#25
2-Butanone
Concen: 3.035 ug/l
RT: 7.500 min Scan# 926
Delta R.T. 0.011 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion:	43	Resp:	3753
Ion	Ratio	Lower	Upper
43	100		
72	27.1	25.5	38.3


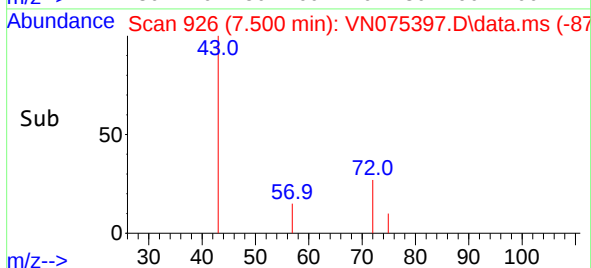
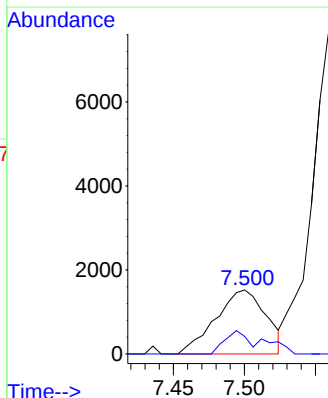



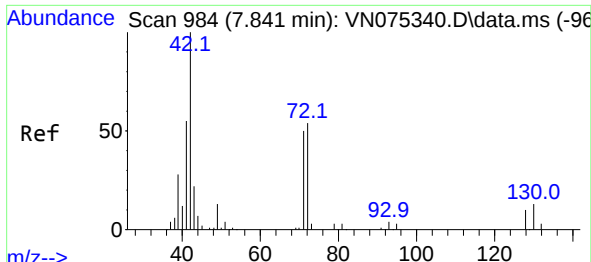

#29
Tetrahydrofuran
Concen: 0.380 ug/l
RT: 7.859 min Scan# 91
Delta R.T. 0.018 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 42 Resp: 286
Ion Ratio Lower Upper
42 100
72 20.3 43.0 64.6#
71 0.0 39.9 59.9#

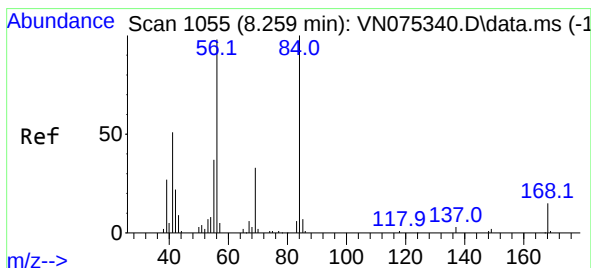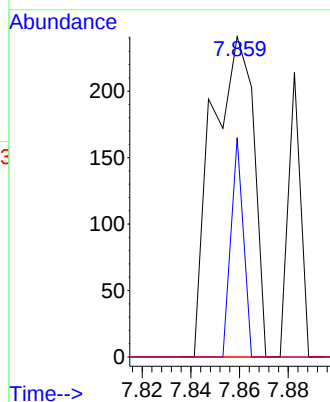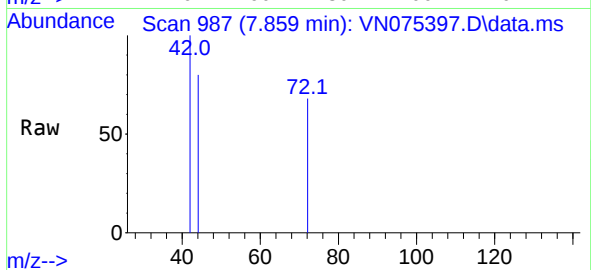

#31
Cyclohexane
Concen: 1.089 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.029 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 56 Resp: 3285
Ion Ratio Lower Upper
56 100
69 171.8 25.2 37.8#
84 154.6 77.8 116.8#


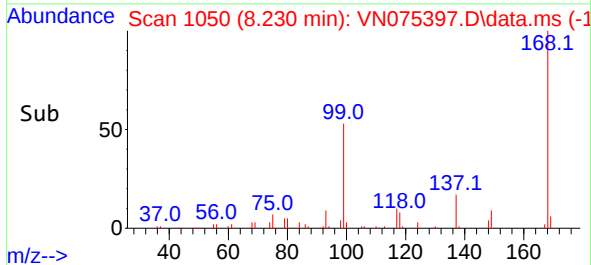
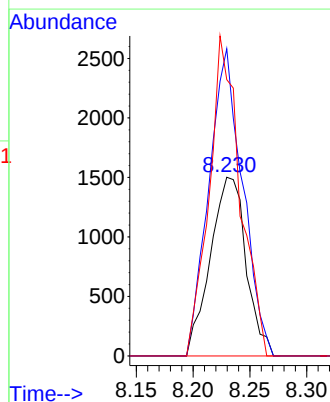
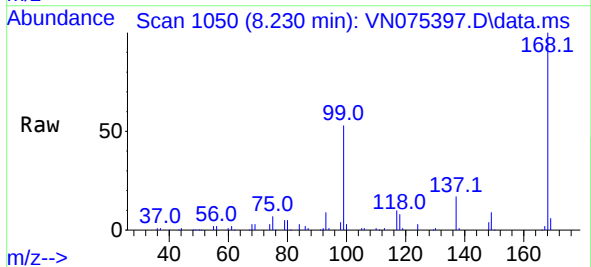


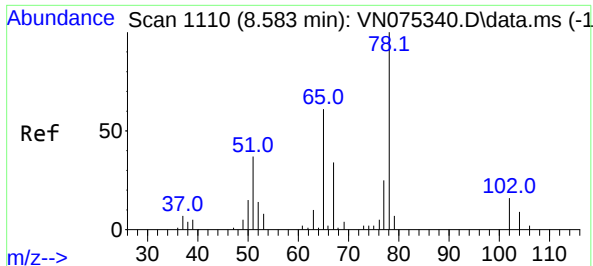

#33
1,2-Dichloroethane-d4
Concen: 48.225 ug/l
RT: 8.582 min Scan# 1110
Delta R.T. -0.001 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 65 Resp: 45795
Ion Ratio Lower Upper
65 100
67 51.3 0.0 102.0

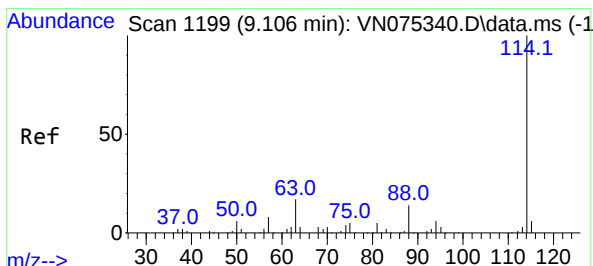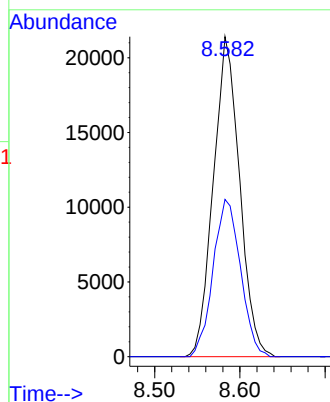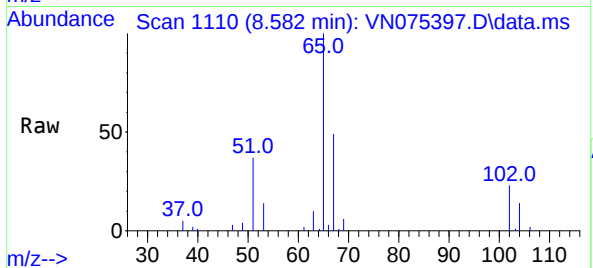

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. 0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion:114 Resp: 296795
Ion Ratio Lower Upper
114 100
63 17.9 0.0 39.6
88 15.1 0.0 29.0


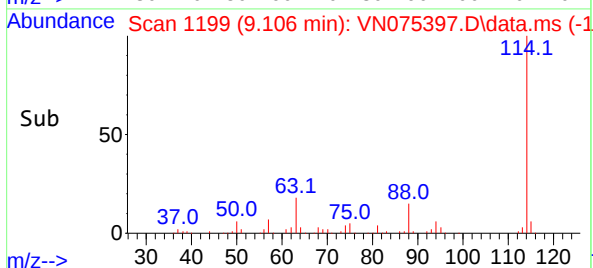






#35
Dibromofluoromethane
Concen: 48.318 ug/l
RT: 8.171 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion:113 Resp: 56334
Ion Ratio Lower Upper
113 100
111 107.3 80.5 120.7
192 20.7 13.2 19.8#

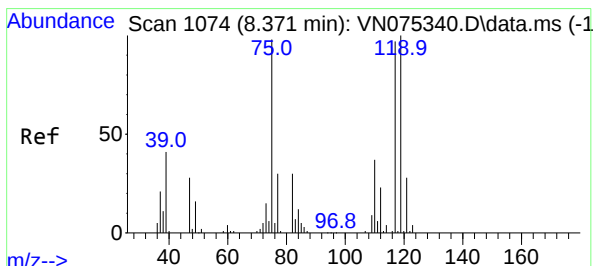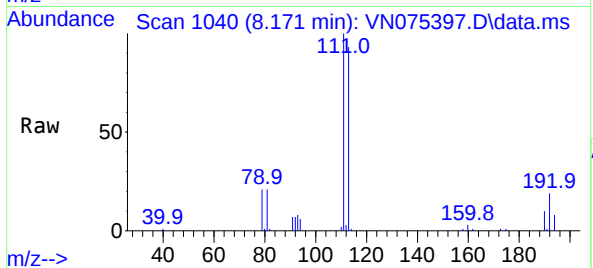

#36
1,1-Dichloropropene
Concen: 4.967 ug/l
RT: 8.224 min Scan# 1049
Delta R.T. -0.147 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 75 Resp: 12629
Ion Ratio Lower Upper
75 100
110 9.3 17.8 53.3#
77 0.0 24.6 37.0#


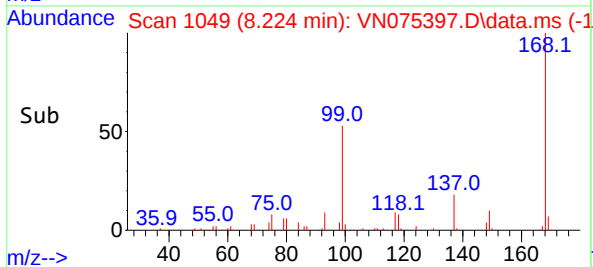

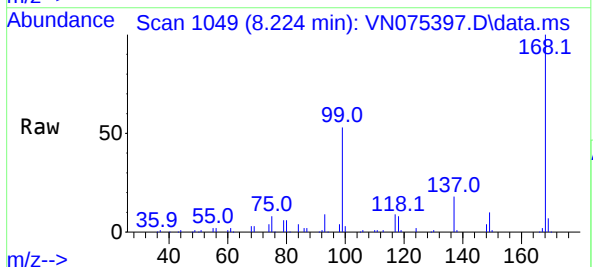




#37
Ethyl Acetate
Concen: 10.553 ug/l
RT: 7.577 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 43 Resp: 24161
Ion Ratio Lower Upper
43 100
61 14.9 12.2 18.4
70 12.6 9.4 14.2



#38
Carbon Tetrachloride
Concen: 6.012 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.135 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 117 Resp: 16793
Ion Ratio Lower Upper
117 100
119 5.2 76.7 115.1#
121 0.0 23.9 35.9#


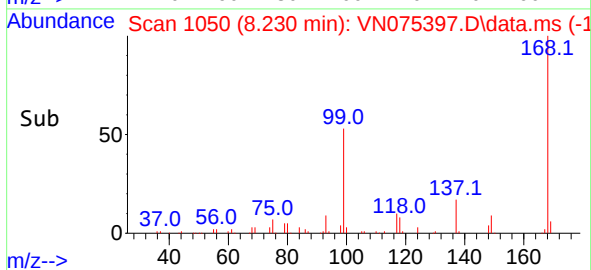




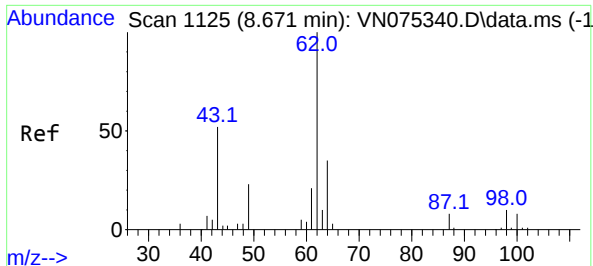

#42
1,2-Dichloroethane
Concen: 0.254 ug/l
RT: 8.688 min Scan# 1128
Delta R.T. 0.017 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 62 Resp: 661
Ion Ratio Lower Upper
62 100
98 0.0 0.0 18.2

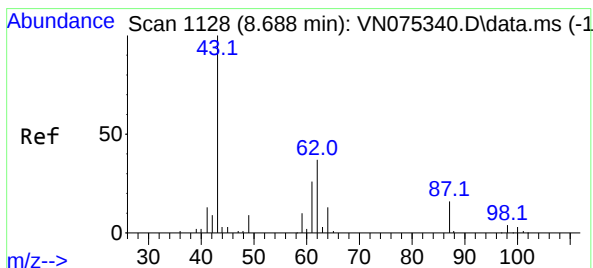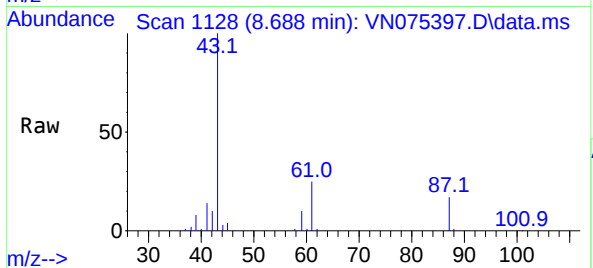

#43
Isopropyl Acetate
Concen: 29.857 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. 0.006 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 43 Resp: 109717
Ion Ratio Lower Upper
43 100
61 22.8 22.4 33.6
87 17.2 12.5 18.7


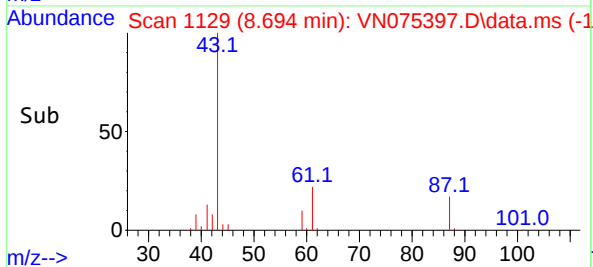

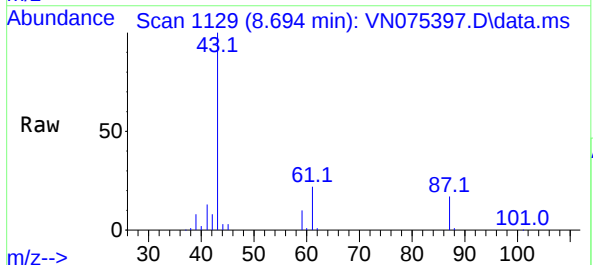




#45
1,2-Dichloropropane
Concen: 0.731 ug/l
RT: 9.747 min Scan# 11
Delta R.T. 0.123 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 63 Resp: 1357
Ion Ratio Lower Upper
63 100
65 0.0 26.1 39.1#

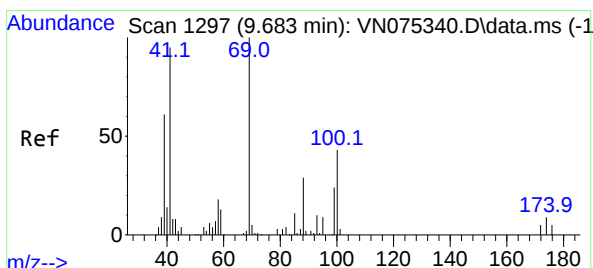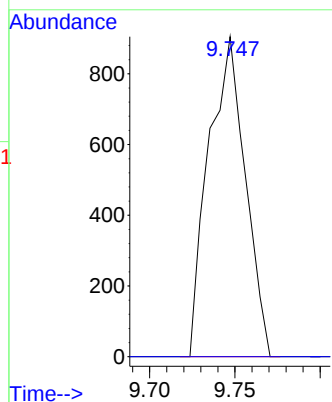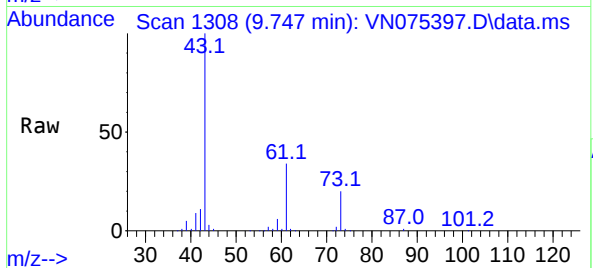

#48
Methyl methacrylate
Concen: 1.882 ug/l
RT: 9.671 min Scan# 1295
Delta R.T. -0.012 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 41 Resp: 3198
Ion Ratio Lower Upper
41 100
69 0.0 80.2 120.2#
39 55.3 56.2 84.2#


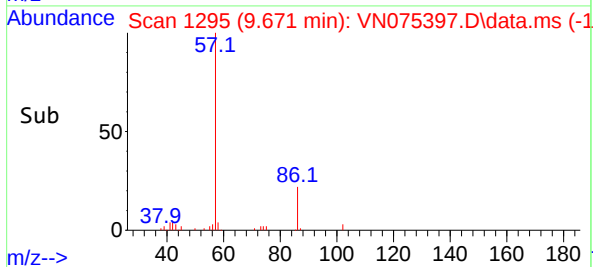
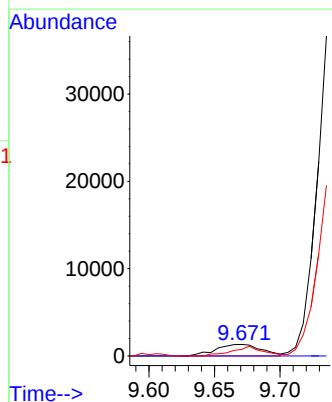
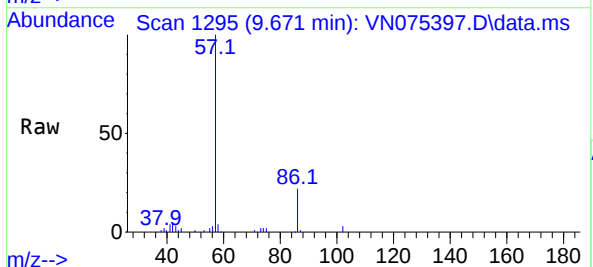




#49
1,4-Dioxane
Concen: 1.264 ug/l
RT: 9.741 min Scan# 11
Delta R.T. 0.041 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 88 Resp: 61
Ion Ratio Lower Upper
88 100
43 1594783.6 17.5 26.3#
58 7375.4 49.8 74.8#

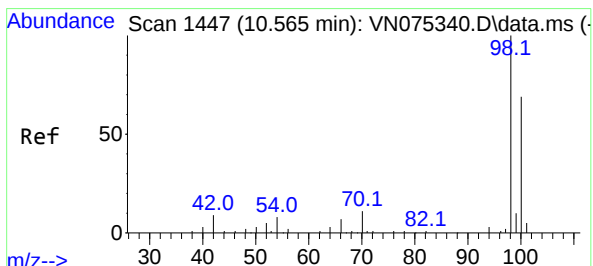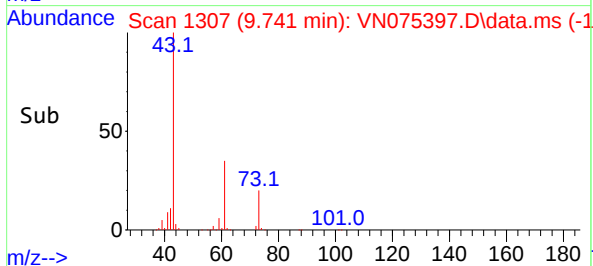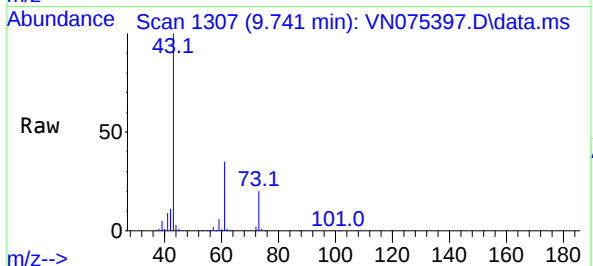

#50
Toluene-d8
Concen: 50.464 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. 0.006 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 98 Resp: 132516
Ion Ratio Lower Upper
98 100
100 65.3 53.0 79.6


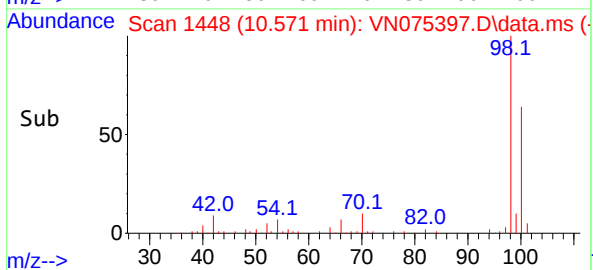






#51
4-Methyl-2-Pentanone
Concen: 4.276 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. 0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 43 Resp: 10009
Ion Ratio Lower Upper
43 100
58 25.0 33.6 50.4#

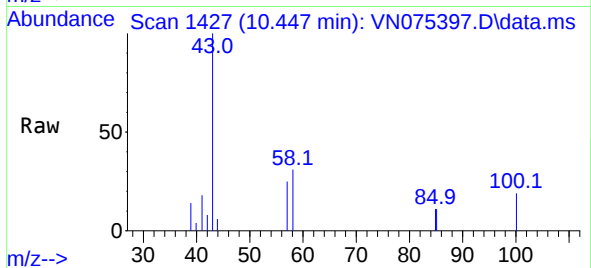

#53
t-1,3-Dichloropropene
Concen: 0.281 ug/l
RT: 10.724 min Scan# 1474
Delta R.T. -0.111 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 75 Resp: 766
Ion Ratio Lower Upper
75 100
77 48.2 25.4 38.2#


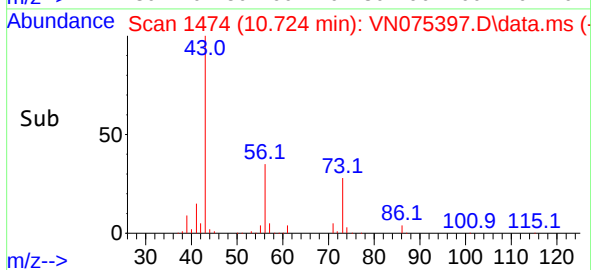






#54
cis-1,3-Dichloropropene
Concen: 16.133 ug/l
RT: 10.359 min Scan# 14
Delta R.T. 0.047 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 75 Resp: 47799
Ion Ratio Lower Upper
75 100
77 0.6 23.7 35.5#
39 24.7 35.8 53.6#



#57
1,3-Dichloropropane
Concen: 1.964 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.041 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 76 Resp: 6544
Ion Ratio Lower Upper
76 100
78 0.0 25.8 38.6#


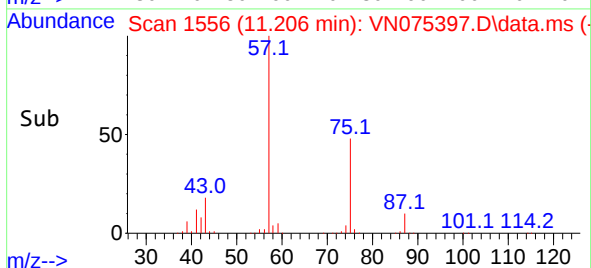
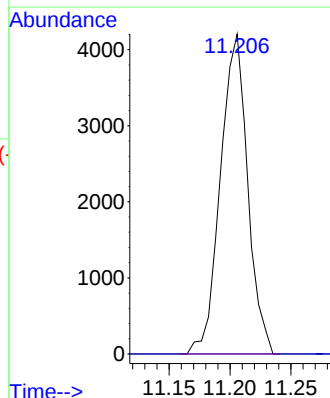





#59
2-Hexanone
Concen: 52.013 ug/l
RT: 11.171 min Scan# 1150
Delta R.T. -0.023 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 43 Resp: 91414
Ion Ratio Lower Upper
43 100
58 0.0 29.6 88.8#

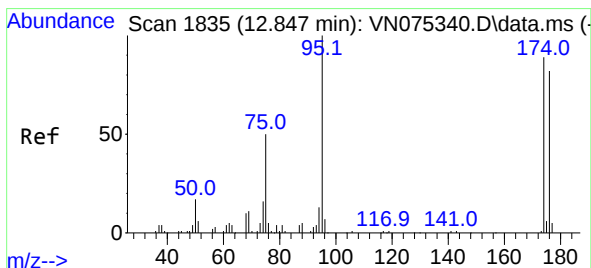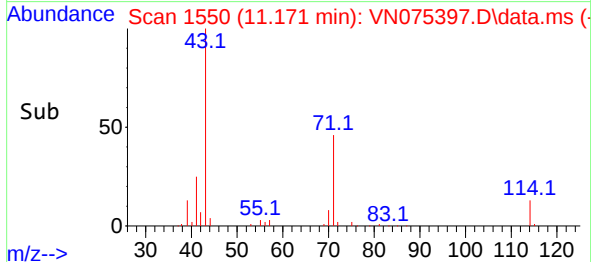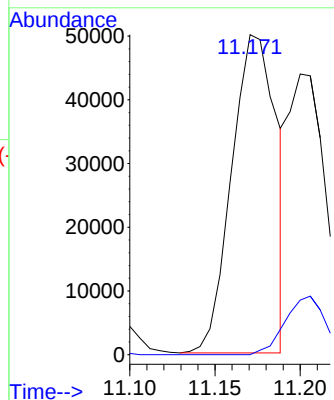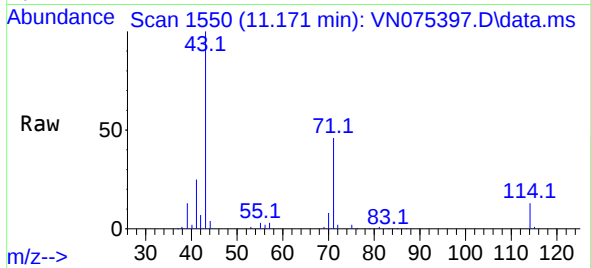

#62
4-Bromofluorobenzene
Concen: 49.327 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 95 Resp: 95608
Ion Ratio Lower Upper
95 100
174 86.3 0.0 147.4
176 83.2 0.0 142.2


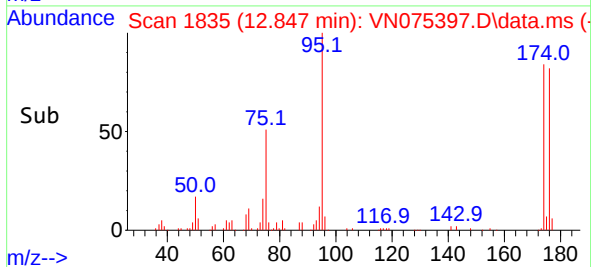
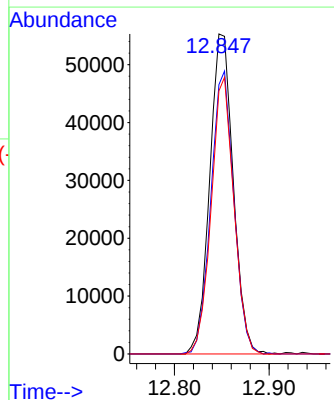
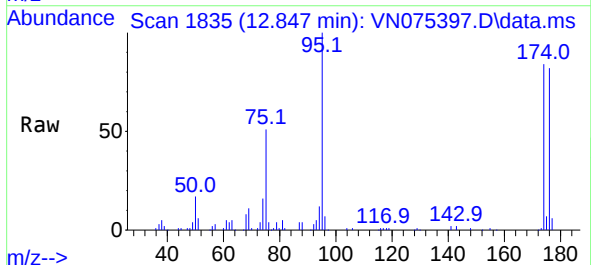




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion:117 Resp: 277007
Ion Ratio Lower Upper
117 100
82 51.1 43.1 64.7
119 30.9 25.5 38.3

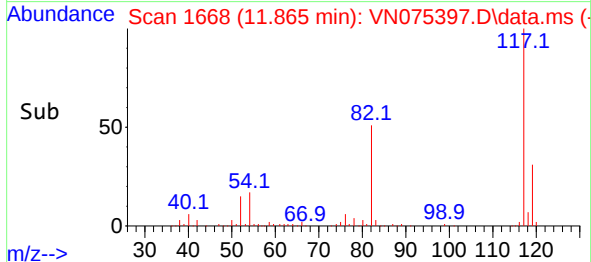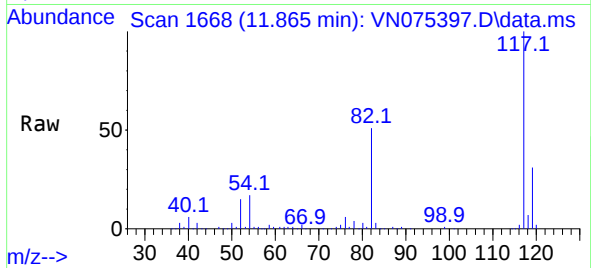

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion:152 Resp: 125924
Ion Ratio Lower Upper
152 100
115 58.1 30.2 90.6
150 157.2 0.0 348.4


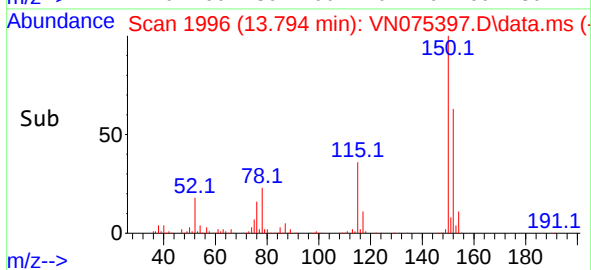






#74
N-amy1 acetate
Concen: 0.724 ug/l
RT: 12.482 min Scan# 11
Delta R.T. -0.012 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 43	Resp: 2047
Ion Ratio	Lower Upper
43	100
70	7.3 39.8 59.8#
55	7.1 19.9 29.9#
61	0.0 21.7 32.5#

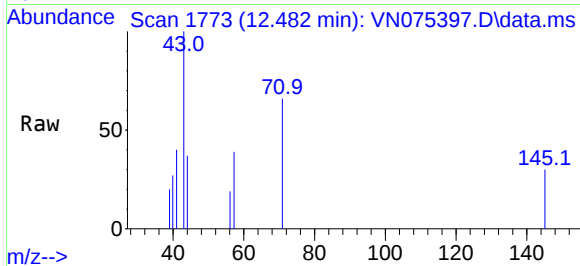

#76
1,2,3-Trichloropropane
Concen: 19.906 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.147 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion: 75	Resp: 47393
Ion Ratio	Lower Upper
75	100
77	1.4 75.6 226.8#


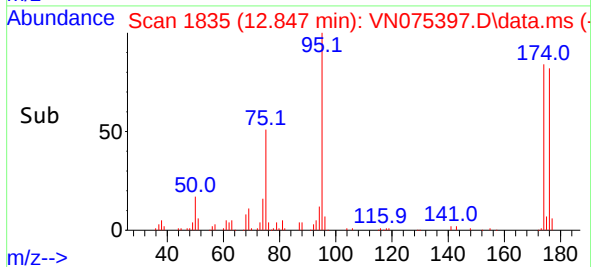

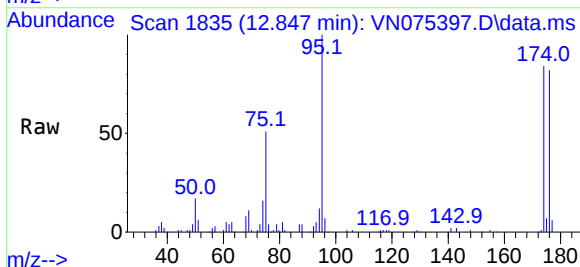




#81
trans-1,4-Dichloro-2-butene
Concen: 58.896 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.112 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 75 Resp: 47393
Ion Ratio Lower Upper
75 100
53 0.0 78.5 117.7#
89 0.0 37.7 56.5#

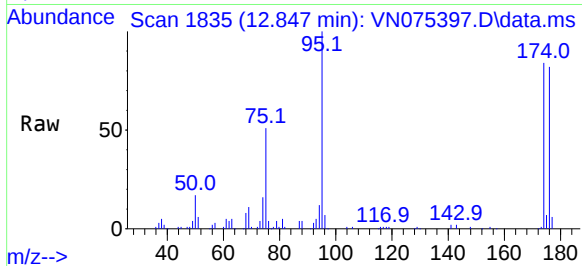

#88
1,4-Dichlorobenzene
Concen: 0.305 ug/l
RT: 13.817 min Scan# 2000
Delta R.T. 0.005 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion:146 Resp: 1335
Ion Ratio Lower Upper
146 100
111 0.0 20.1 60.3#
148 97.2 31.9 95.7#


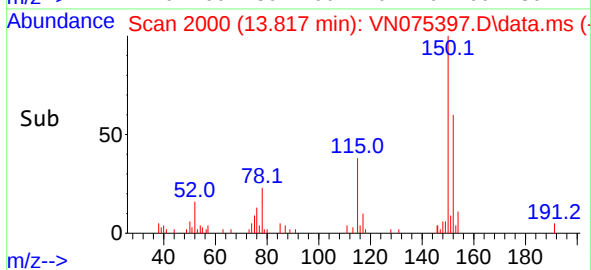

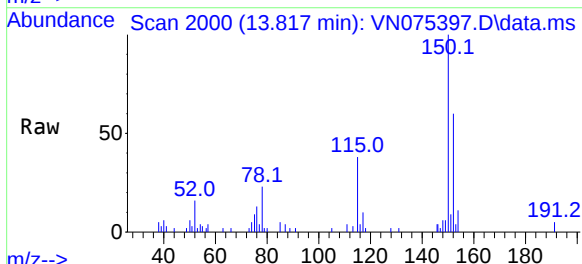




#89
n-Butylbenzene
Concen: 0.256 ug/l
RT: 14.059 min Scan# 2041
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion: 91 Resp: 1721
Ion Ratio Lower Upper
91 100
92 32.9 26.5 79.4
134 3.3 13.0 39.0#

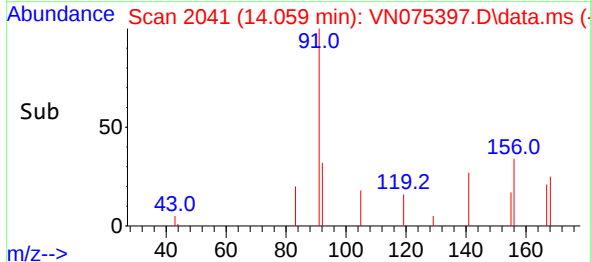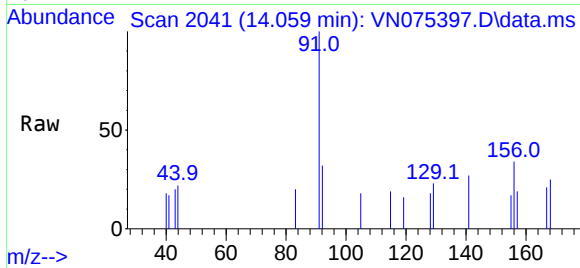

#91
1,2-Dichlorobenzene
Concen: 0.222 ug/l
RT: 14.106 min Scan# 2049
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion:146 Resp: 930
Ion Ratio Lower Upper
146 100
111 24.2 21.3 63.9
148 52.9 31.4 94.2


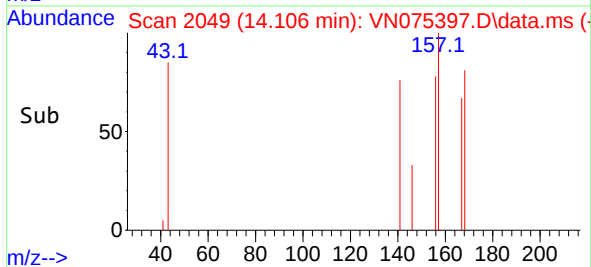

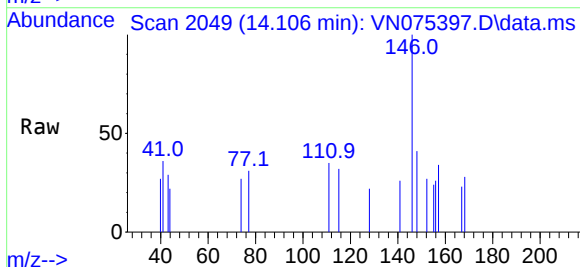




#93
1,2,4-Trichlorobenzene
Concen: 0.544 ug/l
RT: 15.394 min Scan# 211
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35




Instrument :
MSVOA_N
ClientSampleId :
PB149245TB


Tgt Ion:180 Resp: 1169
Ion Ratio Lower Upper
180 100
182 93.5 47.8 143.4
145 28.0 16.8 50.3



#95
Naphthalene
Concen: 1.116 ug/l
RT: 15.641 min Scan# 2310
Delta R.T. -0.000 min
Lab File: VN075397.D
Acq: 23 Nov 2022 15:35

Tgt Ion:128 Resp: 7548
Ion Ratio Lower Upper
128 100
127 15.0 10.4 15.6
129 15.2 8.6 12.8#

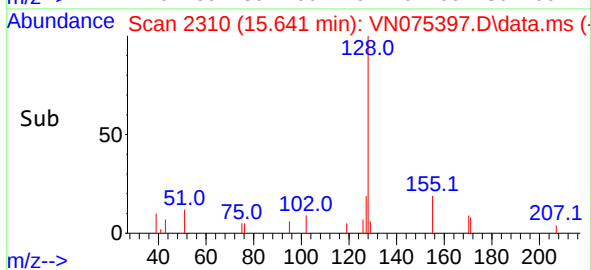



#96
 1,2,3-Trichlorobenzene
 Concen: 0.496 ug/l
 RT: 15.835 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN075397.D
 Acq: 23 Nov 2022 15:35

Instrument :
 MSVOA_N
 ClientSampleId :
 PB149245TB

Tgt Ion:	180	Resp:	1048
Ion	Ratio	Lower	Upper
180	100		
182	105.2	47.3	141.8
145	50.5	17.6	52.9

