
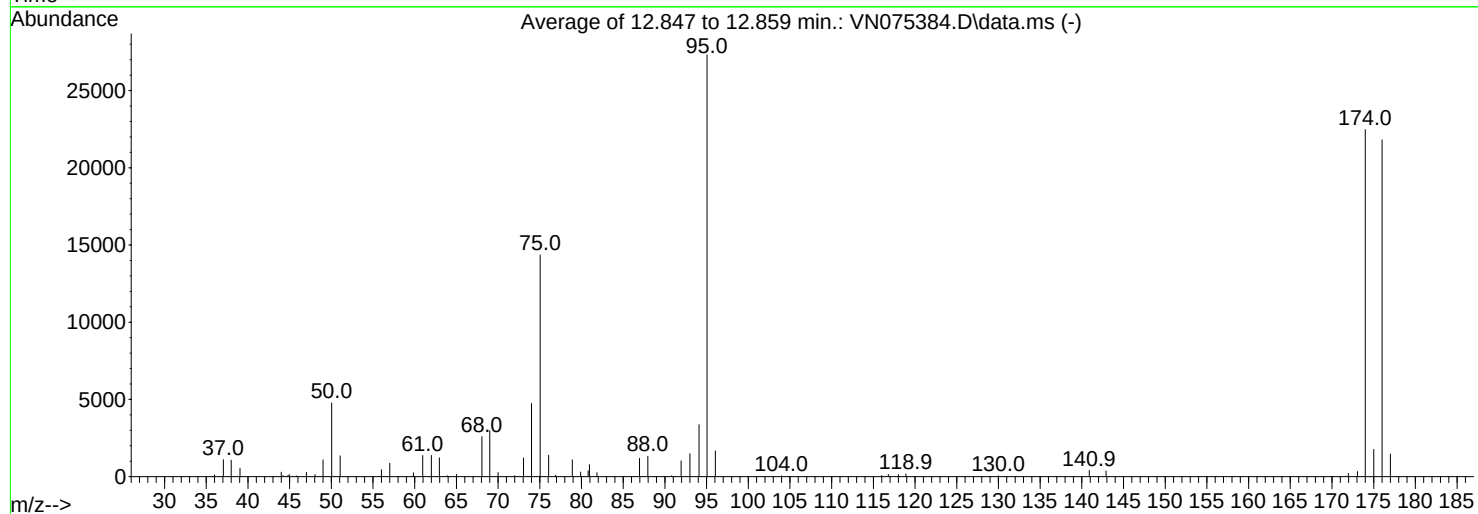


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112322\
Data File : VN075384.D
Acq On : 23 Nov 2022 09:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Title : SW846 8260
Last Update : Wed Nov 23 00:18:03 2022

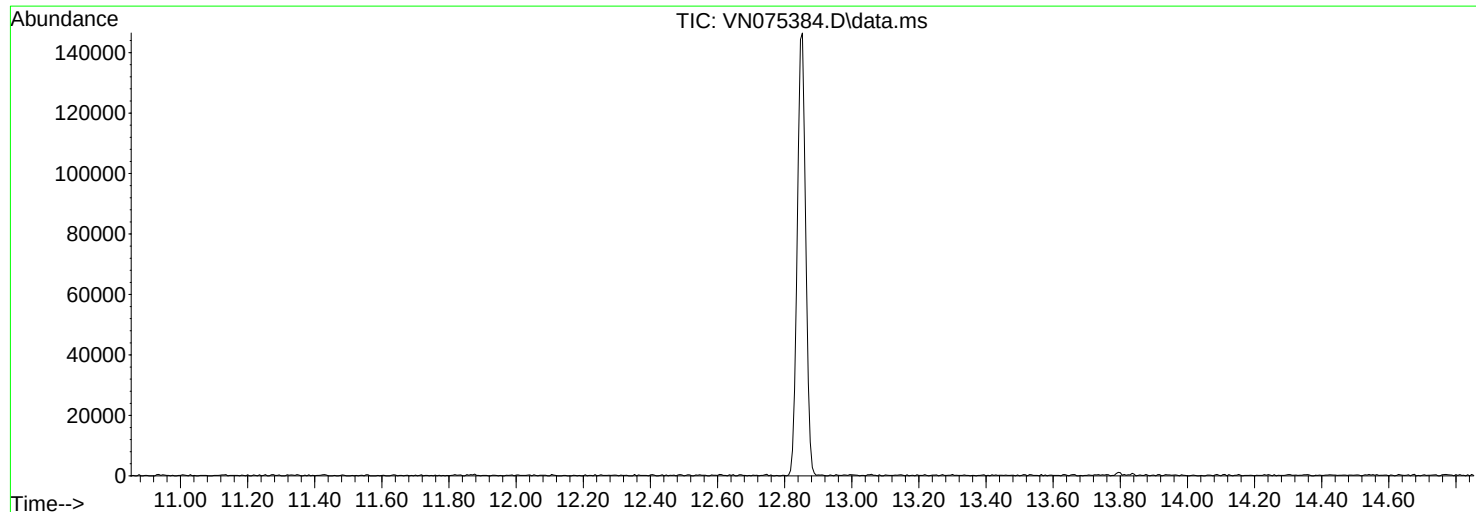

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4775	PASS
75	95	30	60	52.6	14362	PASS
95	95	100	100	100.0	27312	PASS
96	95	5	9	6.1	1665	PASS
173	174	0.00	2	1.5	332	PASS
174	95	50	100	82.3	22475	PASS
175	174	5	9	7.8	1760	PASS
176	174	95	101	97.0	21808	PASS
177	176	5	9	6.7	1460	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	118	49.00	1092	68.05	2594	80.80	371
37.05	1098	50.05	4775	69.00	2984	80.95	781
38.00	1067	51.05	1346	70.00	270	81.85	261
39.05	548	56.00	446	72.00	66	86.95	117
44.00	291	57.00	868	73.05	1213	87.95	1320
44.20	61	59.85	253	74.00	4738	90.80	51
44.80	86	60.95	1365	75.05	14362	91.95	1030
44.95	139	62.00	1381	76.05	1390	93.00	1478
45.80	54	62.95	1226	76.90	94	94.10	3369
47.00	281	63.90	67	78.90	1089	95.05	27312
48.05	132	65.00	150	79.90	297	96.05	1665

Average of 12.847 to 12.859 min.: VN075384.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
104.00	51	175.00	1760				
116.00	68	176.00	21808				
116.80	142	177.00	1460				
118.00	131						
118.90	180						
130.00	54						
140.90	403						
142.90	367						
171.95	203						
173.05	332						
174.00	22475						

Instrument :

MSVOA_N

ClientSampleId :

BFB