

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN112420\
 Data File : VN064833.D
 Acq On : 25 Nov 2020 1:06
 Operator : JC/MD
 Sample : L4798-06 20X
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 45BR-20201118

Quant Time: Nov 25 15:34:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 23 13:54:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	166876	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	293929	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	302373	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	136015	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	7.99	65	102527	52.85	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	105.70%
35) Dibromofluoromethane	7.55	113	94143	53.53	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	107.06%
50) Toluene-d8	10.06	98	366350	50.98	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	101.96%
62) 4-Bromofluorobenzene	12.37	95	141485	55.01	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	110.02%

Target Compounds


					Qvalue
4) Vinyl Chloride	2.17	62	5359	2.735	ug/l 96
27) cis-1,2-Dichloroethene	6.78	96	163537	80.875	ug/l 89
44) Trichloroethene	8.80	130	462848	187.900	ug/l 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN112420\
Data File : VN064833.D
Acq On : 25 Nov 2020 1:06
Operator : JC/MD
Sample : L4798-06 20X
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
45BR-20201118

Quant Time: Nov 25 15:34:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Quant Title : SW846 8260
QLast Update : Mon Nov 23 13:54:12 2020
Response via : Initial Calibration

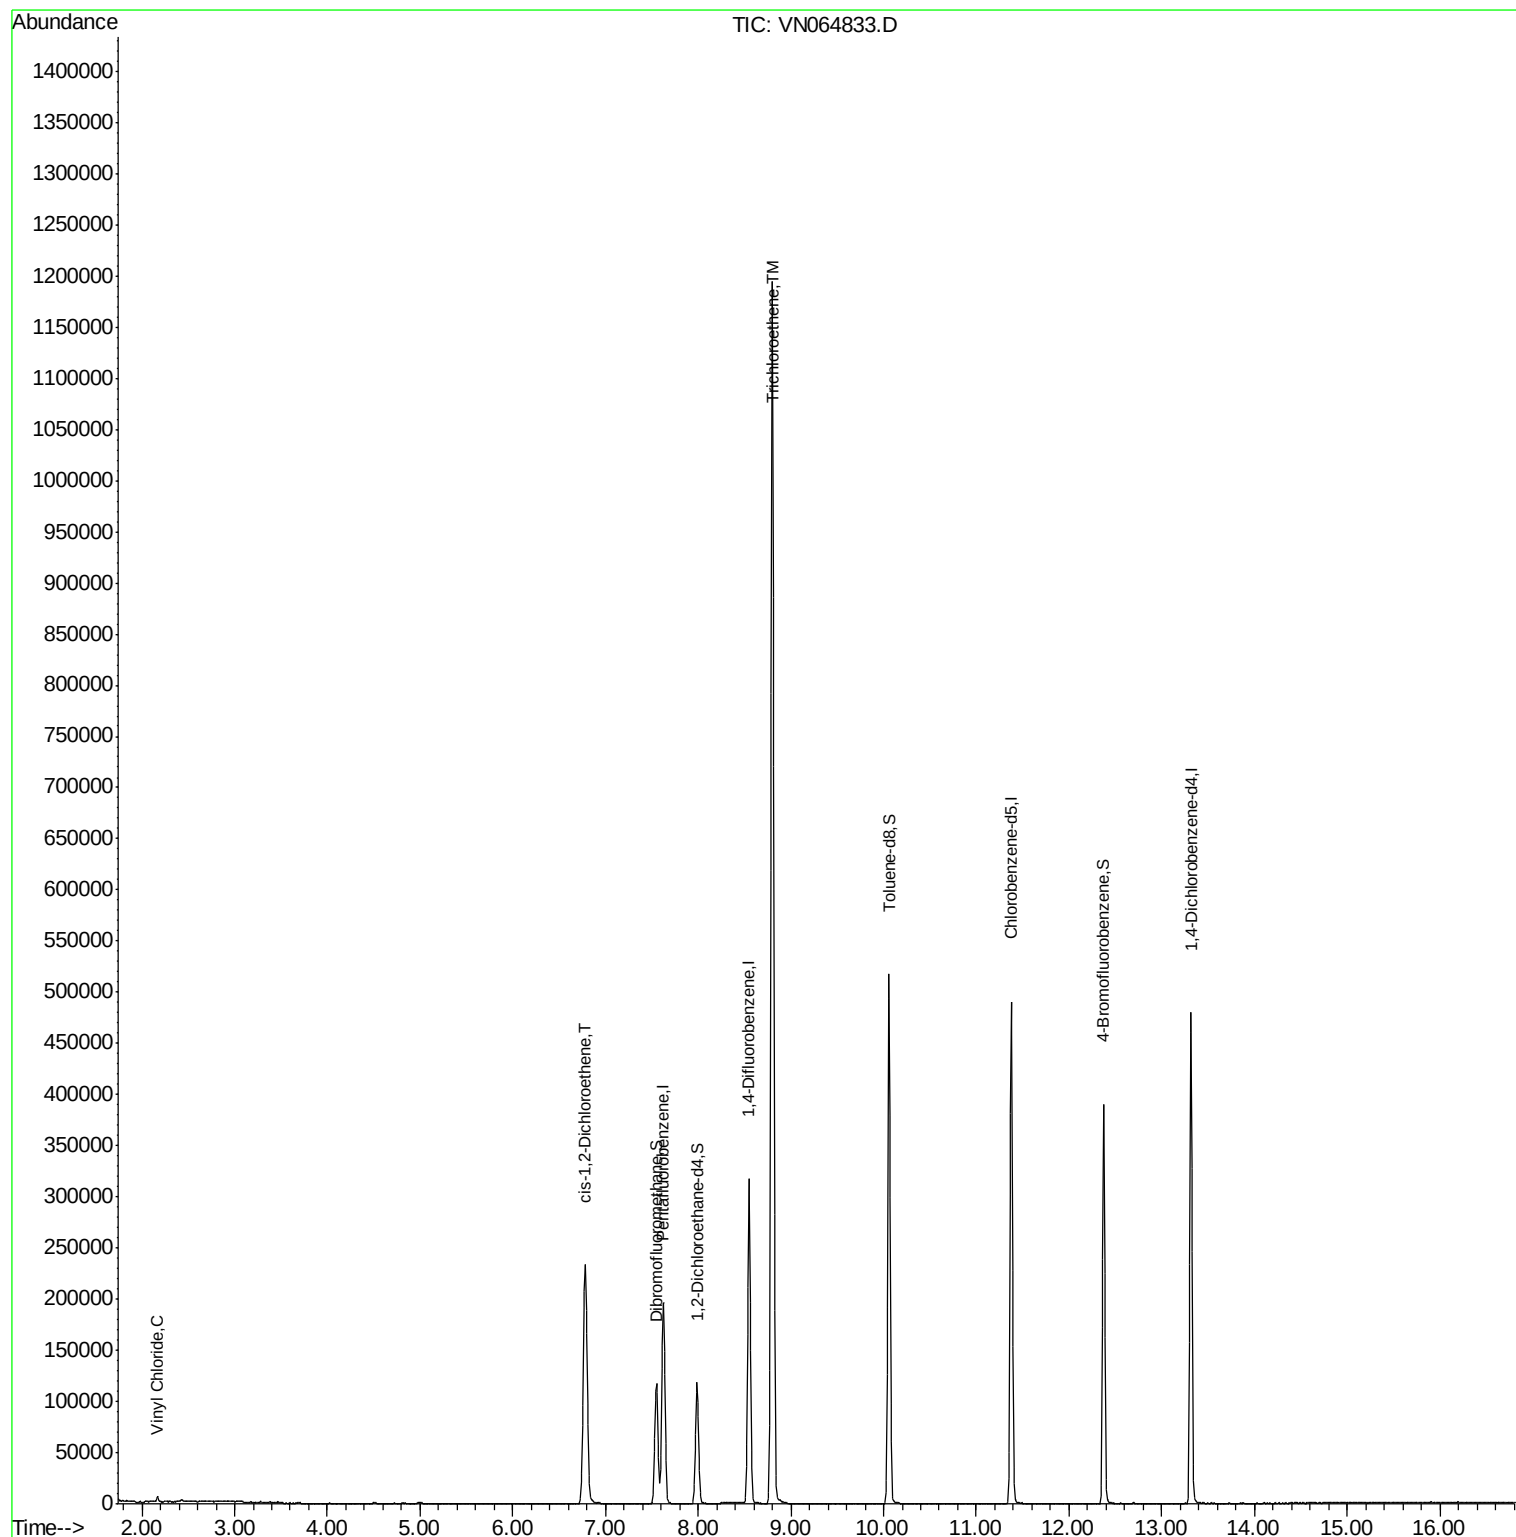

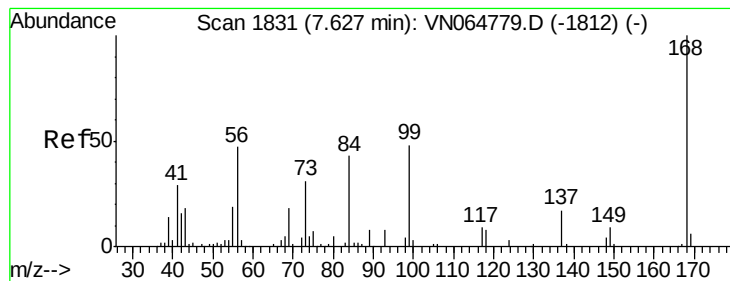

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064833.D

Acq: 25 Nov 2020 1:06

Instrument :

MSVOA_N

ClientSampleId :


45BR-20201118

Tot Ion:168 Resp: 166876

Ion Ratio Lower Upper

168 100

99 53.4 43.0 64.4

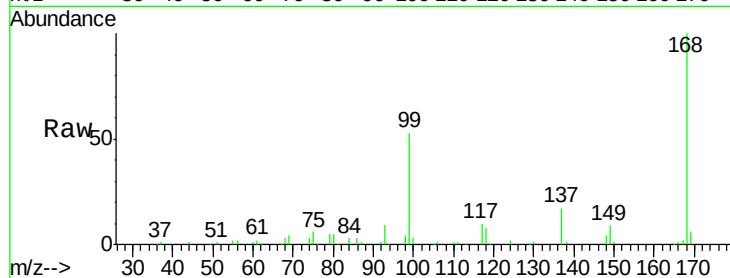

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.63

80000



60000

40000

20000

0

Time-->

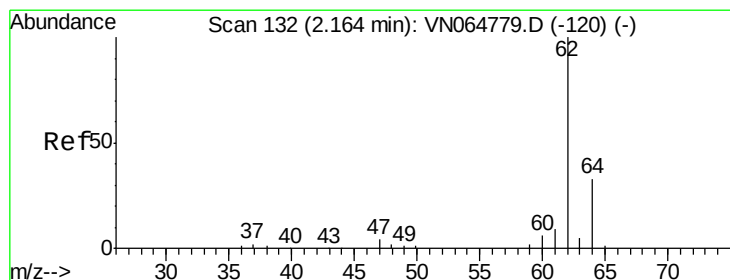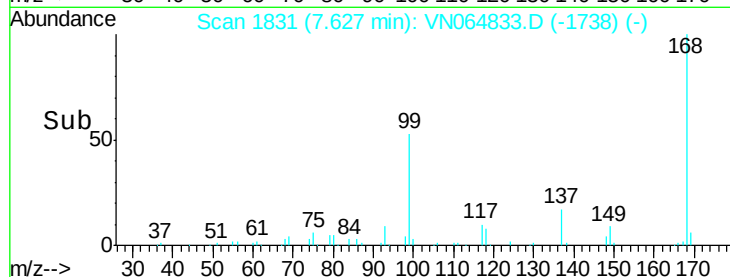

#4

Vinyl Chloride

Concen: 2.735 ug/l

RT: 2.17 min Scan# 133

Delta R.T. 0.00 min

Lab File: VN064833.D


Acq: 25 Nov 2020 1:06

Tgt Ion: 62 Resp: 5359

Ion Ratio Lower Upper

62 100

64 35.6 26.5 39.7

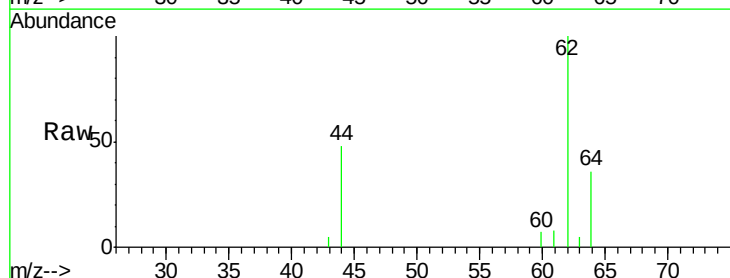

Abundance Ion 61.90 (61.60 to 62.60): VNO

Ion 63.90 (63.60 to 64.60): VNO

2.17

4000


3000


2000

1000

0

Time-->

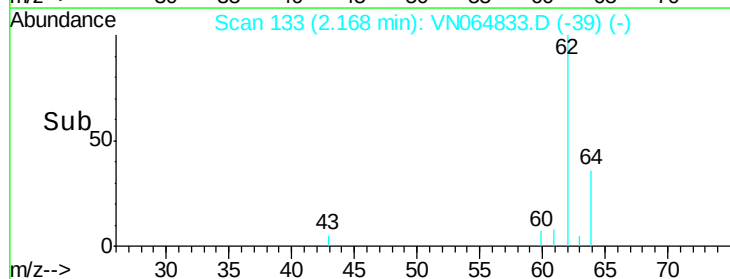

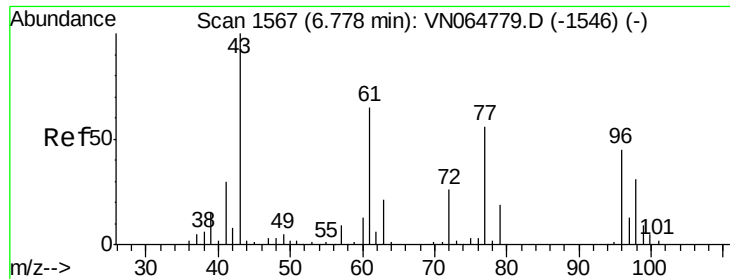

#27

cis-1,2-Dichloroethene

Concen: 80.875 ug/l

RT: 6.78 min Scan# 1569

Delta R.T. 0.01 min

Lab File: VN064833.D

Acq: 25 Nov 2020 1:06

Instrument :

MSVOA_N

ClientSampleId :

45BR-20201118


Tot Ion: 96 Resp: 163537

Ion Ratio Lower Upper

96 100

61 124.5 0.0 285.8




98 64.6 0.0 130.6

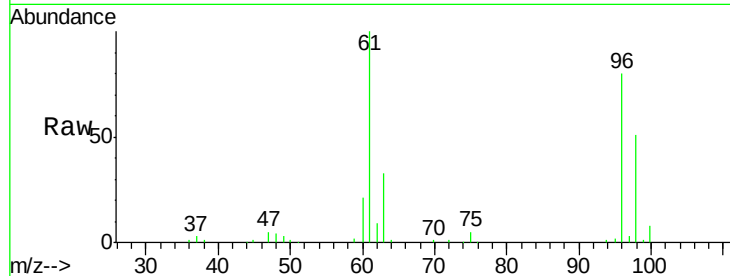

Abundance Ion 95.90 (95.60 to 96.60): VN064833.D (-1474) (-)

Ion 60.90 (60.60 to 61.60): VN064833.D (-1474) (-)

Ion 97.90 (97.60 to 98.60): VN064833.D (-1474) (-)

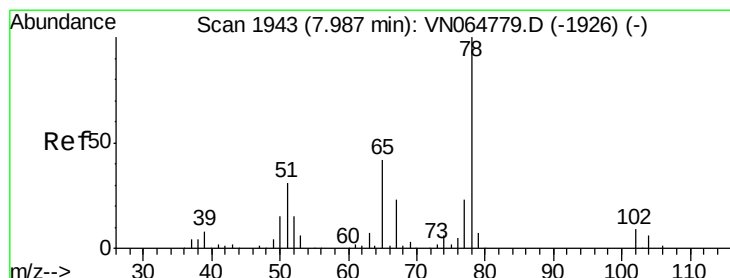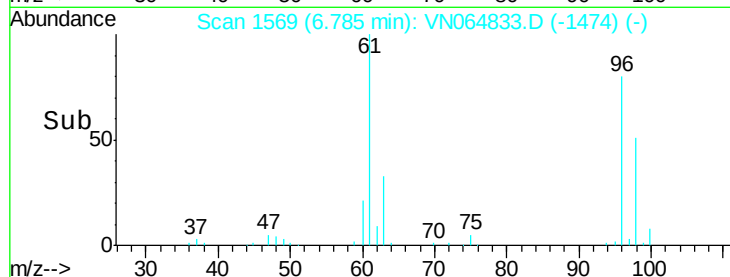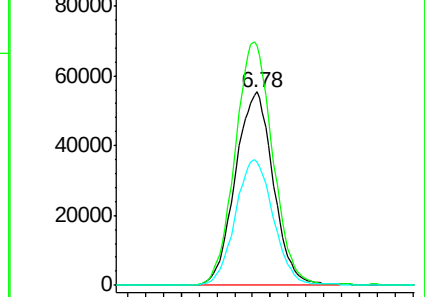

#33

1,2-Dichloroethane-d4

Concen: 52.848 ug/l

RT: 7.99 min Scan# 1943

Delta R.T. 0.00 min

Lab File: VN064833.D


Acq: 25 Nov 2020 1:06

Tgt Ion: 65 Resp: 102527

Ion Ratio Lower Upper



65 100


67 53.2 0.0 108.2

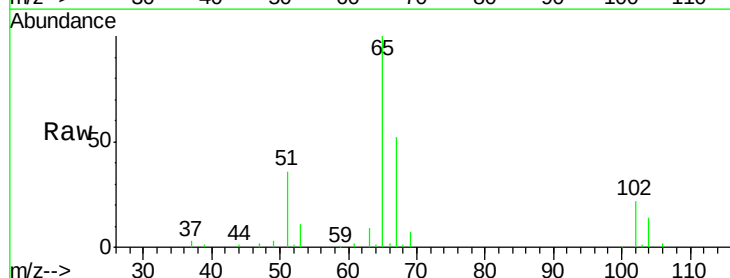

Abundance Ion 64.90 (64.60 to 65.60): VN064833.D (-1850) (-)

Ion 66.90 (66.60 to 67.60): VN064833.D (-1850) (-)

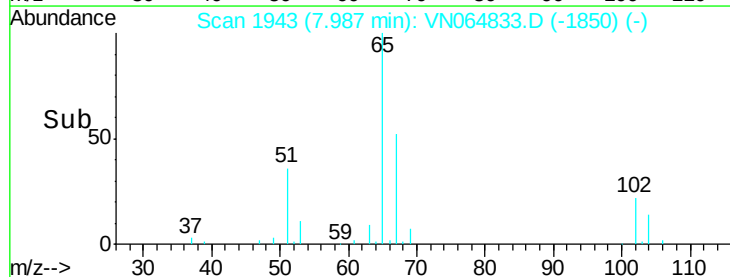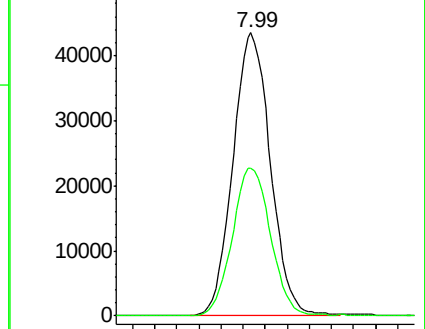

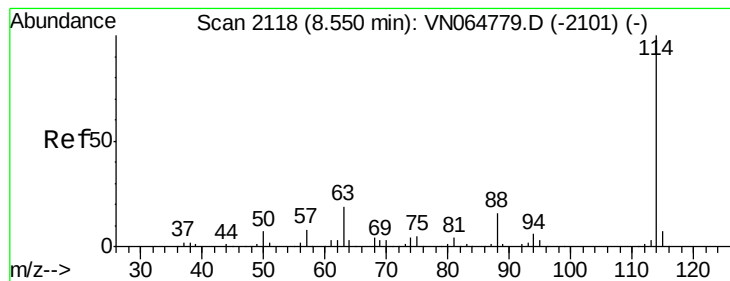

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. 0.00 min

Lab File: VN064833.D

Acq: 25 Nov 2020 1:06

Instrument :

MSVOA_N

ClientSampleId :

45BR-20201118


Tot Ion:114 Resp: 293929

Ion Ratio Lower Upper

114 100

63 19.2 0.0 38.6




88 16.0 0.0 32.6

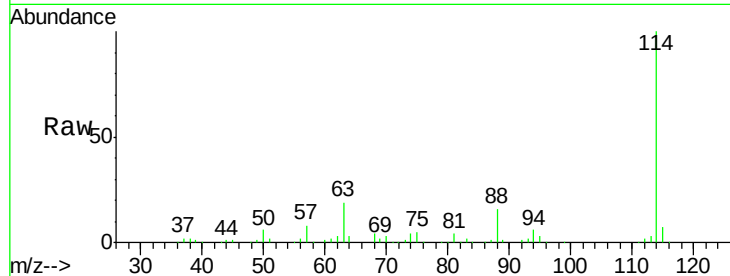

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0

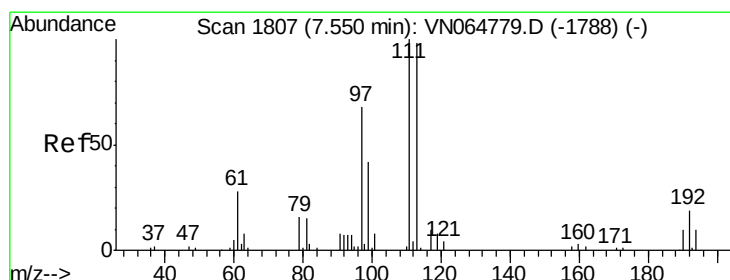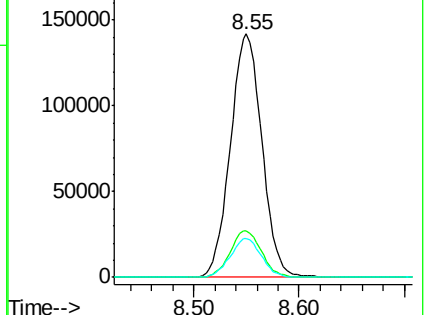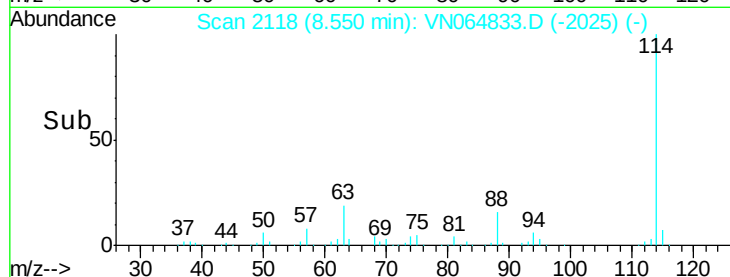

#35

Dibromofluoromethane

Concen: 53.528 ug/l

RT: 7.55 min Scan# 1807

Delta R.T. 0.00 min

Lab File: VN064833.D

Acq: 25 Nov 2020 1:06


Tgt Ion:113 Resp: 94143

Ion Ratio Lower Upper

113 100

111 100.7 81.6 122.4



192 19.5 16.2 24.2

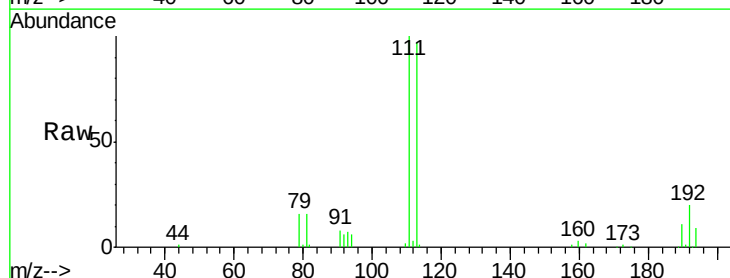


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

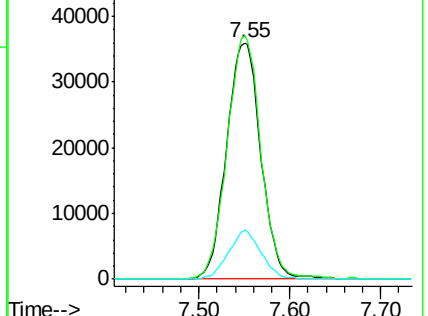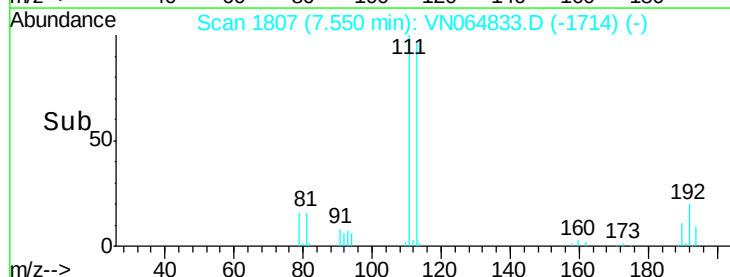

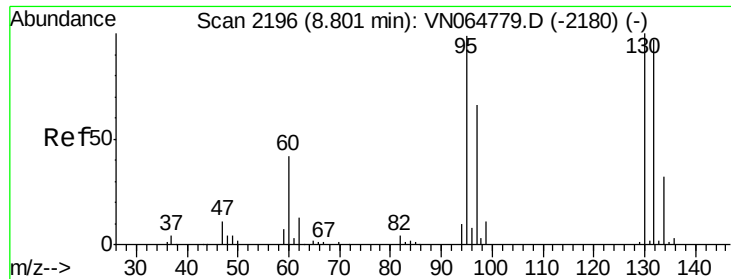

#44

Trichloroethene

Concen: 187.900 ug/l

RT: 8.80 min Scan# 2196

Delta R.T. 0.00 min

Lab File: VN064833.D

Acq: 25 Nov 2020 1:06

Instrument :

MSVOA_N

ClientSampleId :


45BR-20201118

Tot Ion:130 Resp: 462848

Ion Ratio Lower Upper

130 100

95 97.8 0.0 197.8

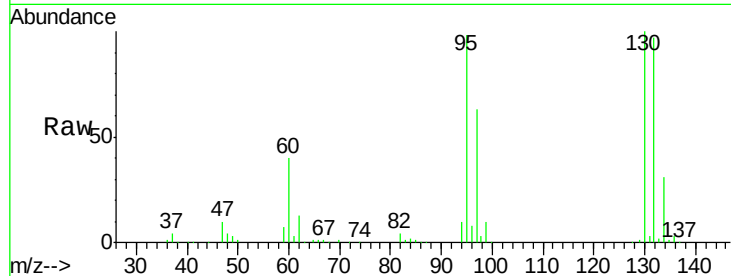

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VN

8.80

250000

200000



150000

100000

50000

0

Time-->

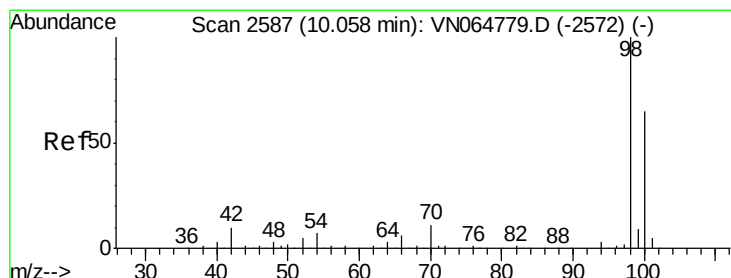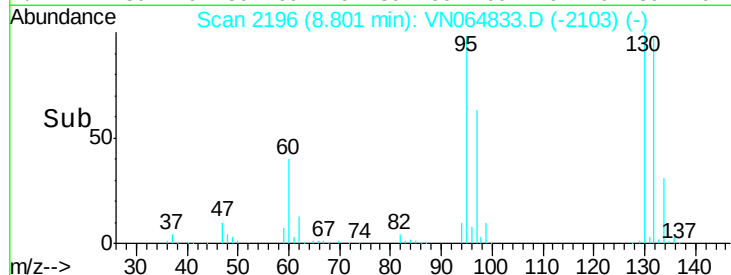

#50

Toluene-d8

Concen: 50.979 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN064833.D


Acq: 25 Nov 2020 1:06

Tgt Ion: 98 Resp: 366350

Ion Ratio Lower Upper

98 100

100 64.2 51.7 77.5

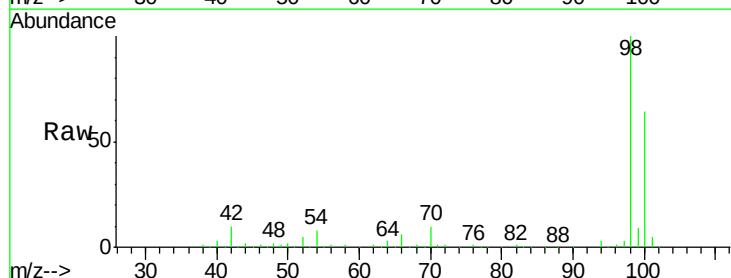

Abundance Ion 98.00 (97.70 to 98.70): VN

Ion 100.00 (99.70 to 100.70): VN

10.06

200000


150000


100000

50000

0

Time-->




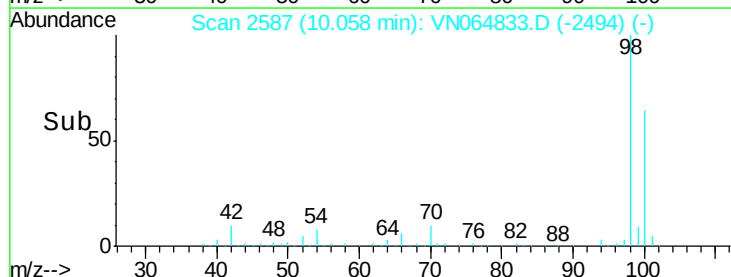


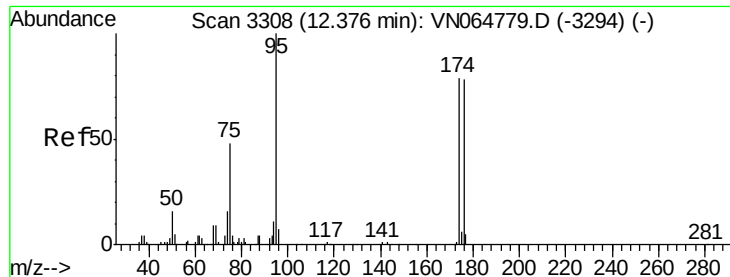

#62
4-Bromofluorobenzene
Concen: 55.014 ug/l
RT: 12.37 min Scan# 3307
Delta R.T. -0.00 min
Lab File: VN064833.D
Acq: 25 Nov 2020 1:06




Instrument :
MSVOA_N
ClientSampleId :
45BR-20201118


Tot Ion: 95 Resp: 141485
Ion Ratio Lower Upper
95 100
174 82.3 0.0 160.4
176 78.6 0.0 158.4

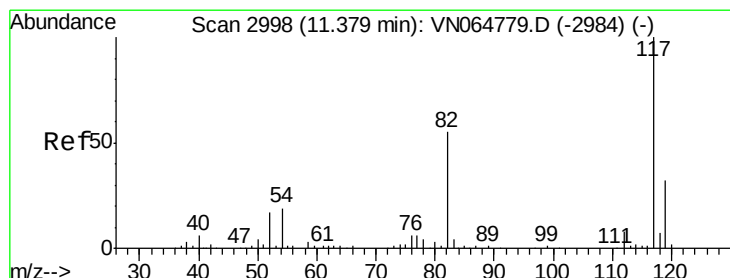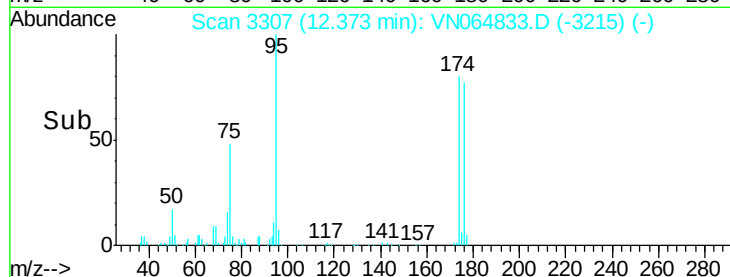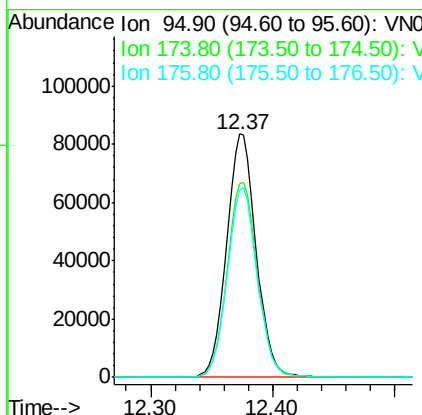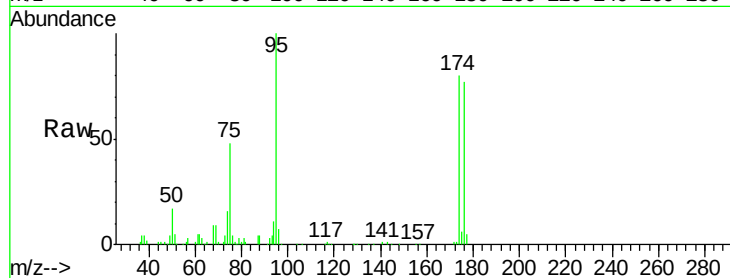

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN064833.D
Acq: 25 Nov 2020 1:06

Tgt Ion: 117 Resp: 302373
Ion Ratio Lower Upper
117 100
82 53.4 44.2 66.2
119 31.9 25.8 38.6

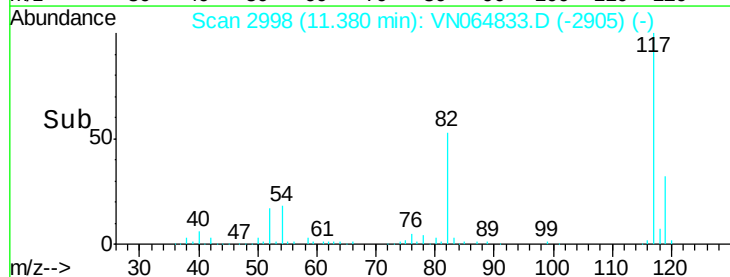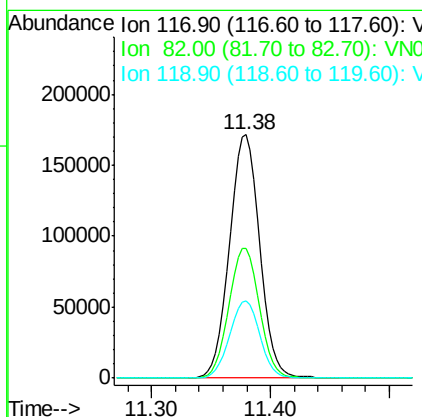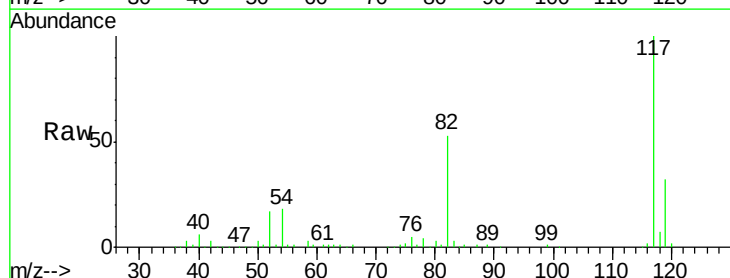

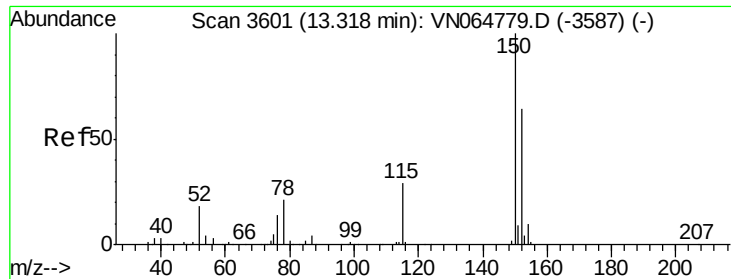

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3600

Delta R.T. -0.00 min

Lab File: VN064833.D

Acq: 25 Nov 2020 1:06

Instrument :

MSVOA_N

ClientSampleId :

45BR-20201118


Tot Ion:152 Resp: 136015

Ion Ratio Lower Upper

152 100

115 58.9 29.7 89.1

150 159.5 0.0 350.6

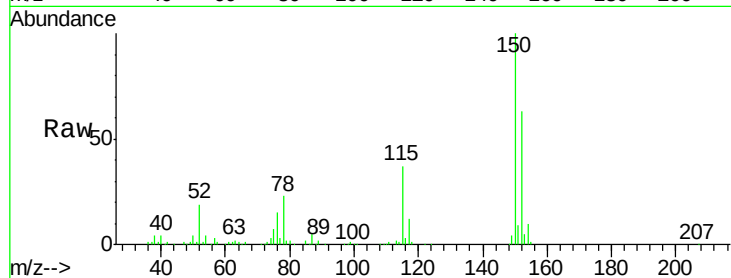

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

