


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN112420\
Data File : VN064798.D
Acq On : 24 Nov 2020 8:50
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Title : SW846 8260
Last Update : Mon Nov 23 13:54:12 2020

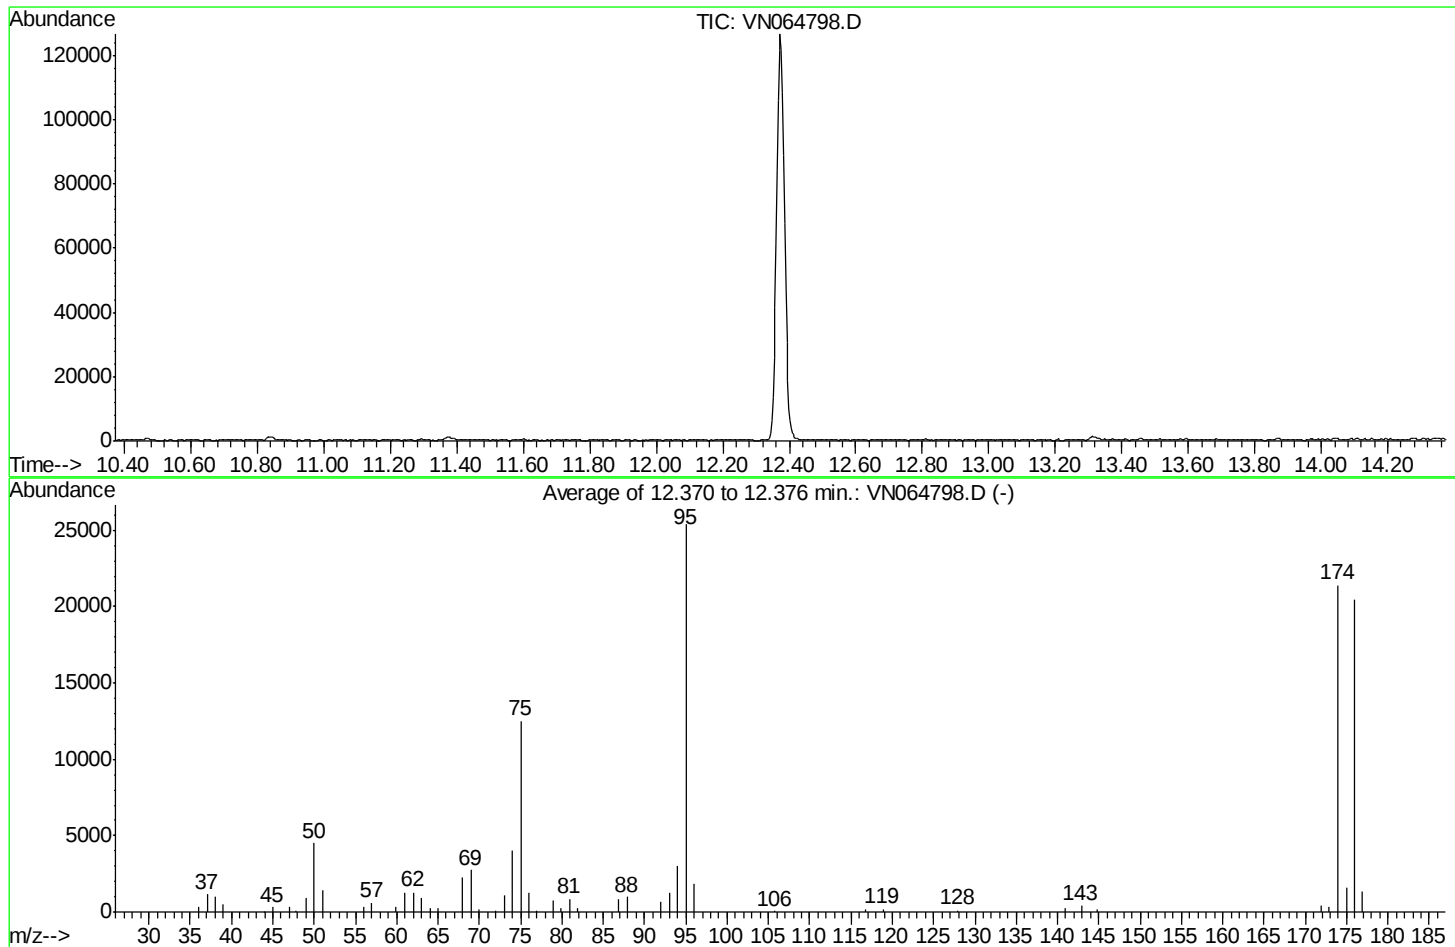

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	4505	PASS
75	95	30	60	49.3	12515	PASS
95	95	100	100	100.0	25381	PASS
96	95	5	9	7.1	1809	PASS
173	174	0.00	2	1.4	309	PASS
174	95	50	100	84.3	21402	PASS
175	174	5	9	7.6	1622	PASS
176	174	95	101	95.5	20442	PASS
177	176	5	9	6.4	1318	PASS