


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN112420\
 Data File : VN064823.D
 Acq On : 24 Nov 2020 20:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
 Title : SW846 8260
 Last Update : Mon Nov 23 13:54:12 2020

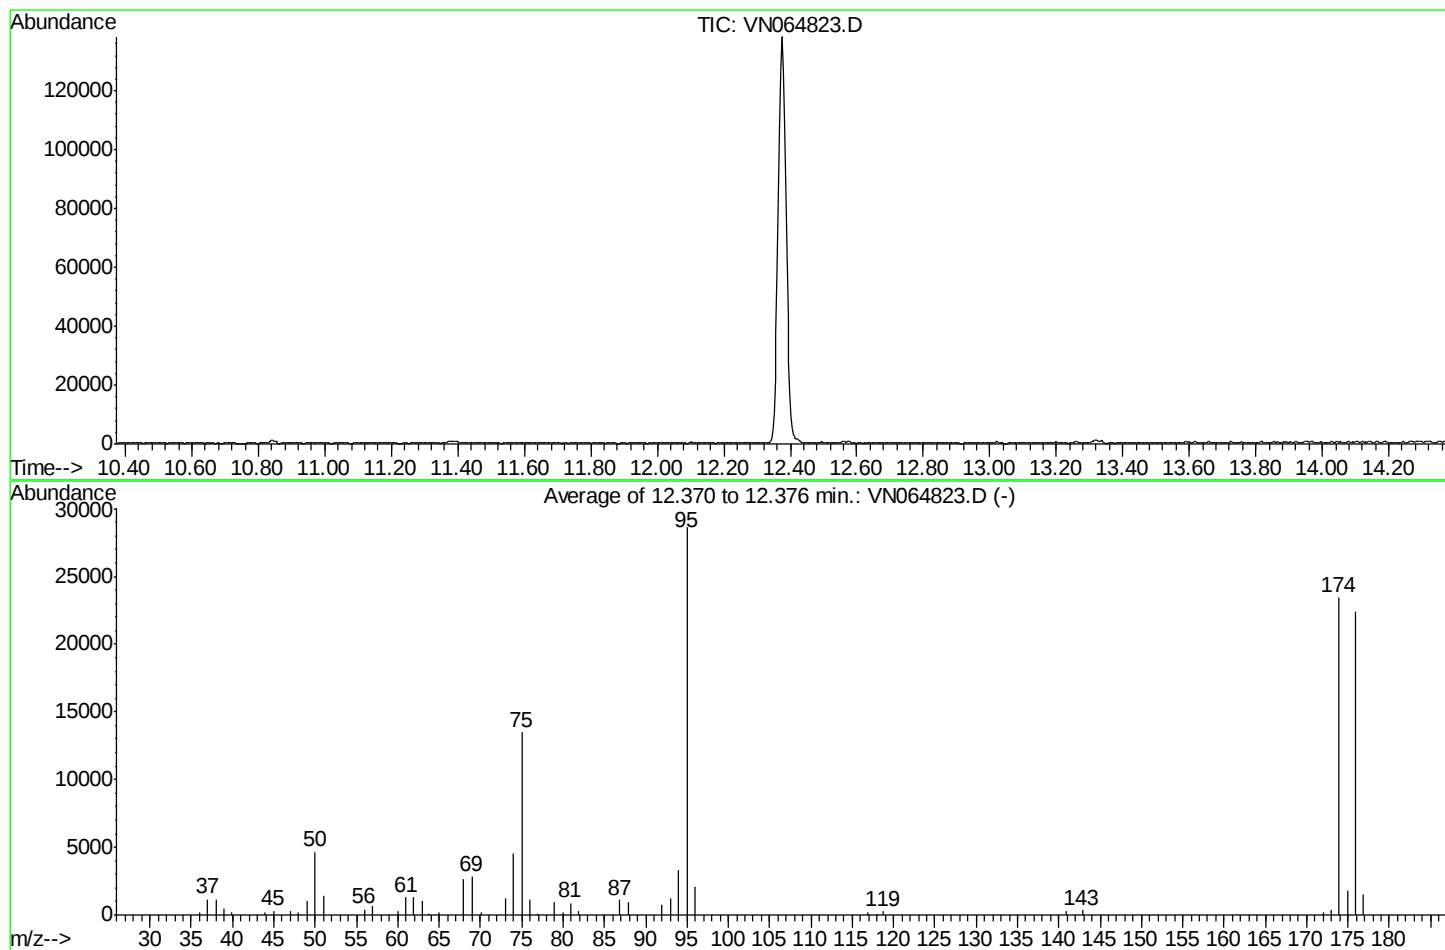

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	4647	PASS
75	95	30	60	47.1	13489	PASS
95	95	100	100	100.0	28626	PASS
96	95	5	9	7.2	2073	PASS
173	174	0.00	2	1.6	386	PASS
174	95	50	100	81.8	23416	PASS
175	174	5	9	7.6	1770	PASS
176	174	95	101	95.6	22376	PASS
177	176	5	9	6.7	1502	PASS