
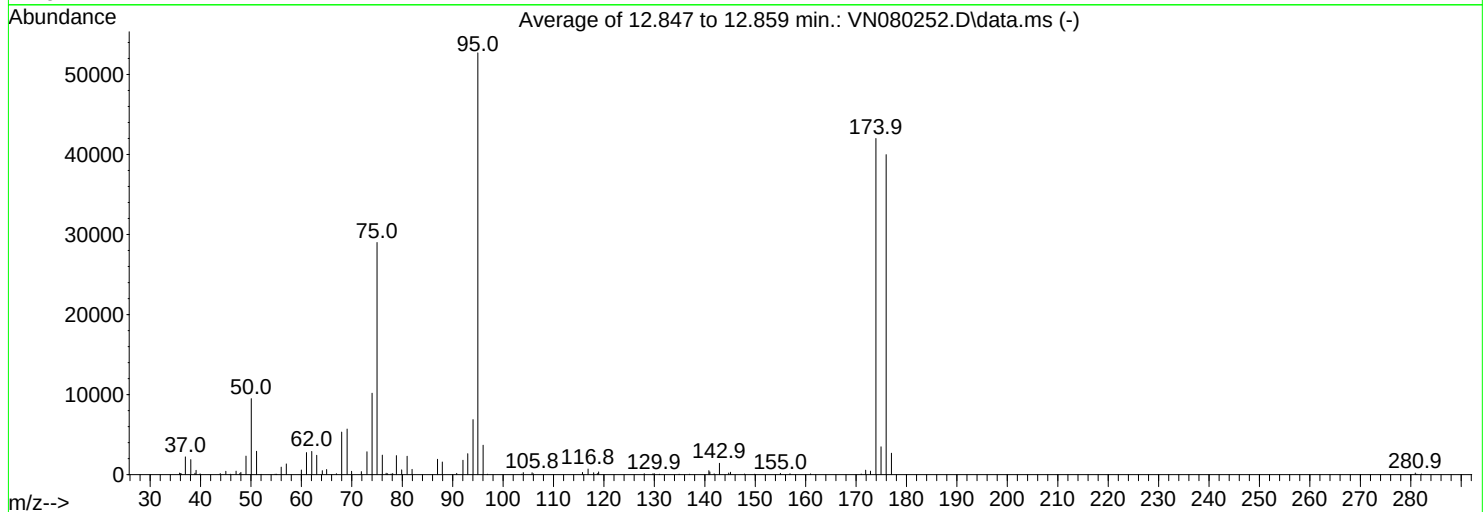


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112423\
Data File : VN080252.D
Acq On : 24 Nov 2023 10:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N110823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Nov 09 04:02:05 2023

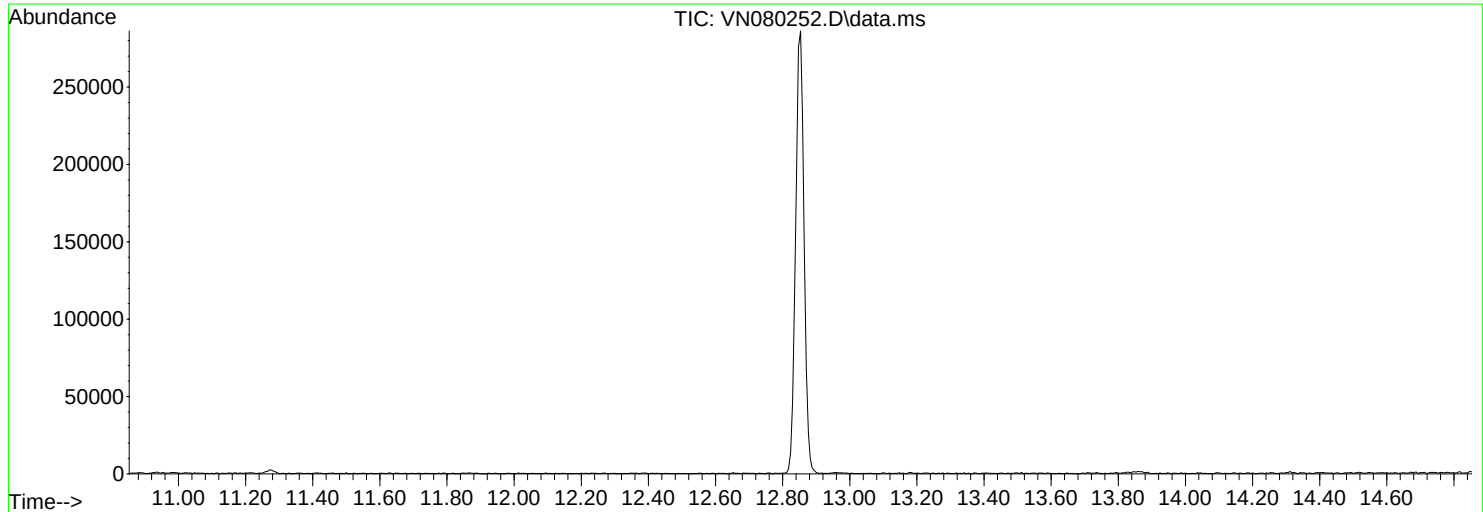

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	9488	PASS
75	95	30	60	55.1	29019	PASS
95	95	100	100	100.0	52701	PASS
96	95	5	9	7.0	3687	PASS
173	174	0.00	2	1.0	439	PASS
174	95	50	100	79.7	42011	PASS
175	174	5	9	8.3	3485	PASS
176	174	95	101	95.2	39984	PASS
177	176	5	9	6.7	2682	PASS