


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN112519\
Data File : VN059379.D
Acq On : 25 Nov 2019 9:13
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112019W.M
Title : SW846 8260
Last Update : Thu Nov 21 08:44:45 2019

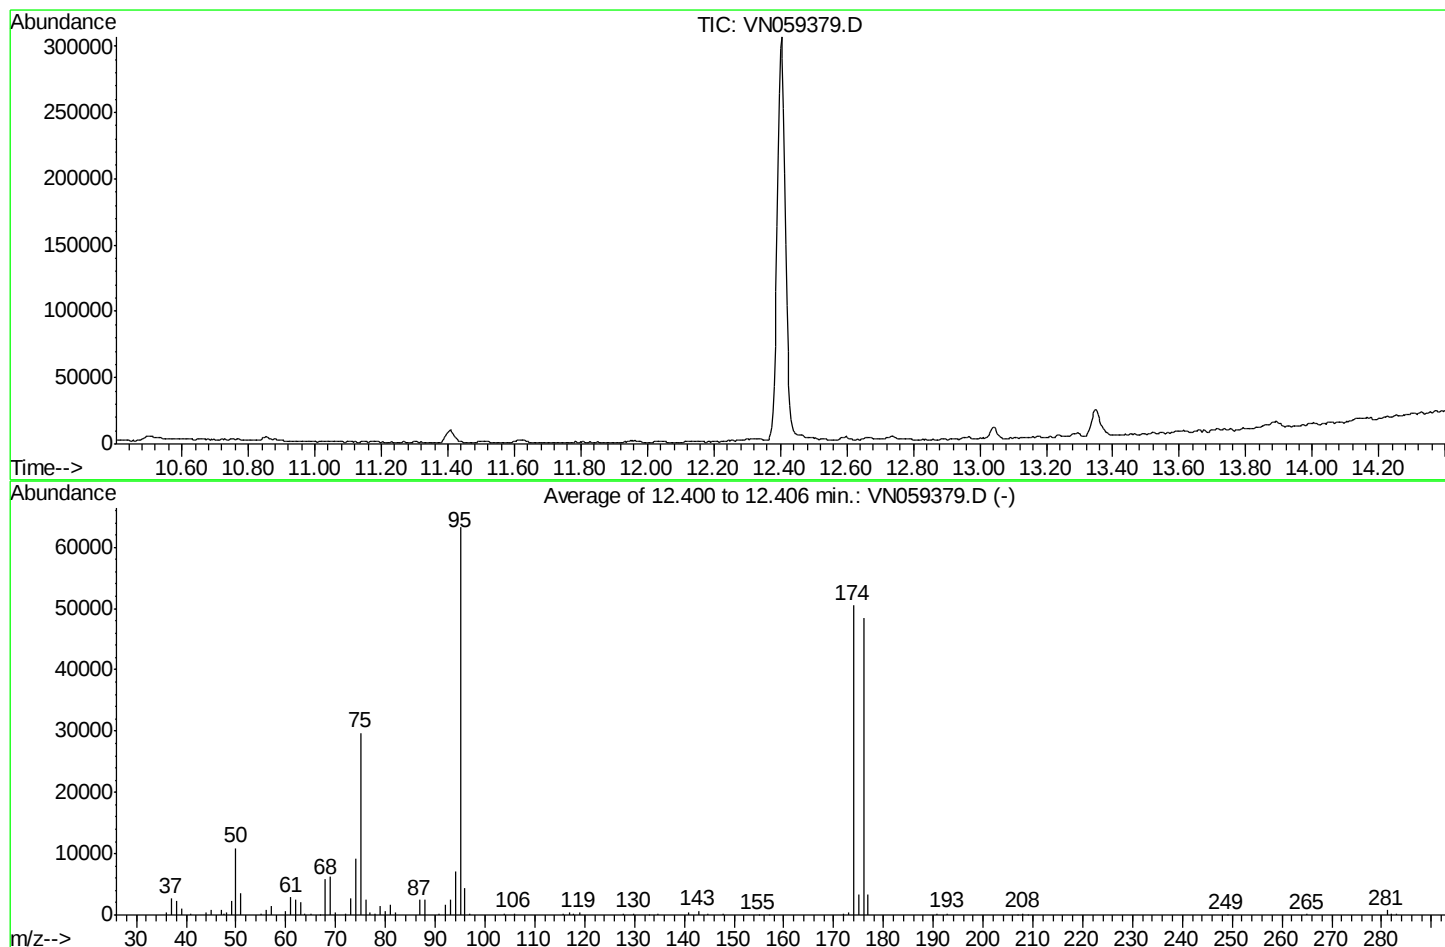

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	10873	PASS
75	95	30	60	46.9	29658	PASS
95	95	100	100	100.0	63248	PASS
96	95	5	9	7.1	4477	PASS
173	174	0.00	2	0.8	386	PASS
174	95	50	100	79.9	50504	PASS
175	174	5	9	6.8	3440	PASS
176	174	95	101	96.0	48488	PASS
177	176	5	9	6.8	3292	PASS