

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN112520\
 Data File : VN064859.D
 Acq On : 25 Nov 2020 16:30
 Operator : JC/MD
 Sample : L4857-07
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TRIP-BLANK

Quant Time: Nov 26 04:34:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 23 13:54:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.62	168	165334	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	313627	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	324444	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	157681	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	7.99	65	104456	54.34	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	108.68%
35) Dibromofluoromethane	7.55	113	94866	50.55	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	101.10%
50) Toluene-d8	10.06	98	384750	50.18	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.36%
62) 4-Bromofluorobenzene	12.37	95	162409	59.18	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	118.36%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN112520\
Data File : VN064859.D
Acq On : 25 Nov 2020 16:30
Operator : JC/MD
Sample : L4857-07
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK

Quant Time: Nov 26 04:34:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Quant Title : SW846 8260
QLast Update : Mon Nov 23 13:54:12 2020
Response via : Initial Calibration

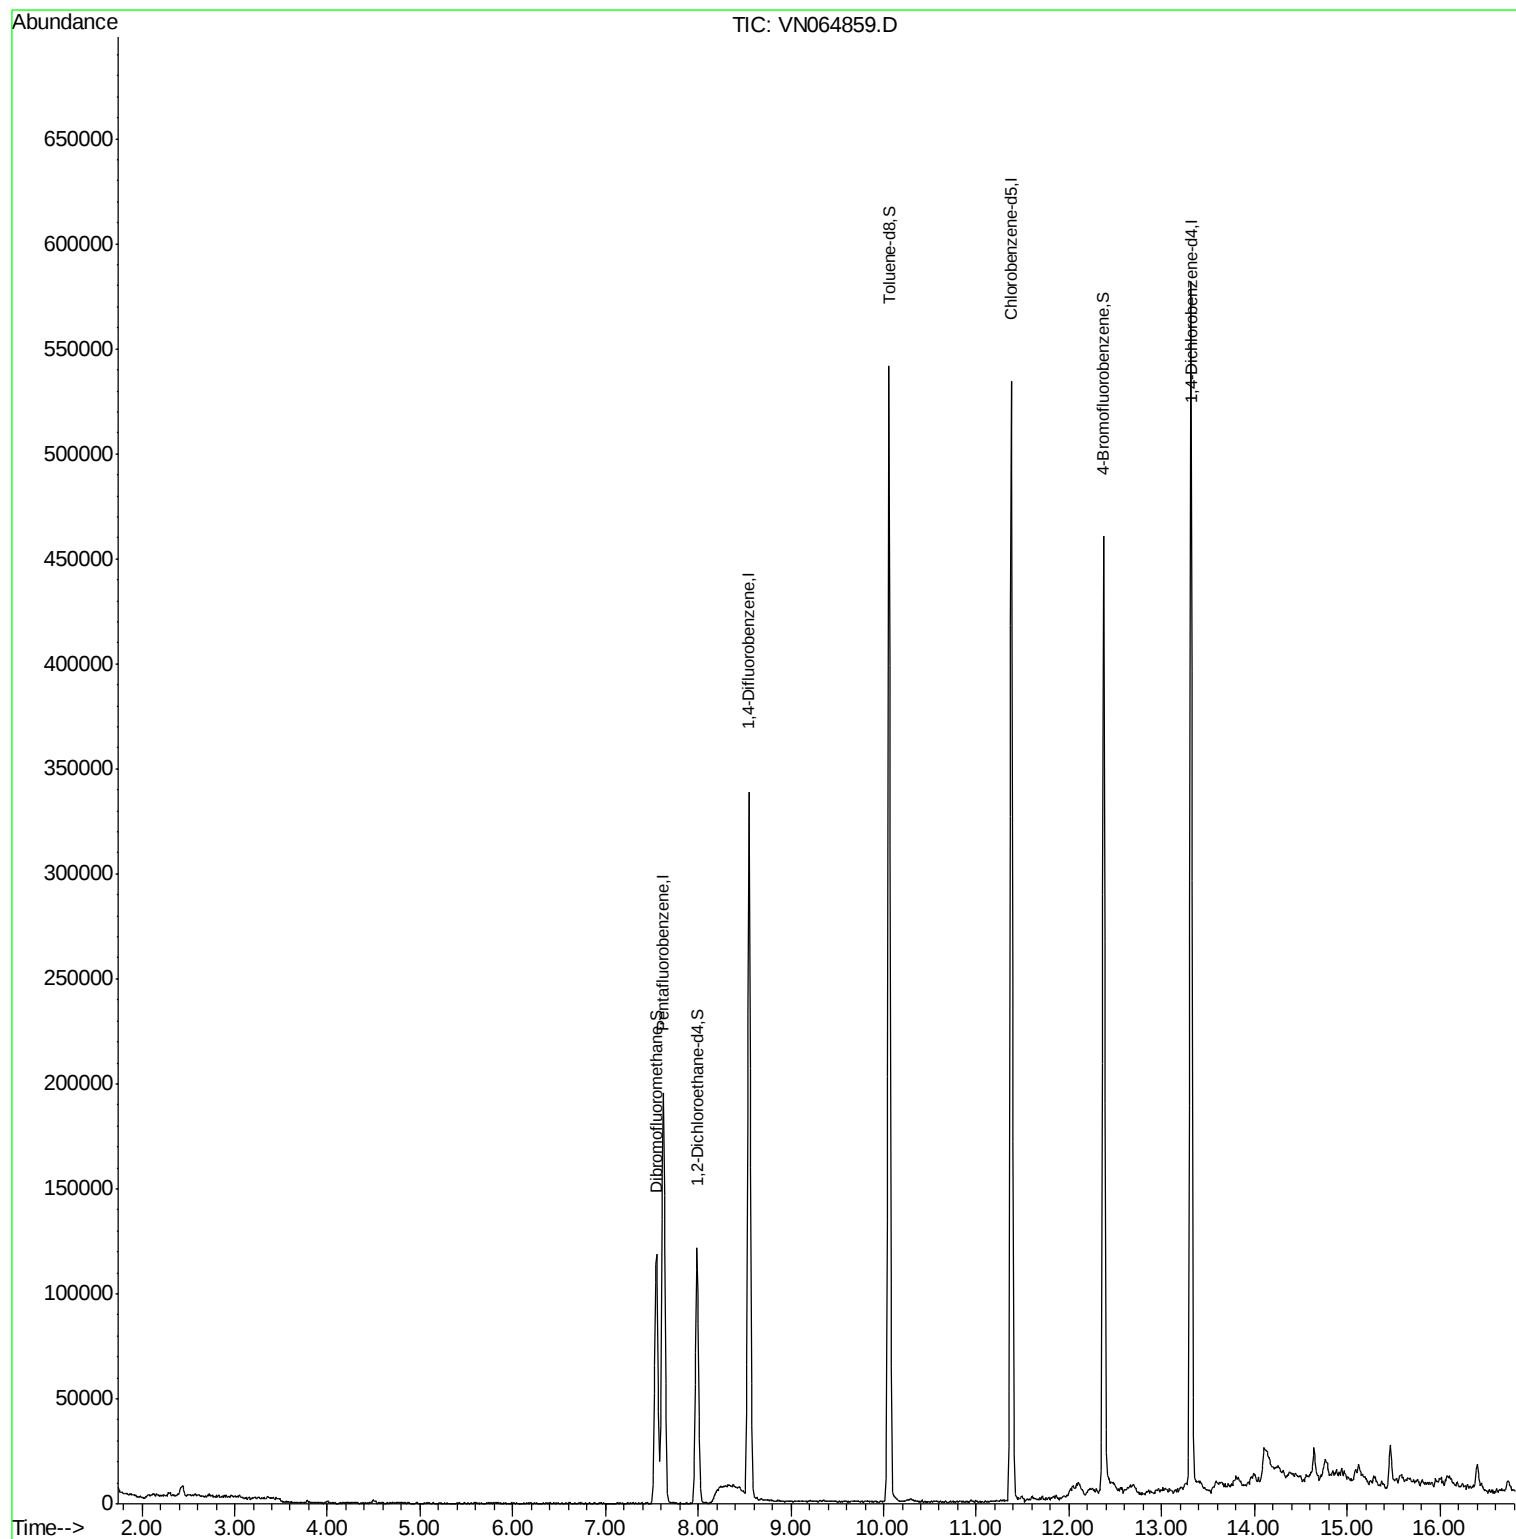

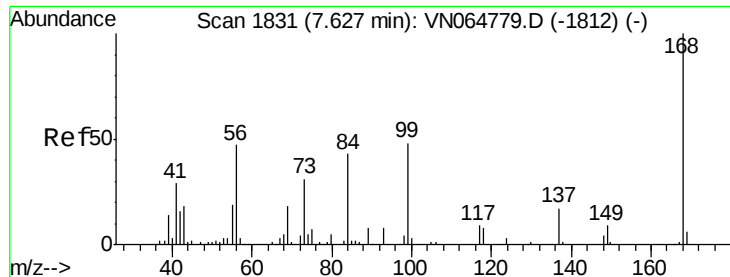

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. -0.00 min

Lab File: VN064859.D

Acq: 25 Nov 2020 16:30

Instrument :

MSVOA_N

ClientSampleId :


TRIP-BLANK

Tot Ion:168 Resp: 165334

Ion Ratio Lower Upper

168 100

99 57.4 43.0 64.4

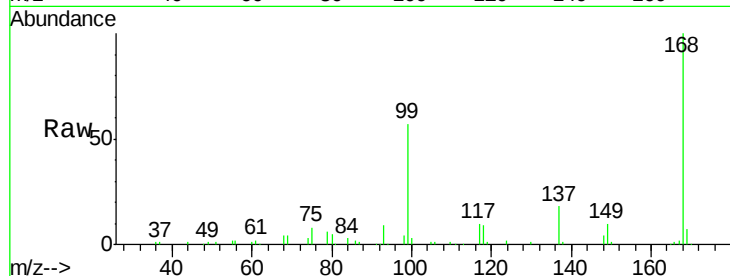

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.62



60000

40000

20000

0

Time--> 7.50 7.60 7.70

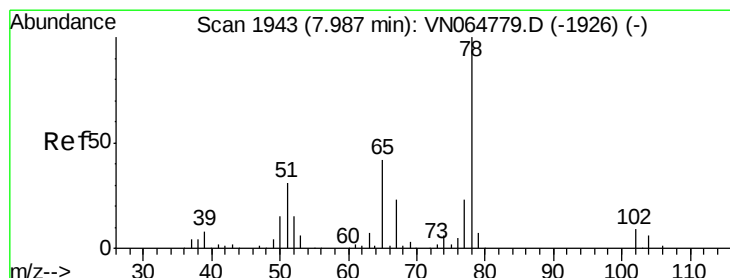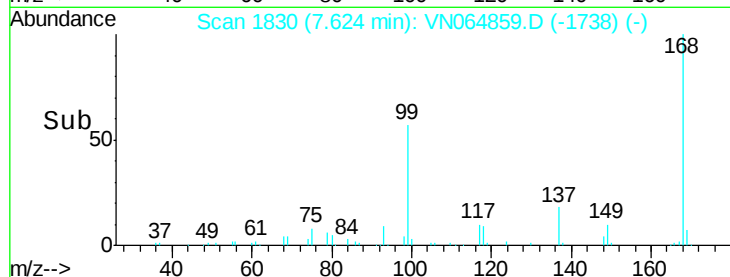

#33

1,2-Dichloroethane-d4

Concen: 54.344 ug/l

RT: 7.99 min Scan# 1943

Delta R.T. 0.00 min

Lab File: VN064859.D


Acq: 25 Nov 2020 16:30

Tgt Ion: 65 Resp: 104456

Ion Ratio Lower Upper

65 100

67 53.4 0.0 108.2

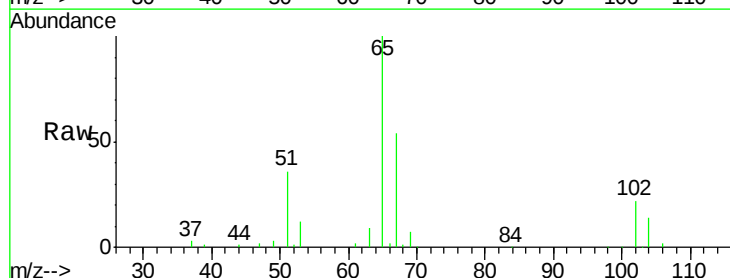

Abundance Ion 64.90 (64.60 to 65.60): VN

Ion 66.90 (66.60 to 67.60): VN

7.99

50000

40000


30000


20000

10000

0

Time--> 7.90 8.00 8.10

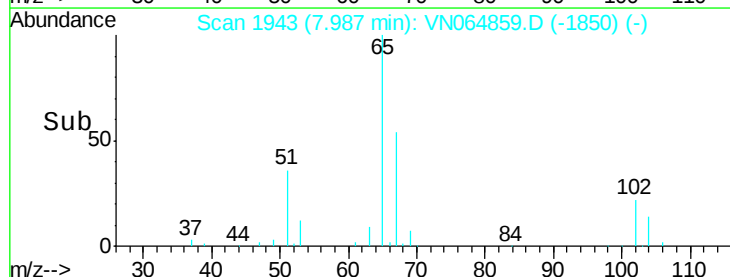

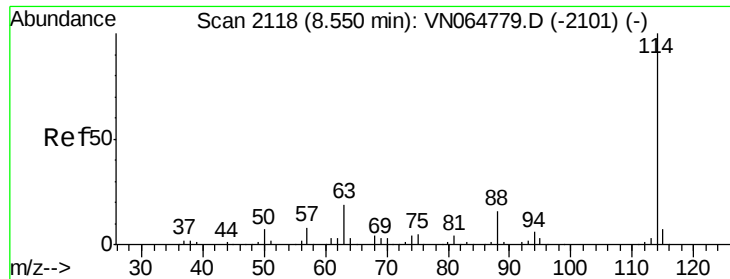

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. 0.00 min

Lab File: VN064859.D

Acq: 25 Nov 2020 16:30

Instrument :

MSVOA_N

ClientSampleId :

TRIP-BLANK


Tot Ion:114 Resp: 313627

Ion Ratio Lower Upper

114 100

63 18.9 0.0 38.6




88 15.1 0.0 32.6

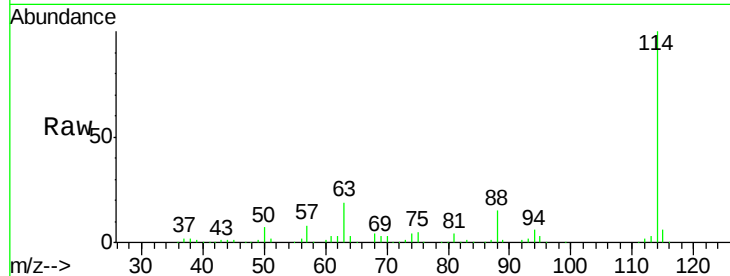

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

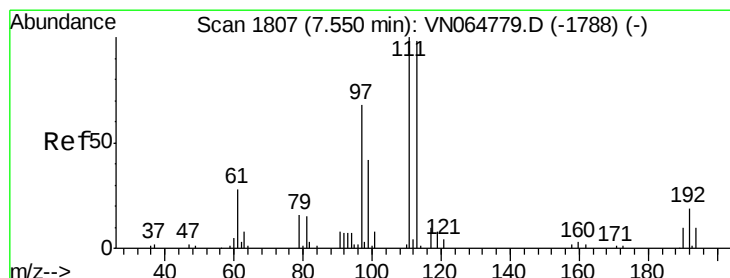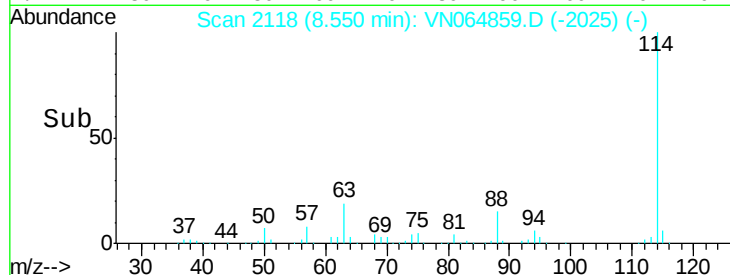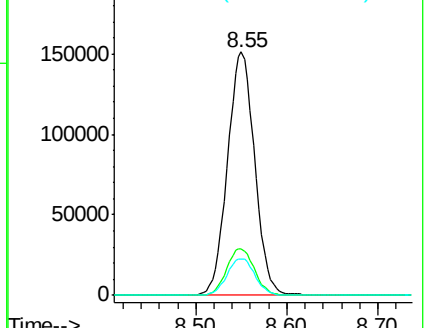

#35

Dibromofluoromethane

Concen: 50.551 ug/l

RT: 7.55 min Scan# 1807

Delta R.T. 0.00 min

Lab File: VN064859.D

Acq: 25 Nov 2020 16:30


Tgt Ion:113 Resp: 94866

Ion Ratio Lower Upper

113 100

111 100.2 81.6 122.4



192 19.4 16.2 24.2

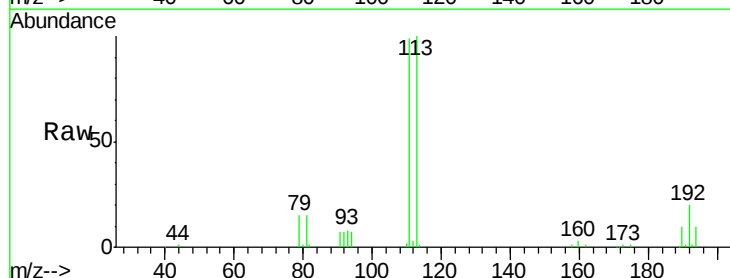


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

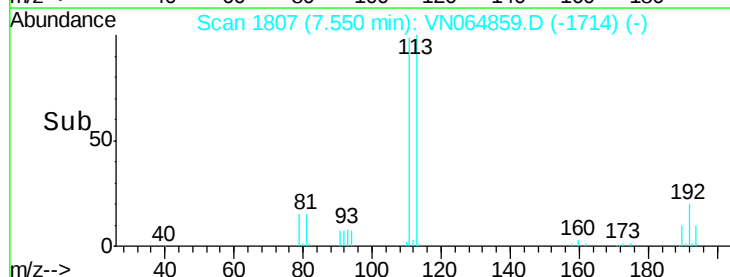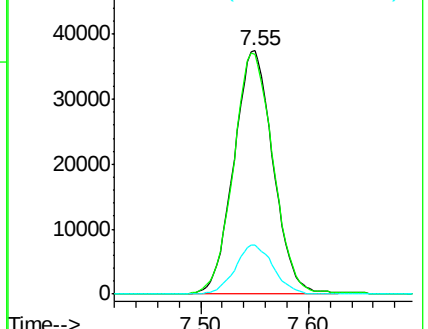

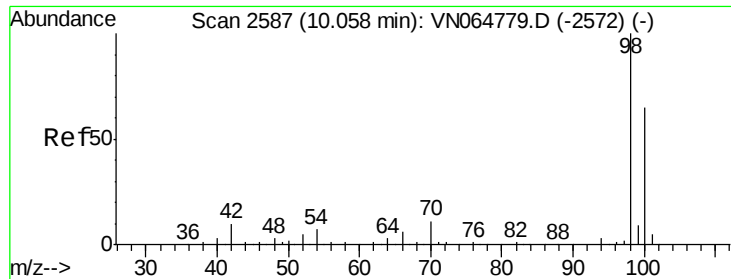

#50

Toluene-d8

Concen: 50.177 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN064859.D

Acq: 25 Nov 2020 16:30

Instrument :

MSVOA_N

ClientSampled :


TRIP-BLANK

Tot Ion: 98 Resp: 384750

Ion Ratio Lower Upper

98 100

100 63.9 51.7 77.5

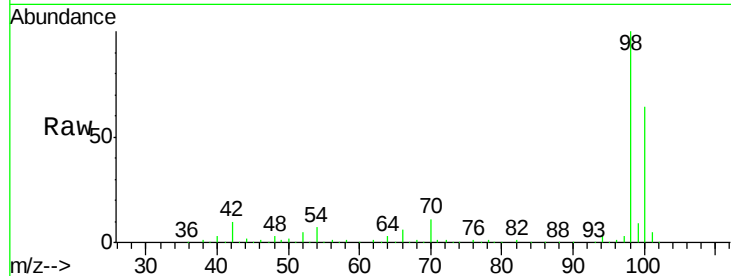

Abundance Ion 98.00 (97.70 to 98.70): VN064779.D (-2572) (-)

Ion 100.00 (99.70 to 100.70): VN064779.D (-2572) (-)

10.06

200000



150000

100000

50000

0

Time-->

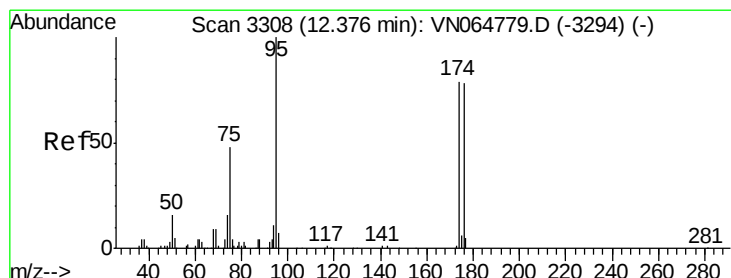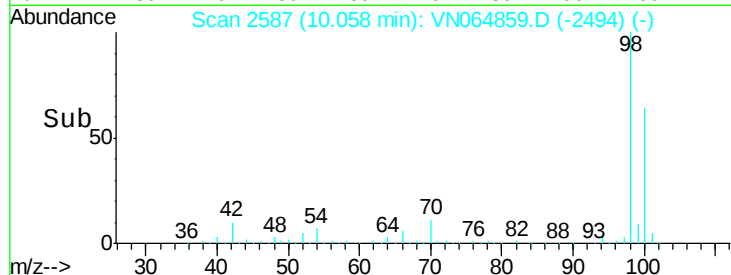

#62

4-Bromofluorobenzene

Concen: 59.183 ug/l

RT: 12.37 min Scan# 3307

Delta R.T. -0.00 min

Lab File: VN064859.D

Acq: 25 Nov 2020 16:30


Tgt Ion: 95 Resp: 162409

Ion Ratio Lower Upper

95 100

174 81.4 0.0 160.4

176 78.1 0.0 158.4

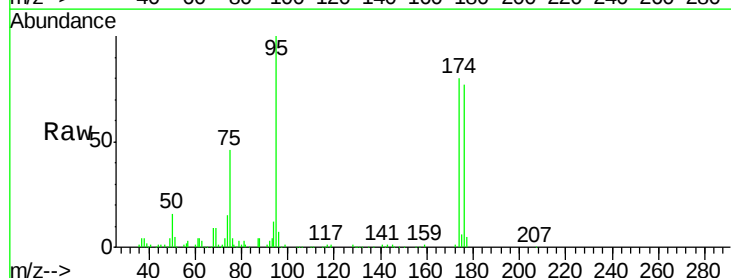

Abundance Ion 94.90 (94.60 to 95.60): VN064779.D (-3294) (-)

Ion 173.80 (173.50 to 174.50): VN064779.D (-3294) (-)

Ion 175.80 (175.50 to 176.50): VN064779.D (-3294) (-)

12.37

120000

100000

80000


60000


40000

20000

0

Time-->

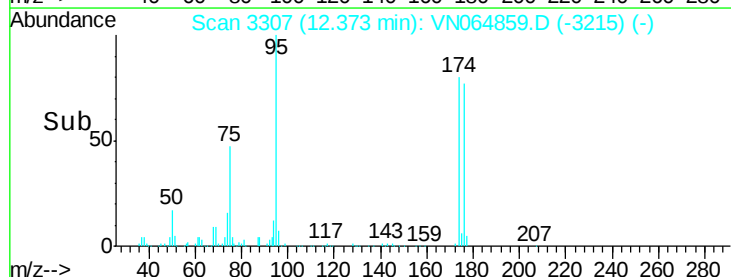


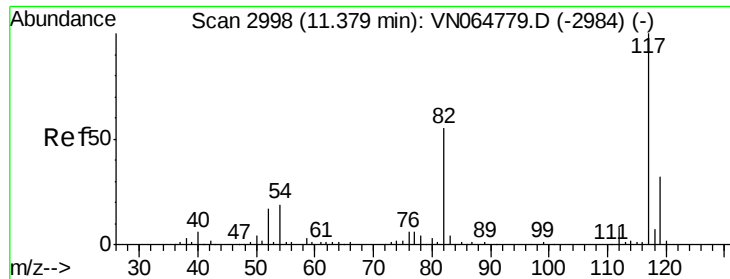




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN064859.D
Acq: 25 Nov 2020 16:30

Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK

Tot Ion:117 Resp: 324444
Ion Ratio Lower Upper
117 100
82 53.9 44.2 66.2
119 31.9 25.8 38.6

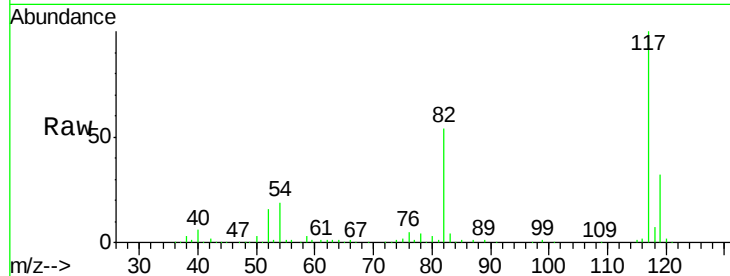


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

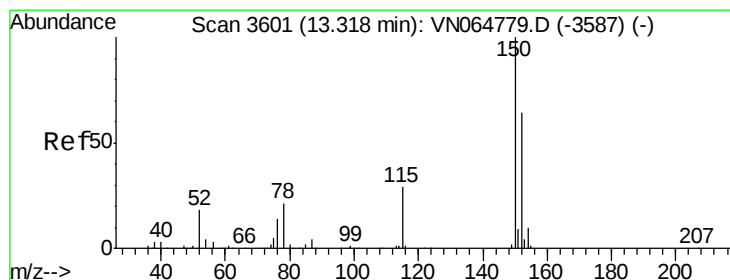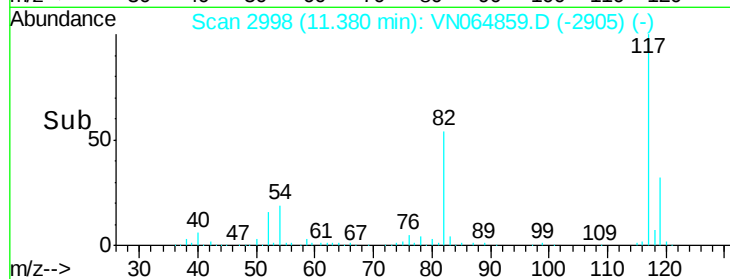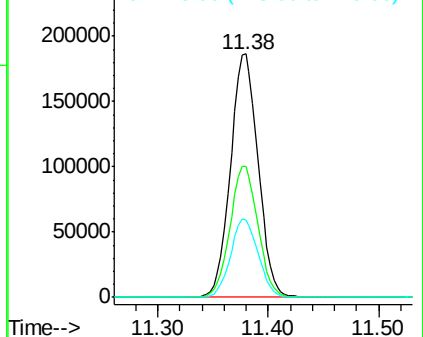

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3600
Delta R.T. -0.00 min
Lab File: VN064859.D
Acq: 25 Nov 2020 16:30

Tgt Ion:152 Resp: 157681
Ion Ratio Lower Upper
152 100
115 58.7 29.7 89.1
150 158.1 0.0 350.6

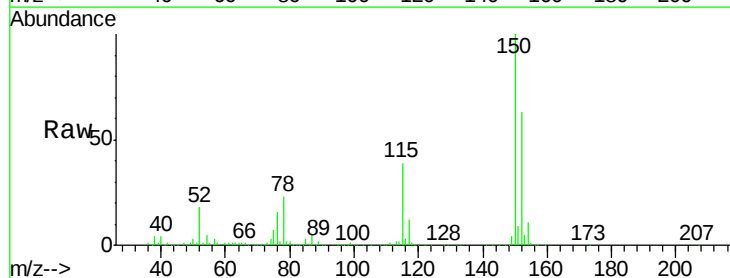

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

