


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN112520\
Data File : VN064844.D
Acq On : 25 Nov 2020 8:26
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Title : SW846 8260
Last Update : Mon Nov 23 13:54:12 2020

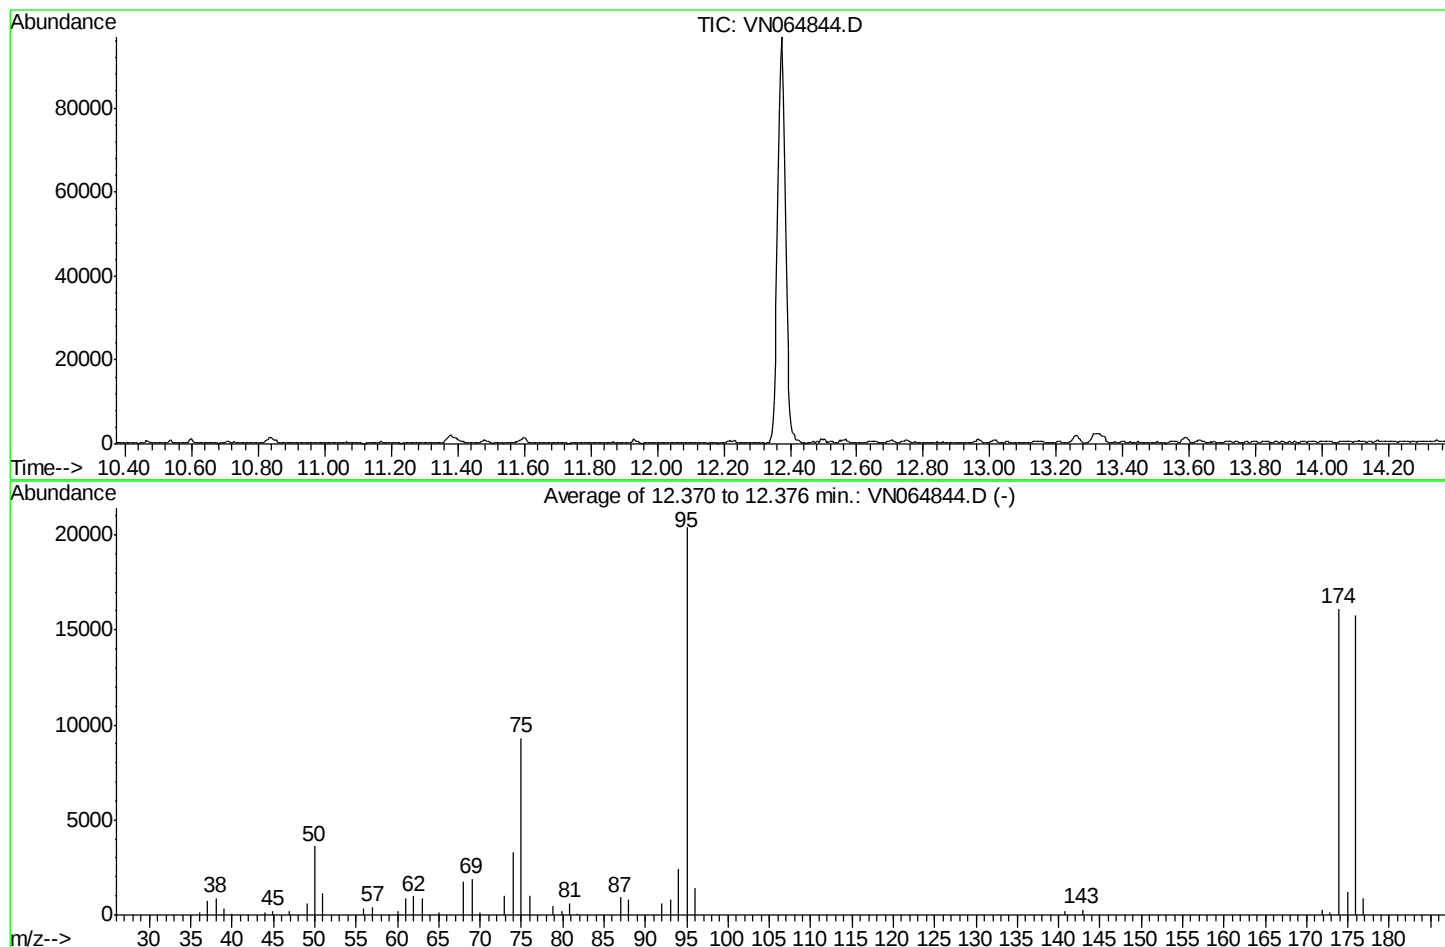

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	3609	PASS
75	95	30	60	45.6	9311	PASS
95	95	100	100	100.0	20400	PASS
96	95	5	9	7.1	1439	PASS
173	174	0.00	2	0.8	129	PASS
174	95	50	100	79.0	16111	PASS
175	174	5	9	7.7	1237	PASS
176	174	95	101	97.9	15776	PASS
177	176	5	9	5.6	887	PASS