
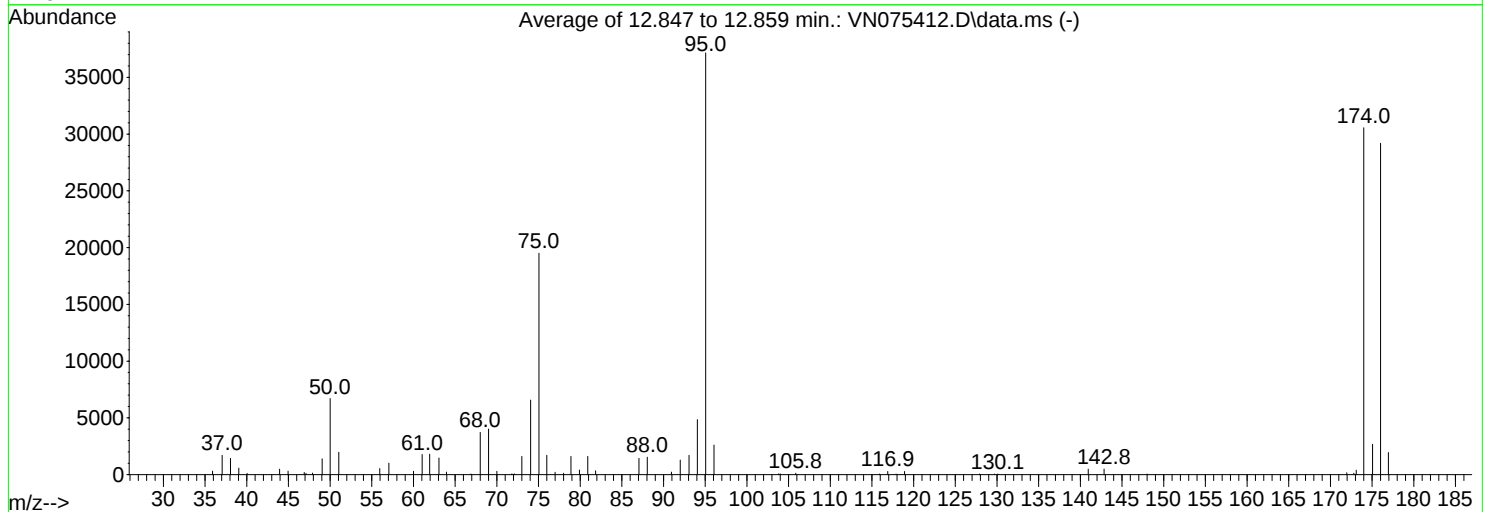


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112522\
Data File : VN075412.D
Acq On : 25 Nov 2022 09:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Title : SW846 8260
Last Update : Wed Nov 23 00:18:03 2022

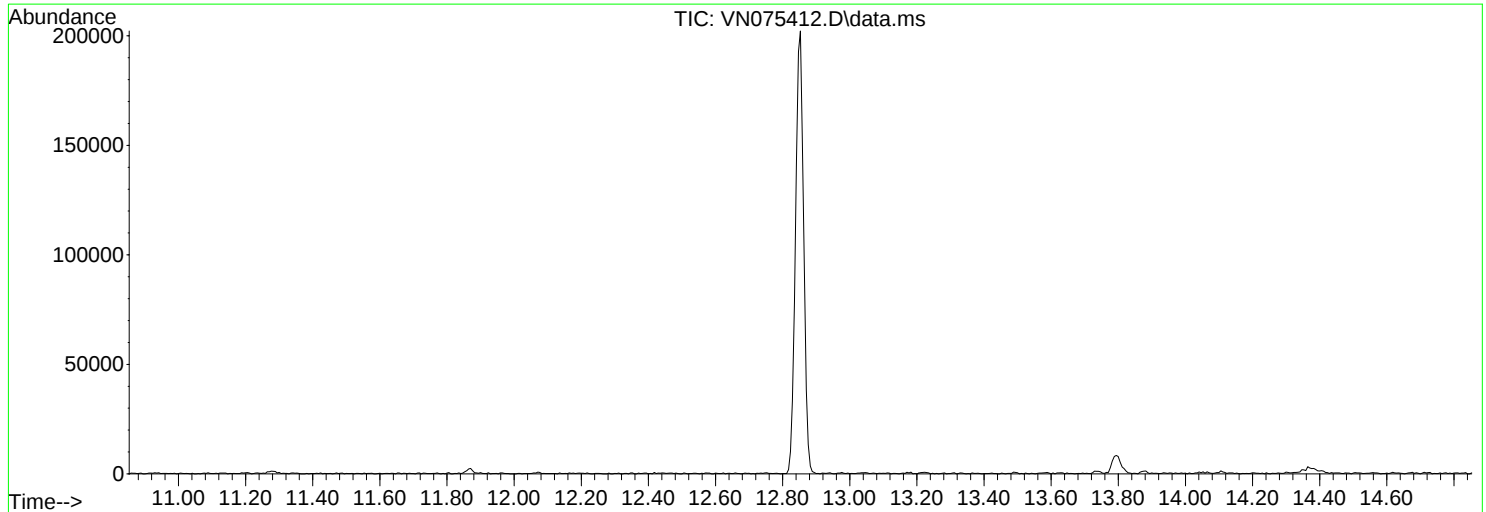

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	6706	PASS
75	95	30	60	52.5	19503	PASS
95	95	100	100	100.0	37157	PASS
96	95	5	9	7.0	2604	PASS
173	174	0.00	2	1.3	393	PASS
174	95	50	100	82.2	30557	PASS
175	174	5	9	8.8	2681	PASS
176	174	95	101	95.5	29192	PASS
177	176	5	9	6.7	1944	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	304	50.00	6706	69.00	4015	79.90	401
37.05	1713	51.05	1977	70.00	291	80.90	161
38.05	1441	55.95	543	71.80	66	81.85	34
39.05	584	57.05	1017	72.10	64	87.05	143
40.05	111	60.00	300	73.00	1603	88.05	1543
43.95	480	61.05	1783	74.05	6574	90.95	224
44.95	309	61.95	1801	75.05	19503	92.00	1281
46.90	192	63.05	1467	76.00	1700	93.05	1704
47.10	111	63.95	226	77.00	212	94.05	4851
47.90	139	66.90	55	78.00	134	95.05	37157
49.05	1395	68.00	3729	78.90	1602	96.05	2604

Average of 12.847 to 12.859 min.: VN075412.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.80	76	142.85	493				
104.00	75	148.00	51				
105.85	134	171.95	174				
115.90	52	172.80	125				
116.90	288	173.10	393				
117.90	58	174.00	30557				
118.90	285	175.05	2681				
127.90	51	176.00	29192				
129.70	50	176.95	1944				
130.10	63						
140.95	483						

Instrument :

MSVOA_N

ClientSampleId :

BFB