

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112524\
 Data File : VN085028.D
 Acq On : 25 Nov 2024 14:02
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Nov 26 07:32:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N103124W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Nov 01 02:38:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.806	128	23409	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.094	114	118400	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.865	117	105610	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.571	65	58185	30.917	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	103.067%
60) 4-Bromofluorobenzene	12.847	95	43357	23.843	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	79.467%
63) Toluene-d8	10.565	98	138092	27.621	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	92.067%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112524\
Data File : VN085028.D
Acq On : 25 Nov 2024 14:02
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Nov 26 07:32:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N103124W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Nov 01 02:38:04 2024
Response via : Initial Calibration




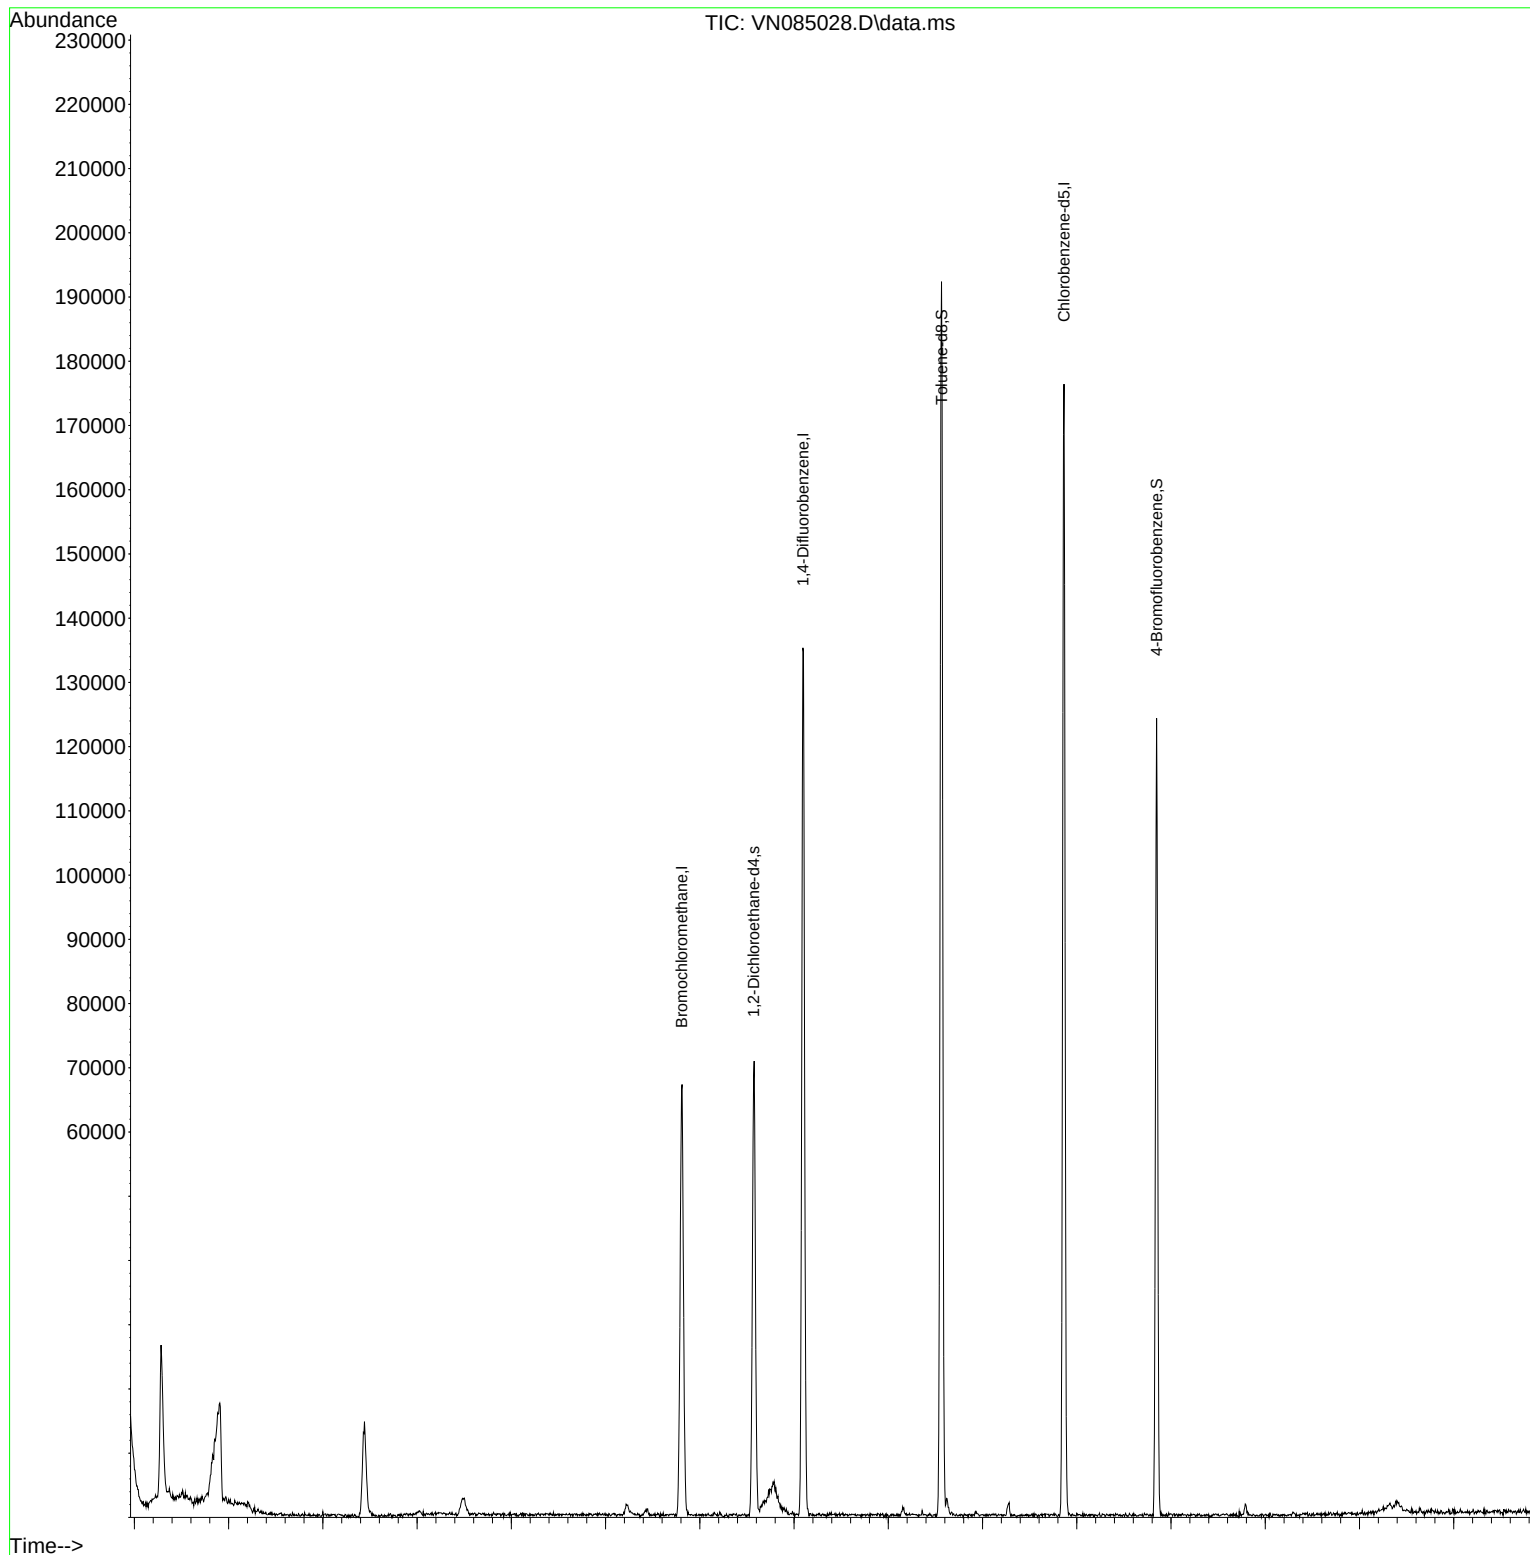


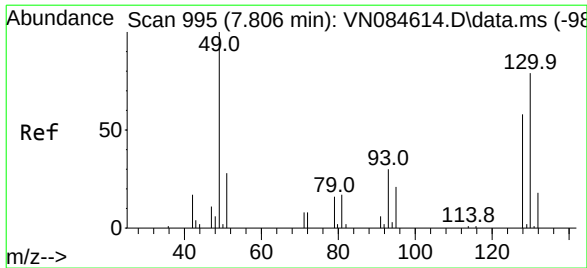

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.806 min Scan# 995
Delta R.T. 0.000 min
Lab File: VN085028.D
Acq: 25 Nov 2024 14:02




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion	Ratio	Lower	Upper
128	100		
49	168.3	0.0	427.0
130	129.2	0.0	322.2

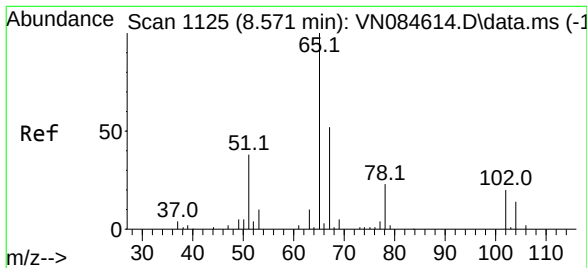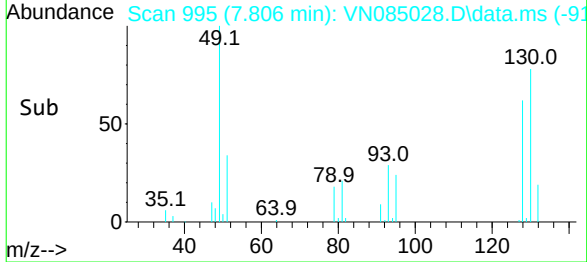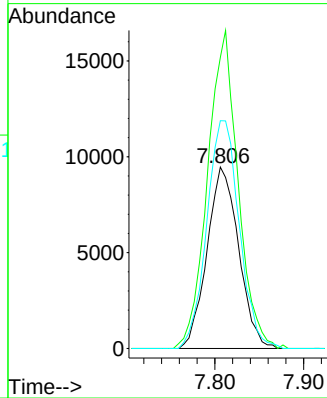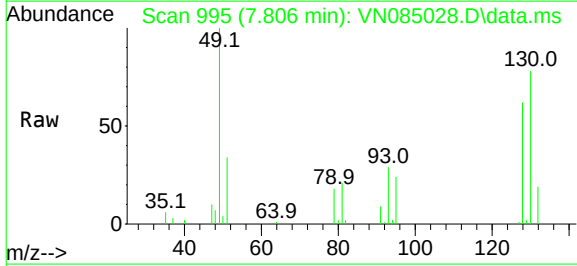

#27
1,2-Dichloroethane-d4
Concen: 30.917 ug/l
RT: 8.571 min Scan# 1125
Delta R.T. 0.000 min
Lab File: VN085028.D
Acq: 25 Nov 2024 14:02

Tgt Ion	Ratio	Lower	Upper
65	100		
67	52.7	40.7	61.1


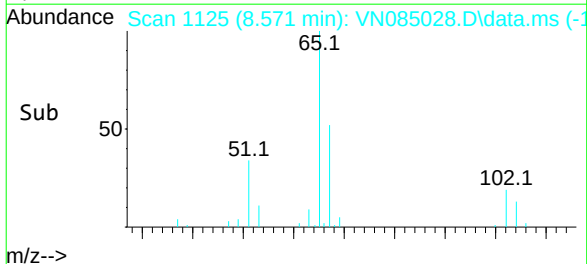
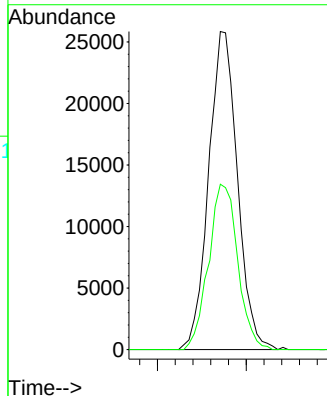
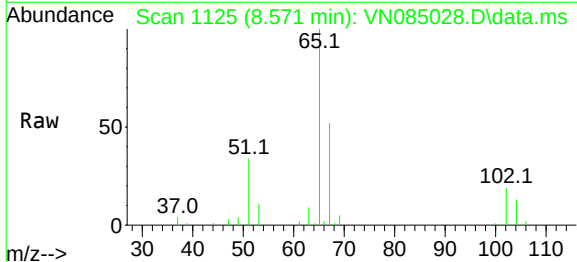


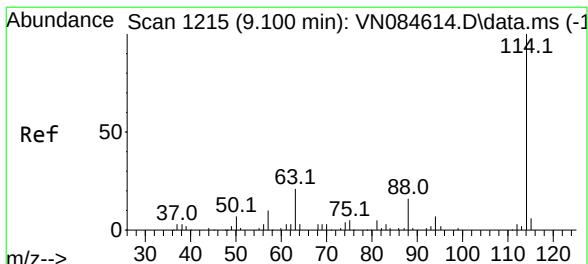

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 9.094 min Scan# 1214
 Delta R.T. -0.006 min
 Lab File: VN085028.D
 Acq: 25 Nov 2024 14:02




Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK


Tgt Ion:	114	Resp:	118400
Ion	Ratio	Lower	Upper
114	100		
63	20.6	16.8	25.2
88	16.0	12.9	19.3

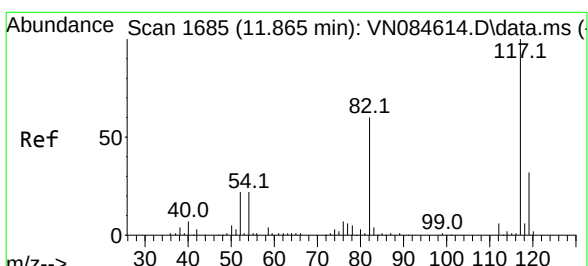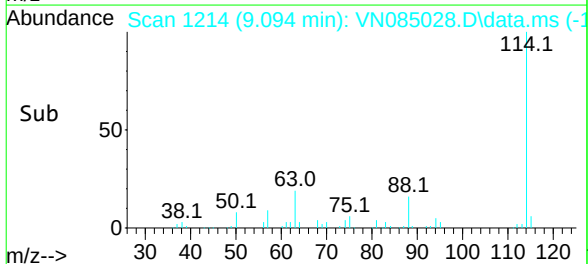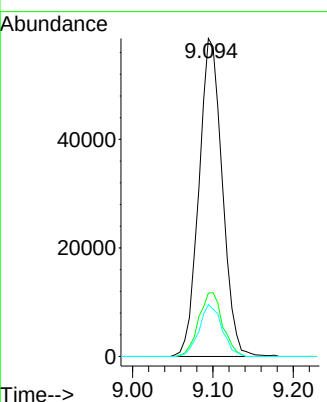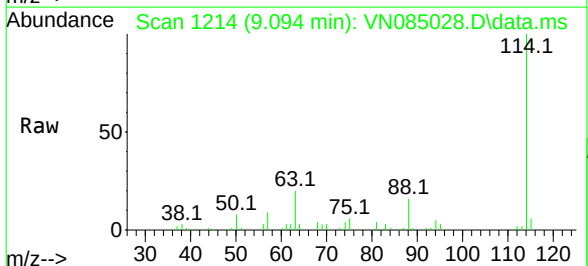

#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 11.865 min Scan# 1685
 Delta R.T. 0.000 min
 Lab File: VN085028.D
 Acq: 25 Nov 2024 14:02


Tgt Ion:	117	Resp:	105610
Ion	Ratio	Lower	Upper
117	100		
82	55.0	45.5	68.3
119	30.9	25.3	37.9

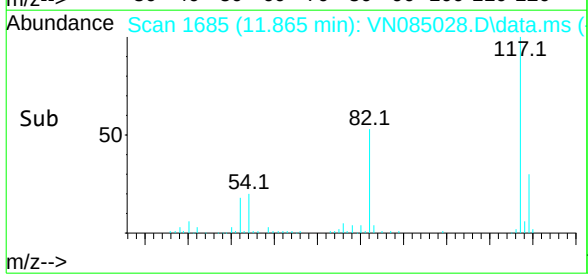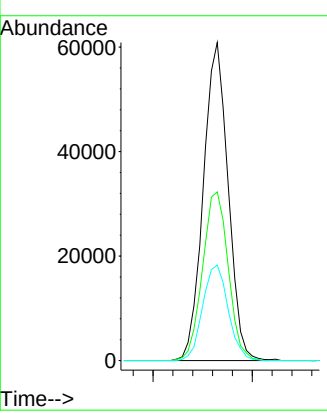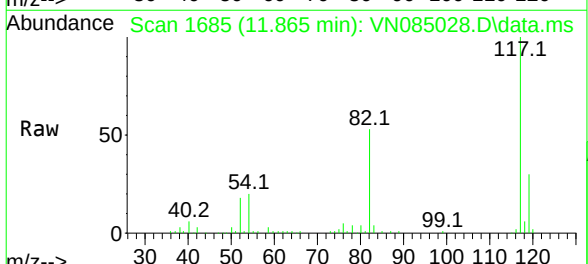



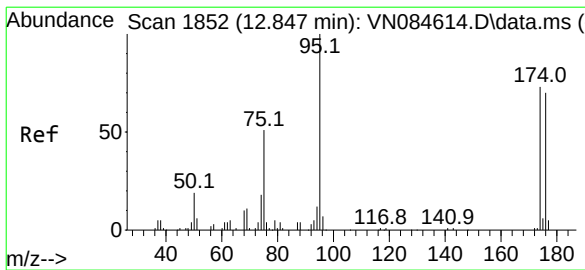


#60
4-Bromofluorobenzene
Concen: 23.843 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN085028.D
Acq: 25 Nov 2024 14:02

Instrument :
MSVOA_N
ClientSampleId :
IBLK

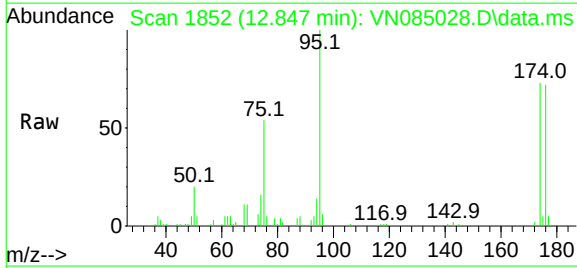

Tgt Ion: 95 Resp: 43357
Ion Ratio Lower Upper
95 100
174 74.6 59.6 89.4
176 69.5 58.6 88.0

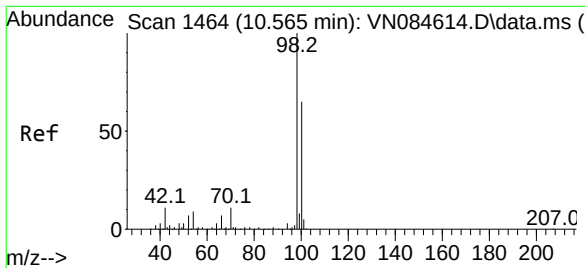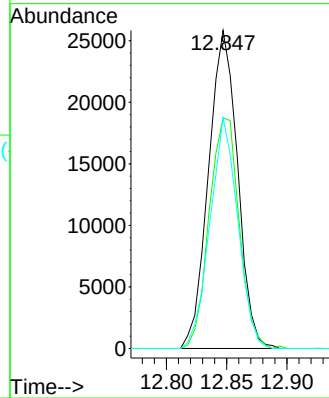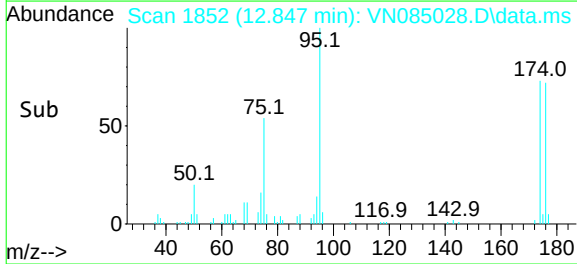

#63
Toluene-d8
Concen: 27.621 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN085028.D
Acq: 25 Nov 2024 14:02

Tgt Ion: 98 Resp: 138092
Ion Ratio Lower Upper
98 100
100 64.5 52.2 78.2

