


Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_N\DATA\VN112618\  
Data File : VN052454.D  
Acq On : 26 Nov 2018 12:14  
Operator : MD\SY  
Sample : BFB  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 28

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\624N112618W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Tue Nov 27 00:48:33 2018

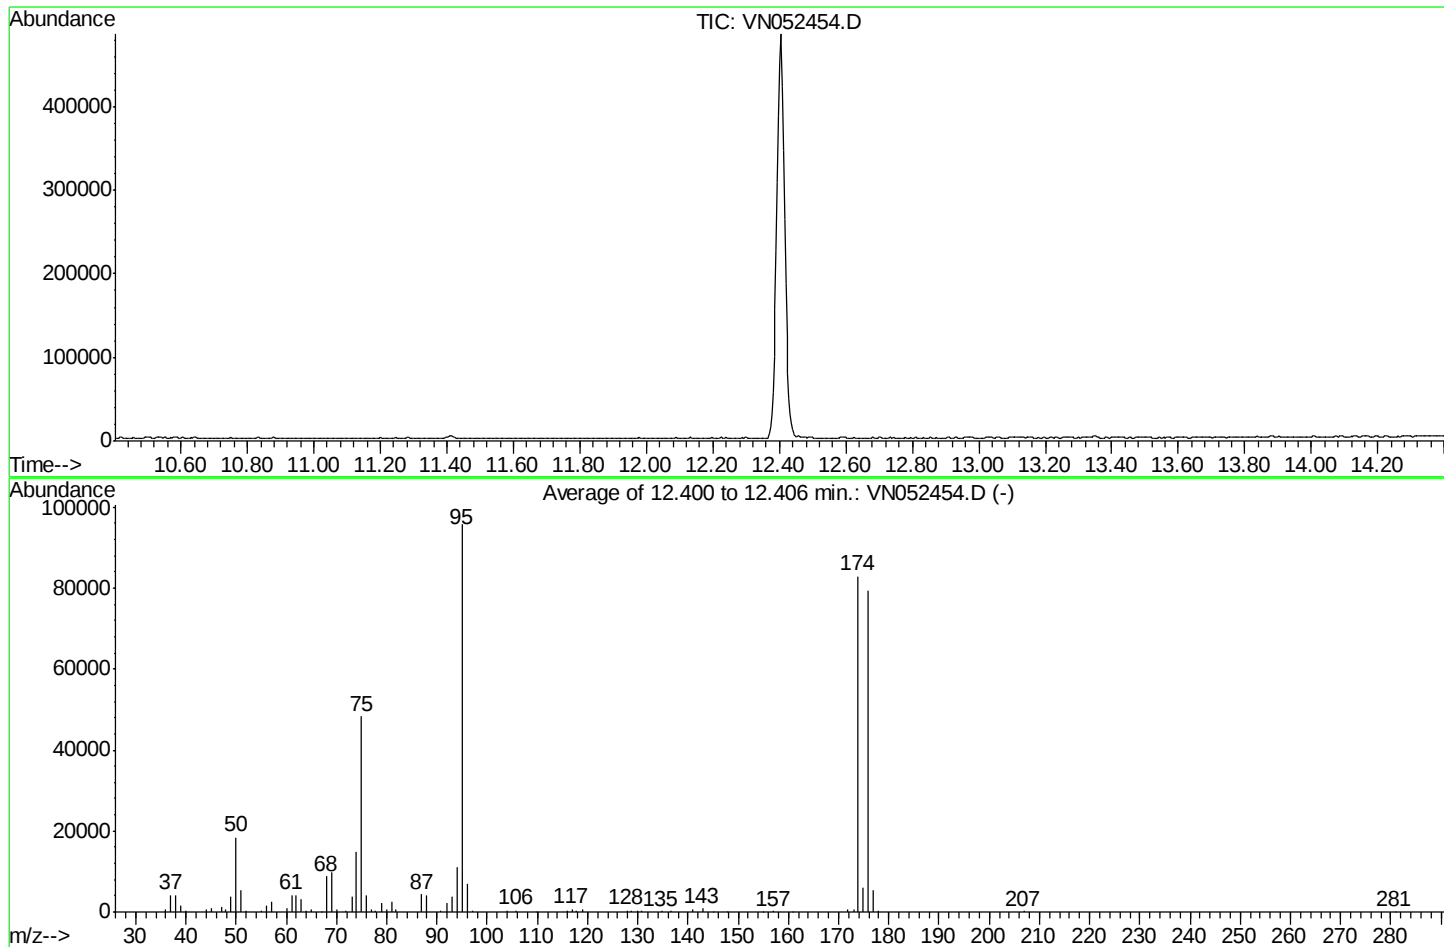

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.2      | 18402   | PASS             |
| 75          | 95           | 30           | 60           | 50.4      | 48253   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 95762   | PASS             |
| 96          | 95           | 5            | 9            | 7.1       | 6843    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.0       | 799     | PASS             |
| 174         | 95           | 50           | 100          | 86.6      | 82922   | PASS             |
| 175         | 174          | 5            | 9            | 7.2       | 5995    | PASS             |
| 176         | 174          | 95           | 101          | 95.9      | 79525   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 5265    | PASS             |