


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN112619\
Data File : VN059398.D
Acq On : 26 Nov 2019 9:22
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112019W.M
Title : SW846 8260
Last Update : Thu Nov 21 08:44:45 2019

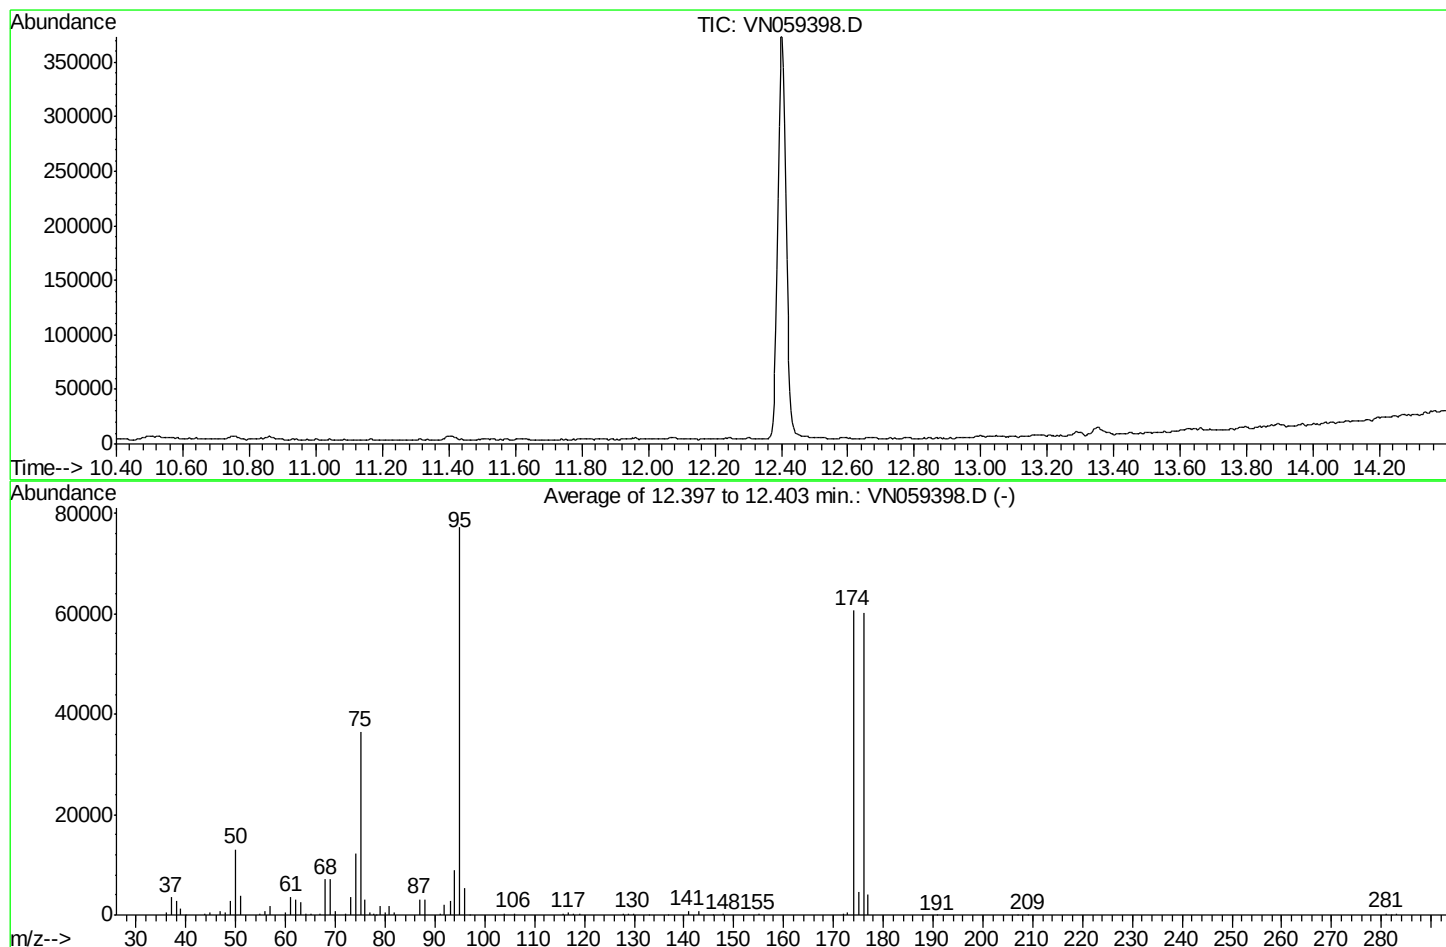

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	13060	PASS
75	95	30	60	47.4	36589	PASS
95	95	100	100	100.0	77256	PASS
96	95	5	9	6.9	5346	PASS
173	174	0.00	2	0.8	490	PASS
174	95	50	100	78.5	60629	PASS
175	174	5	9	7.5	4548	PASS
176	174	95	101	99.4	60258	PASS
177	176	5	9	6.9	4165	PASS