
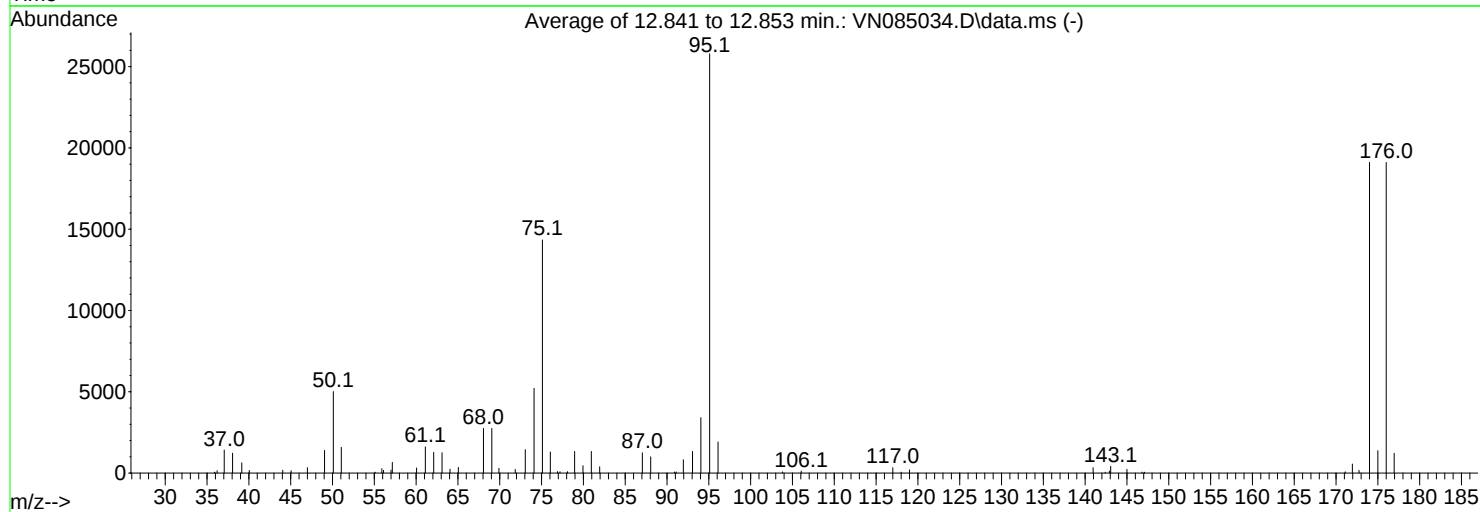


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112624\
Data File : VN085034.D
Acq On : 26 Nov 2024 08:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

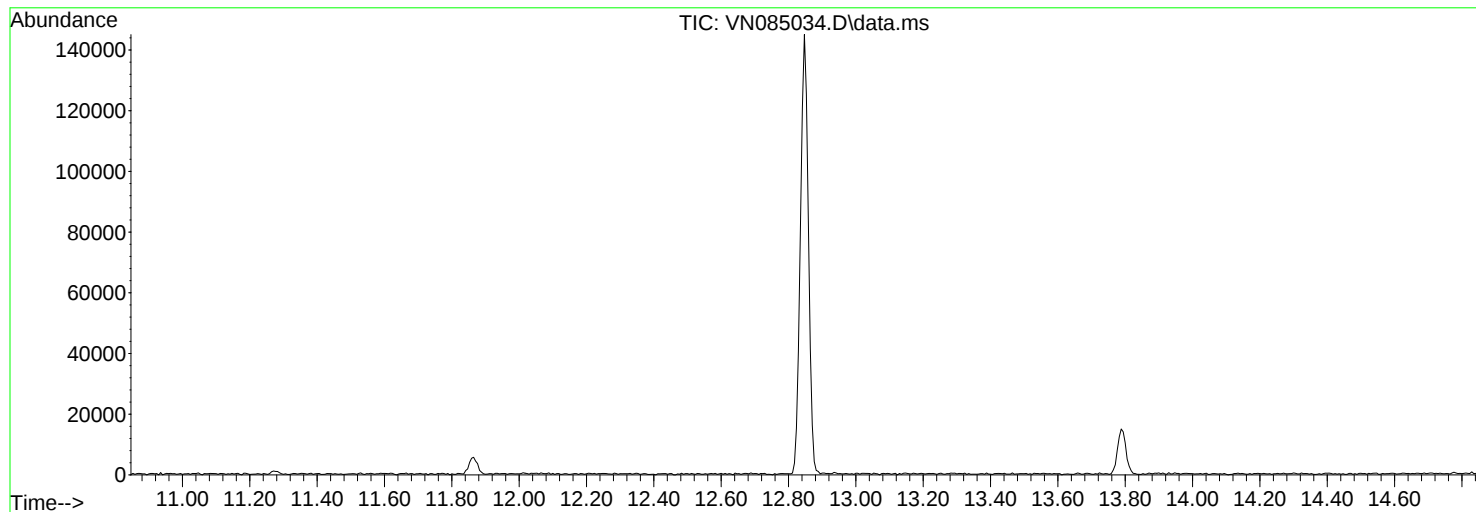

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	5016	PASS
75	95	30	60	55.6	14340	PASS
95	95	100	100	100.0	25792	PASS
96	95	5	9	7.4	1916	PASS
173	174	0.00	2	0.9	167	PASS
174	95	50	100	74.1	19109	PASS
175	174	5	9	7.2	1379	PASS
176	174	95	101	100.0	19109	PASS
177	176	5	9	6.4	1218	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	58	51.05	1584	65.05	349	78.10	89
36.20	149	55.10	57	68.05	2745	78.95	1332
37.05	1416	55.90	273	69.05	2748	79.95	455
38.05	1222	56.10	165	69.90	298	80.95	1335
39.15	631	57.00	184	71.85	223	81.95	387
40.05	166	57.15	655	73.05	1443	87.05	1249
44.05	176	60.05	314	74.10	5212	88.05	998
45.05	148	61.10	1616	75.10	14340	90.90	69
47.00	333	62.10	1275	76.05	1300	91.10	72
49.05	1392	63.10	1252	76.90	94	91.95	822
50.10	5016	64.05	243	77.20	83	93.05	1334

Average of 12.841 to 12.853 min.: VN085034.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	3406	143.05	415				
95.10	25792	145.00	231				
96.10	1916	146.80	61				
103.80	78	147.10	54				
106.05	121	171.10	76				
117.00	329	171.95	557				
118.00	57	172.75	167				
119.00	198	174.00	19109				
140.95	334	175.00	1379				
142.40	57	176.00	19109				
142.90	126	176.95	1218				

Instrument :

MSVOA_N

ClientSampleId :

BFB