



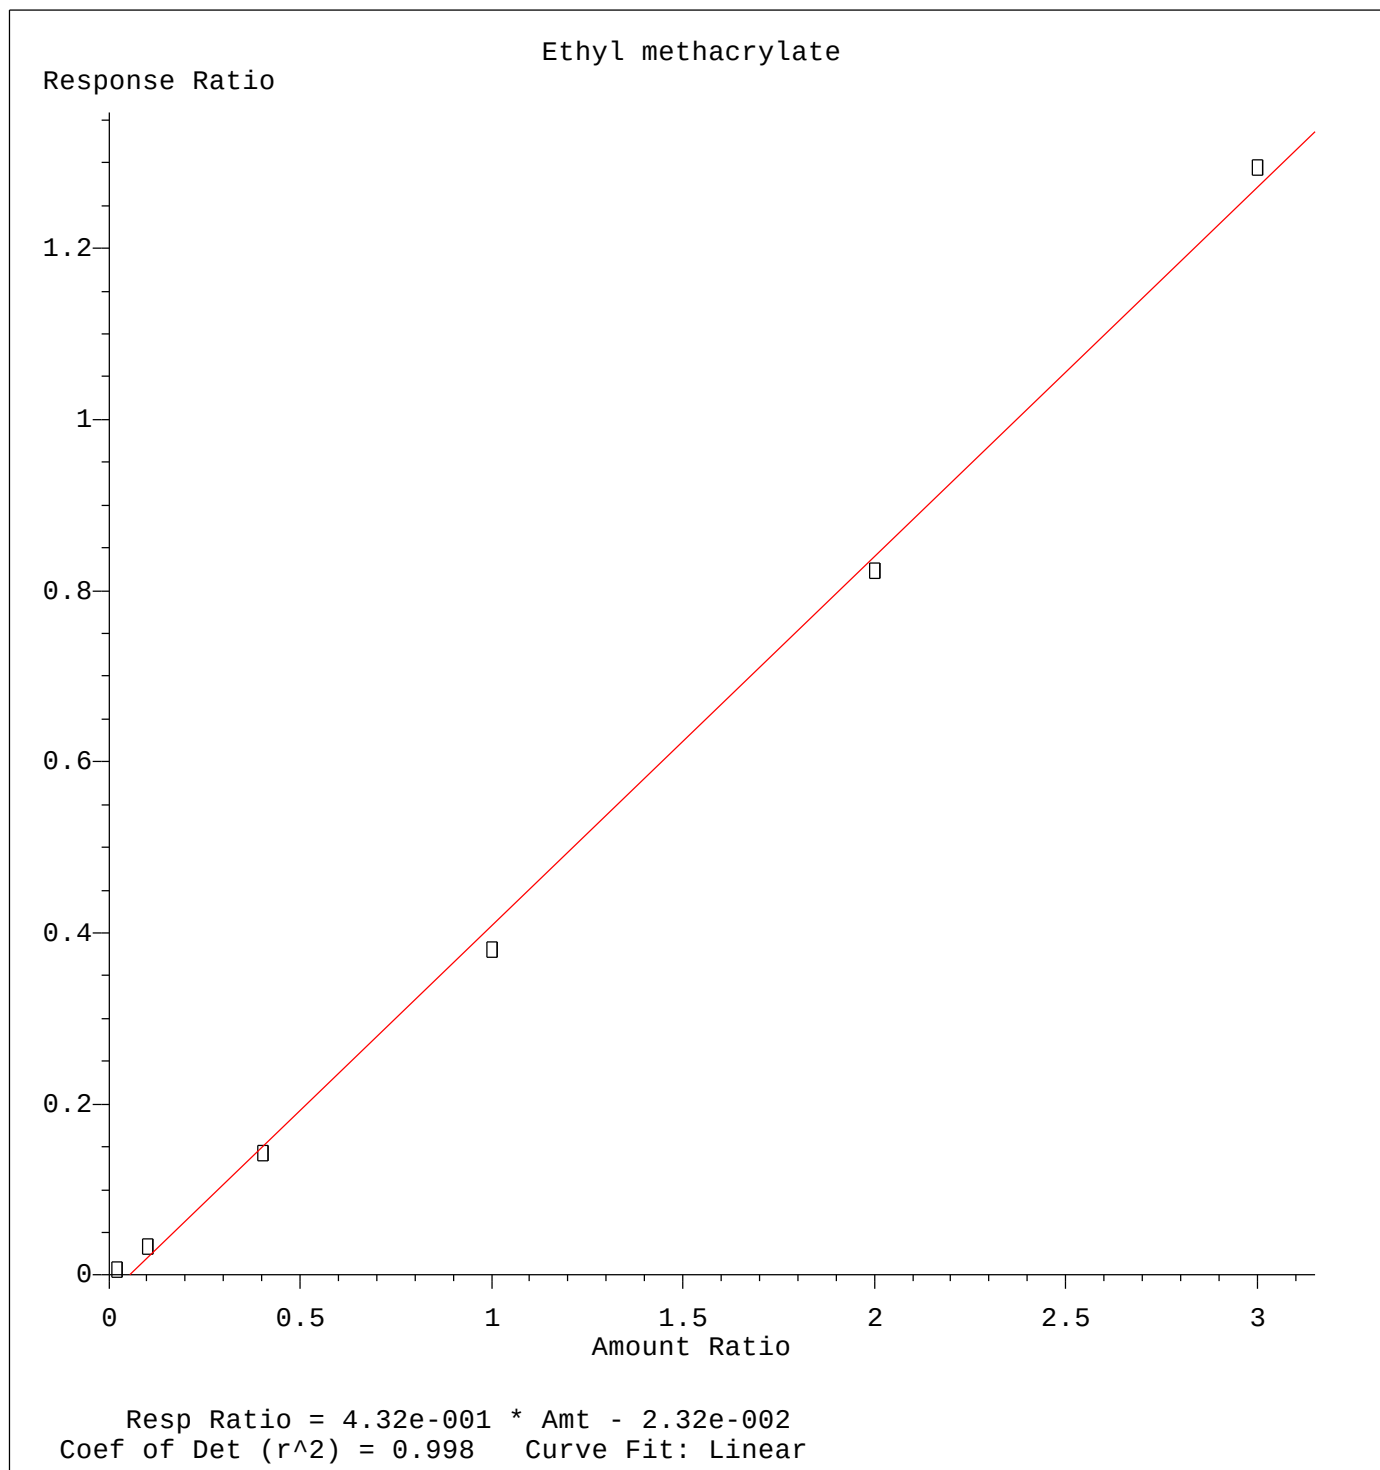


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Calibration Table Last Updated: Wed Nov 28 01:11:38 2018

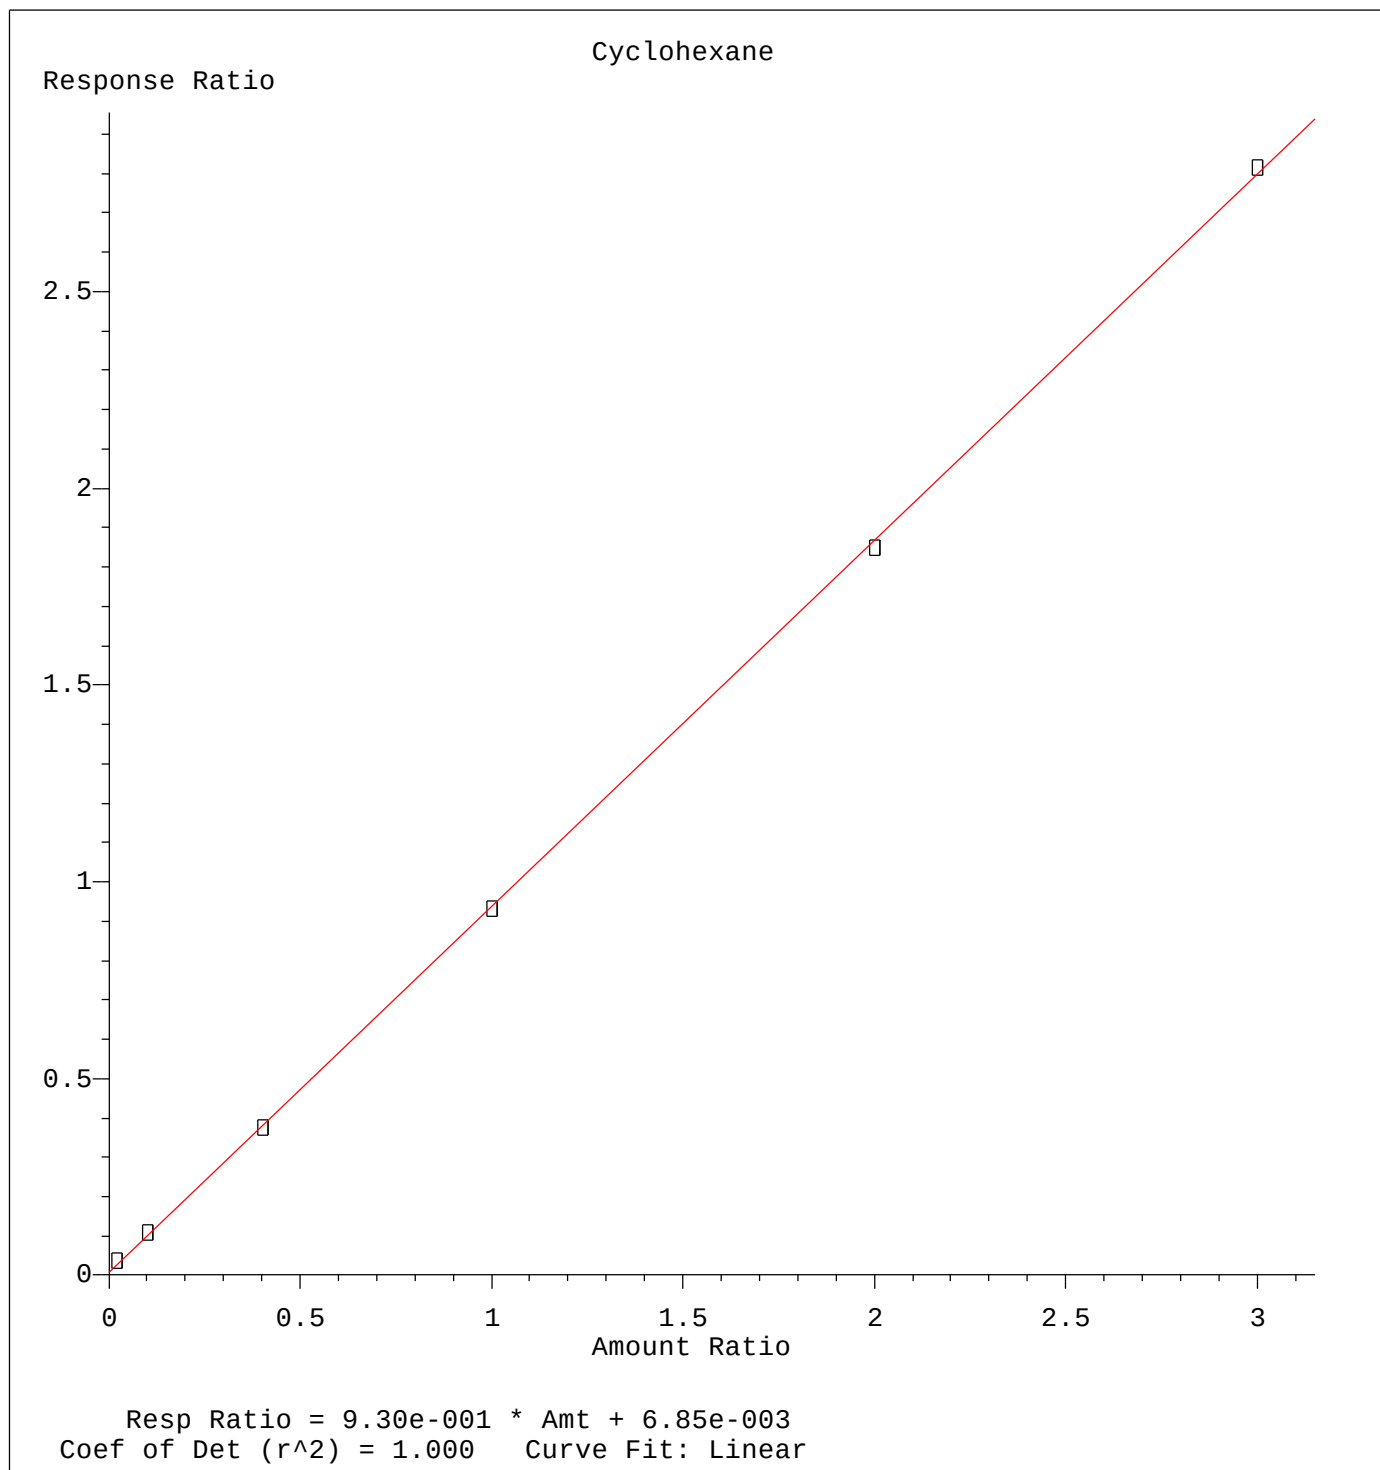

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Calibration Table Last Updated: Wed Nov 28 01:11:38 2018

1,2,3-Trichlorobenzene

Response Ratio

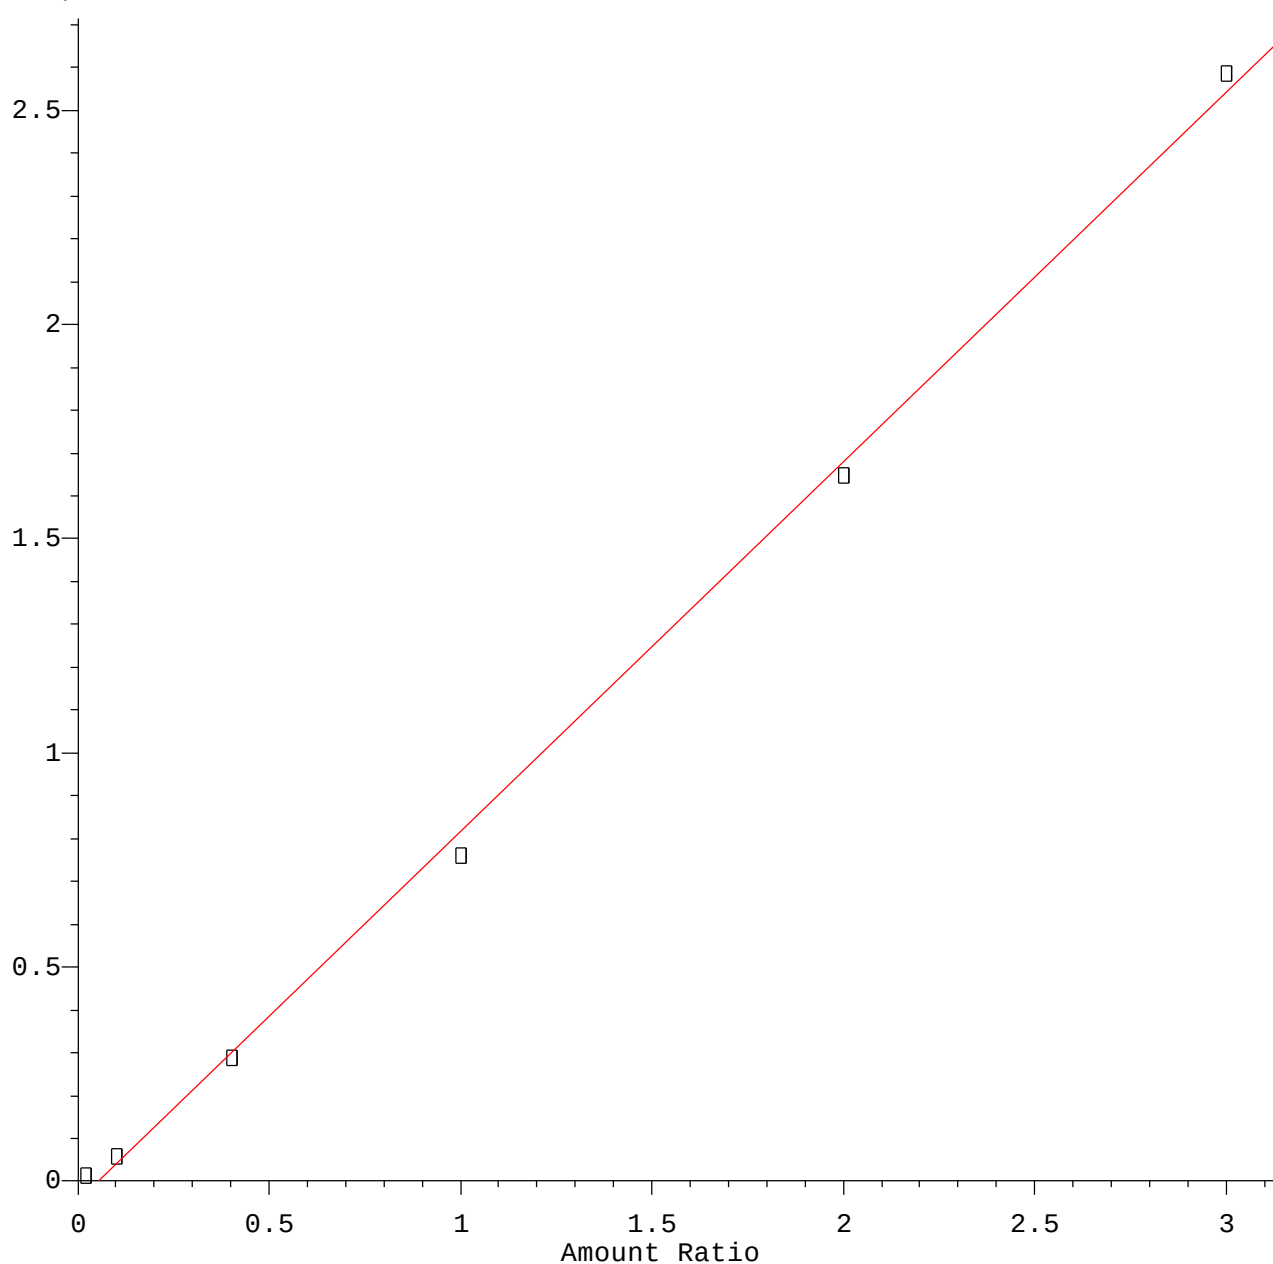


Resp Ratio = $8.63 \times 10^{-1} \times \text{Amt} - 4.71 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Calibration Table Last Updated: Wed Nov 28 01:11:38 2018

Naphthalene

Response Ratio

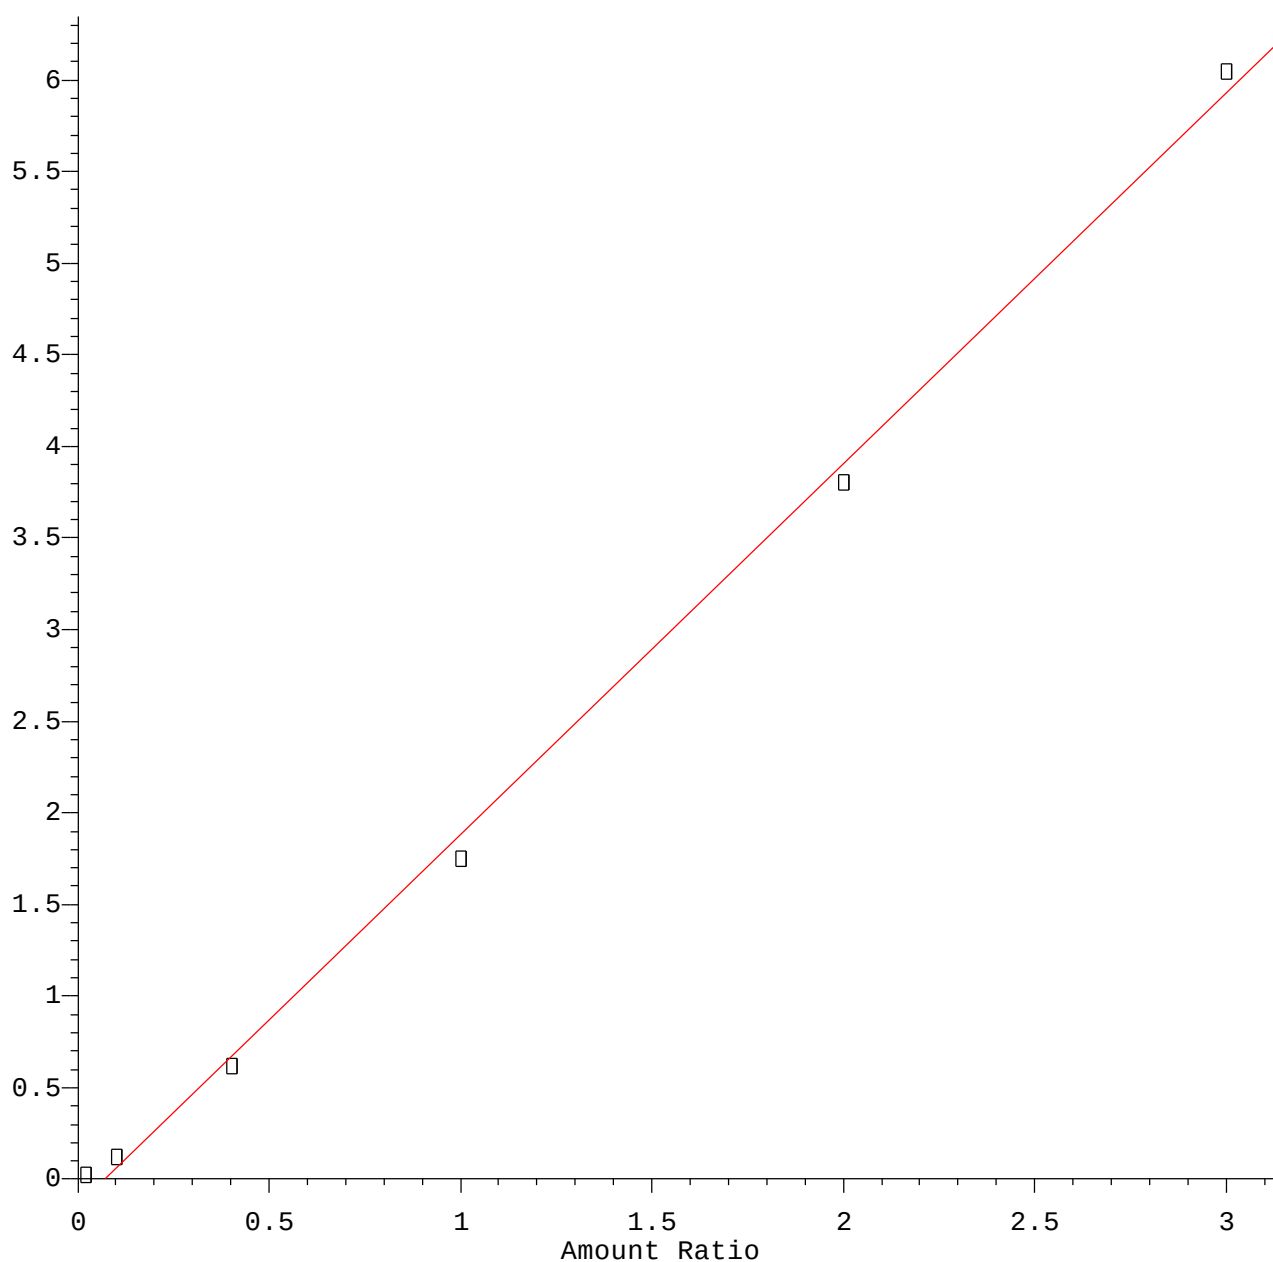


Resp Ratio = 2.02e+000 * Amt - 1.39e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Calibration Table Last Updated: Wed Nov 28 01:11:38 2018

1,2,4-Trichlorobenzene

Response Ratio

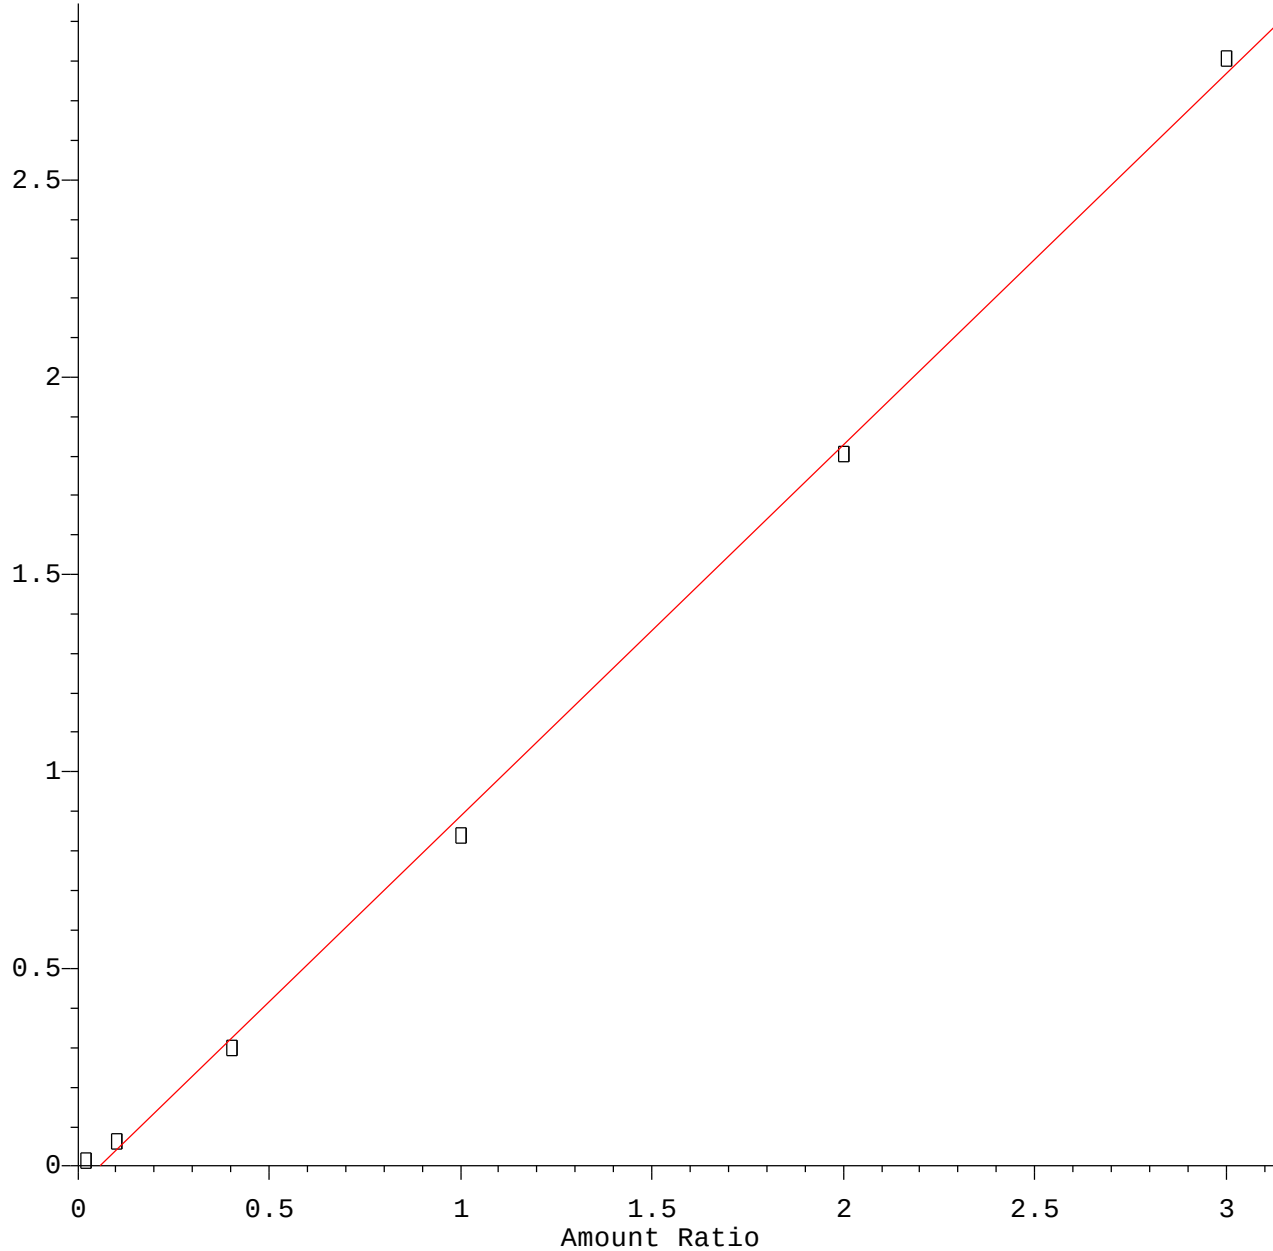

Resp Ratio = $9.41 \times 10^{-1} \times \text{Amt} - 5.32 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Calibration Table Last Updated: Wed Nov 28 01:11:38 2018