


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN112718\
 Data File : VN052491.D
 Acq On : 27 Nov 2018 20:46
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 26 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N112618W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Nov 27 00:48:33 2018

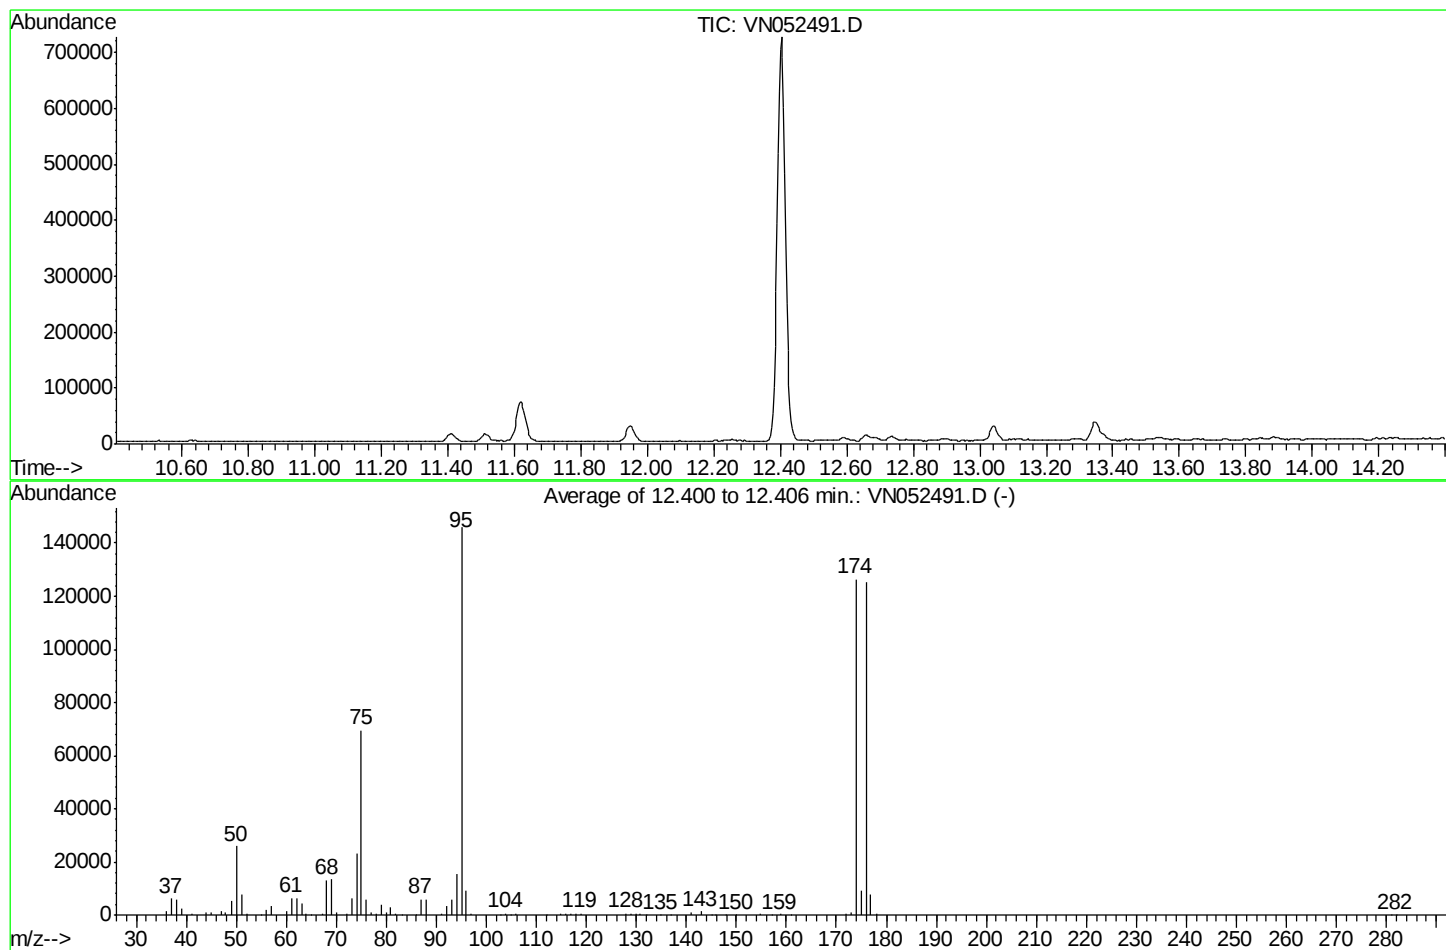

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	25981	PASS
75	95	30	60	47.7	69616	PASS
95	95	100	100	100.0	145941	PASS
96	95	5	9	6.4	9293	PASS
173	174	0.00	2	0.8	972	PASS
174	95	50	100	86.7	126501	PASS
175	174	5	9	7.2	9124	PASS
176	174	95	101	99.1	125394	PASS
177	176	5	9	6.3	7856	PASS