


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN112719\
Data File : VN059416.D
Acq On : 27 Nov 2019 9:17
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112719W.M
Title : SW846 8260
Last Update : Wed Nov 27 16:56:05 2019

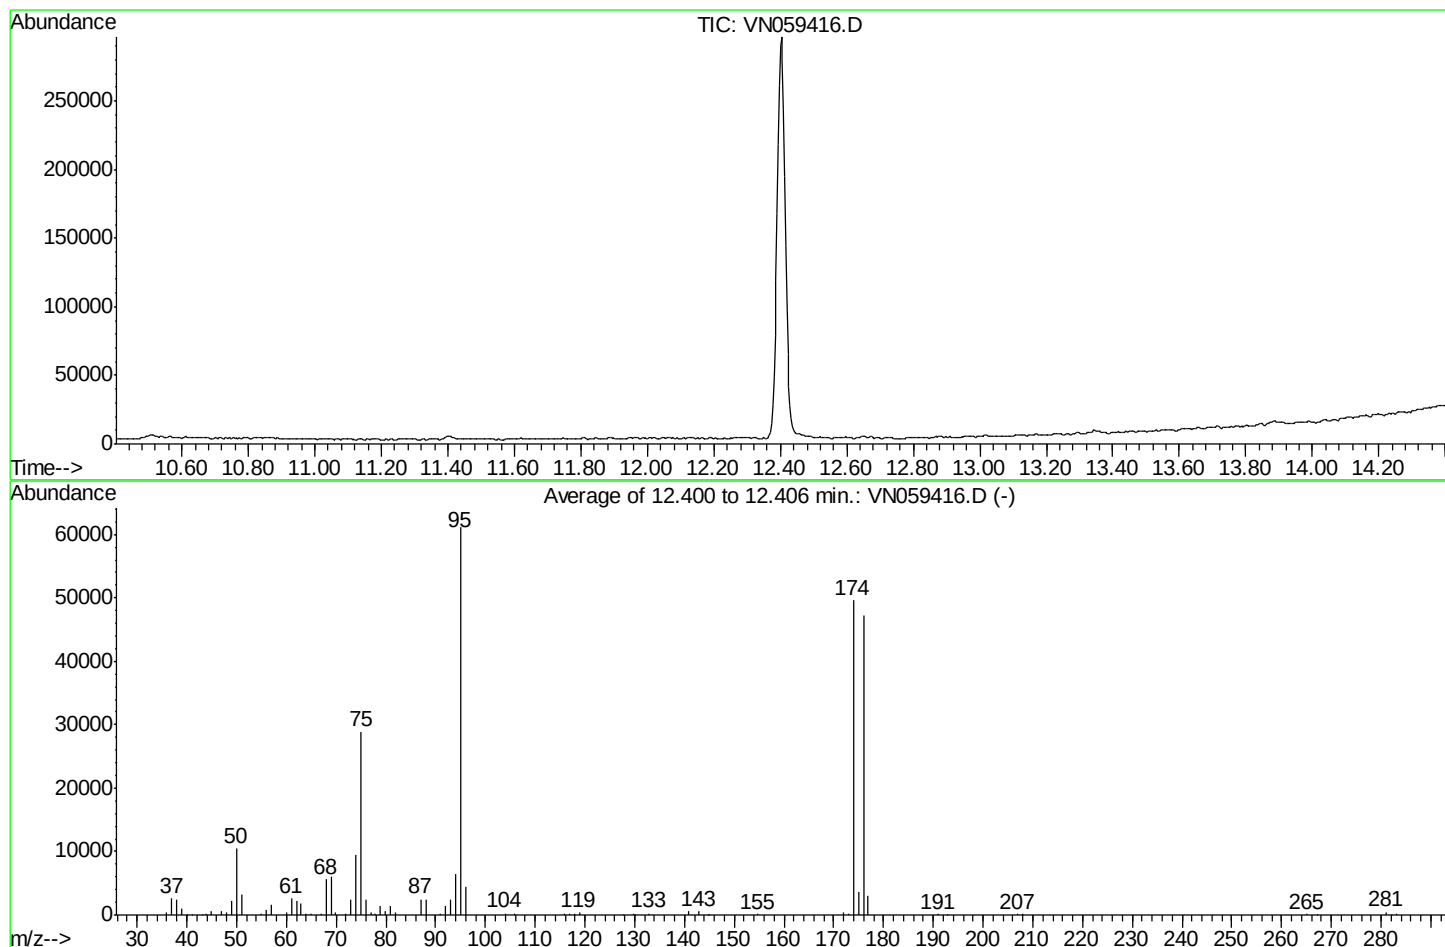

Spectrum Information: Average of 12.400 to 12.406 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	10463	PASS
75	95	30	60	47.4	28957	PASS
95	95	100	100	100.0	61114	PASS
96	95	5	9	7.3	4467	PASS
173	174	0.00	2	0.5	269	PASS
174	95	50	100	81.1	49562	PASS
175	174	5	9	7.3	3632	PASS
176	174	95	101	95.4	47285	PASS
177	176	5	9	6.3	2997	PASS