


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN112719\  
Data File : VN059416.D  
Acq On : 27 Nov 2019 9:17  
Operator : JC/SP  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N112719W.M  
Title : SW846 8260  
Last Update : Wed Nov 27 16:56:05 2019

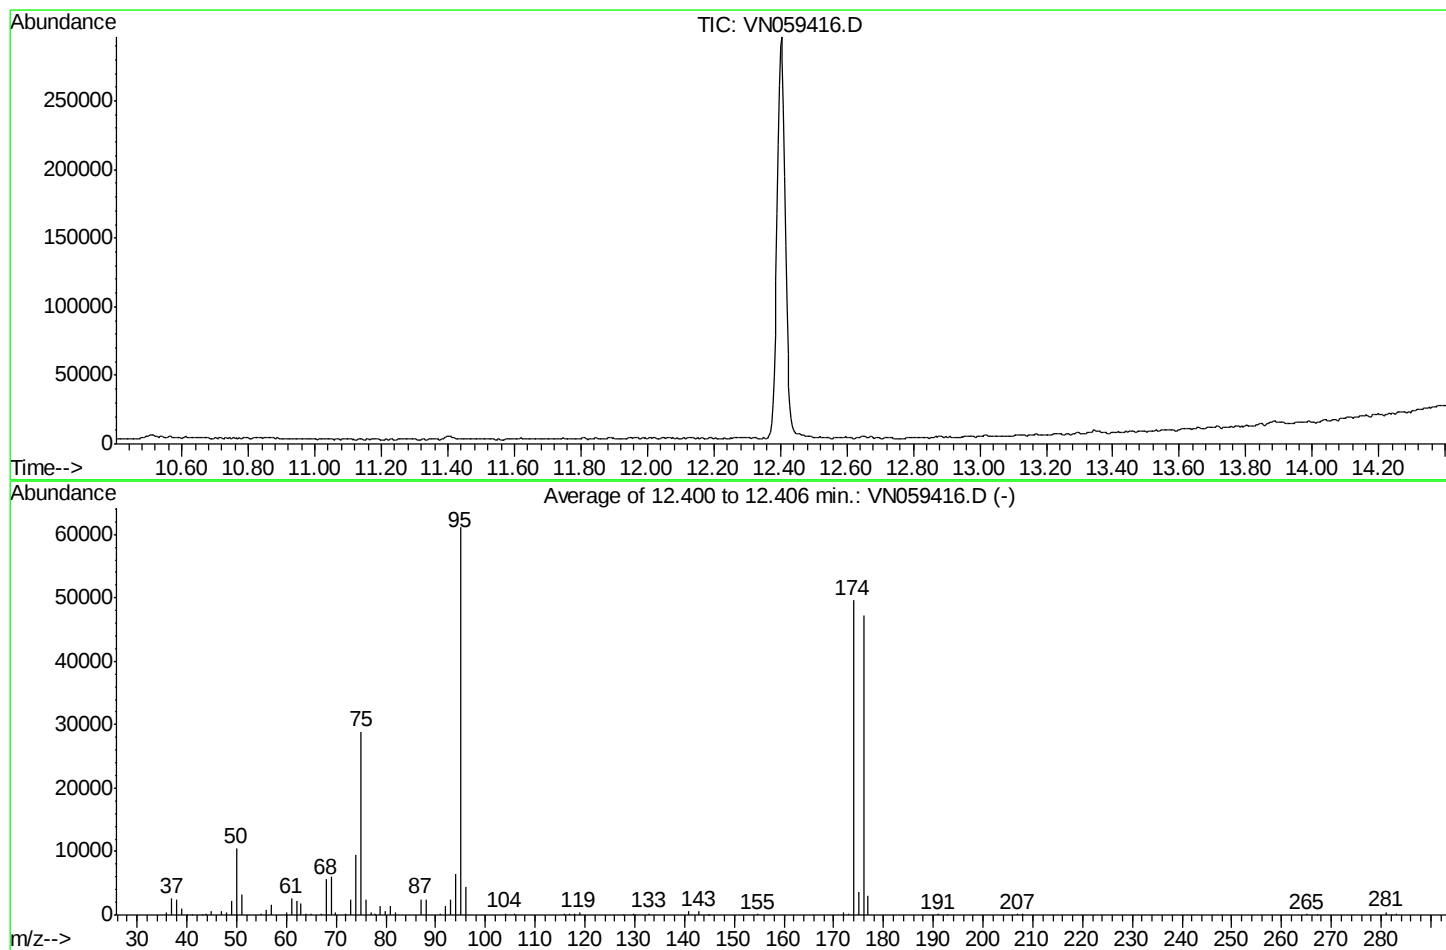

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.1      | 10463   | PASS             |
| 75          | 95           | 30           | 60           | 47.4      | 28957   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 61114   | PASS             |
| 96          | 95           | 5            | 9            | 7.3       | 4467    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.5       | 269     | PASS             |
| 174         | 95           | 50           | 100          | 81.1      | 49562   | PASS             |
| 175         | 174          | 5            | 9            | 7.3       | 3632    | PASS             |
| 176         | 174          | 95           | 101          | 95.4      | 47285   | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 2997    | PASS             |