


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN112719\
Data File : VN059434.D
Acq On : 27 Nov 2019 20:15
Operator : JC/SP
Sample : VSTDCCC050
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
LabSampleId :
VSTDCCC050

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112719W.M
Title : SW846 8260
Last Update : Wed Nov 27 16:56:05 2019

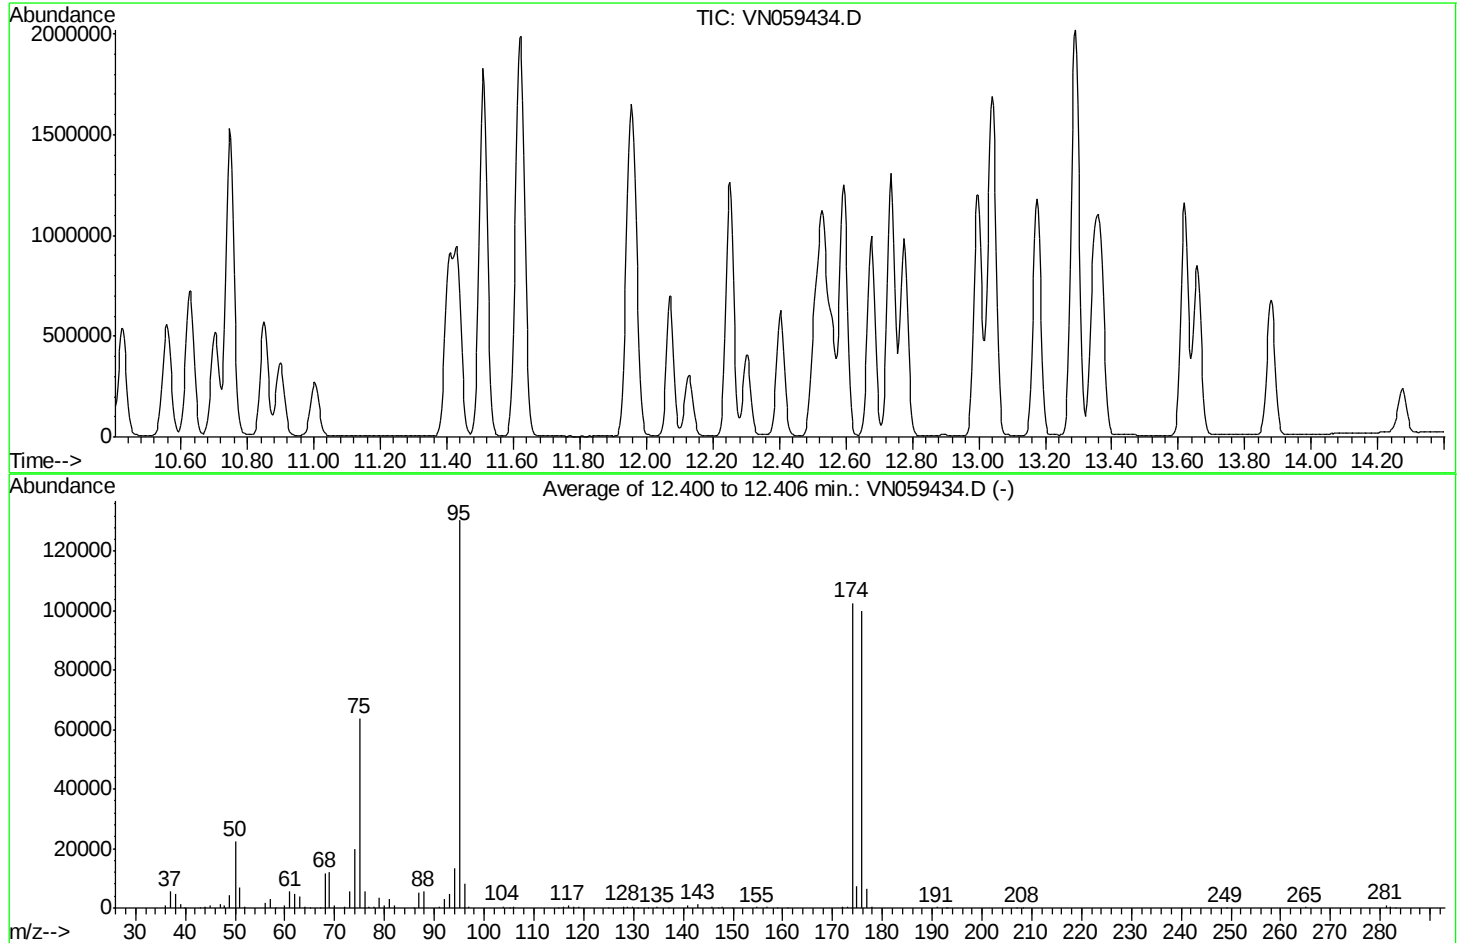

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	22341	PASS
75	95	30	60	48.7	63589	PASS
95	95	100	100	100.0	130466	PASS
96	95	5	9	6.4	8309	PASS
173	174	0.00	2	0.5	559	PASS
174	95	50	100	78.7	102656	PASS
175	174	5	9	7.1	7282	PASS
176	174	95	101	97.2	99800	PASS
177	176	5	9	6.6	6551	PASS