


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN112818\
Data File : VN052532.D
Acq On : 28 Nov 2018 21:14
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 29 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N112618W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Nov 27 00:48:33 2018

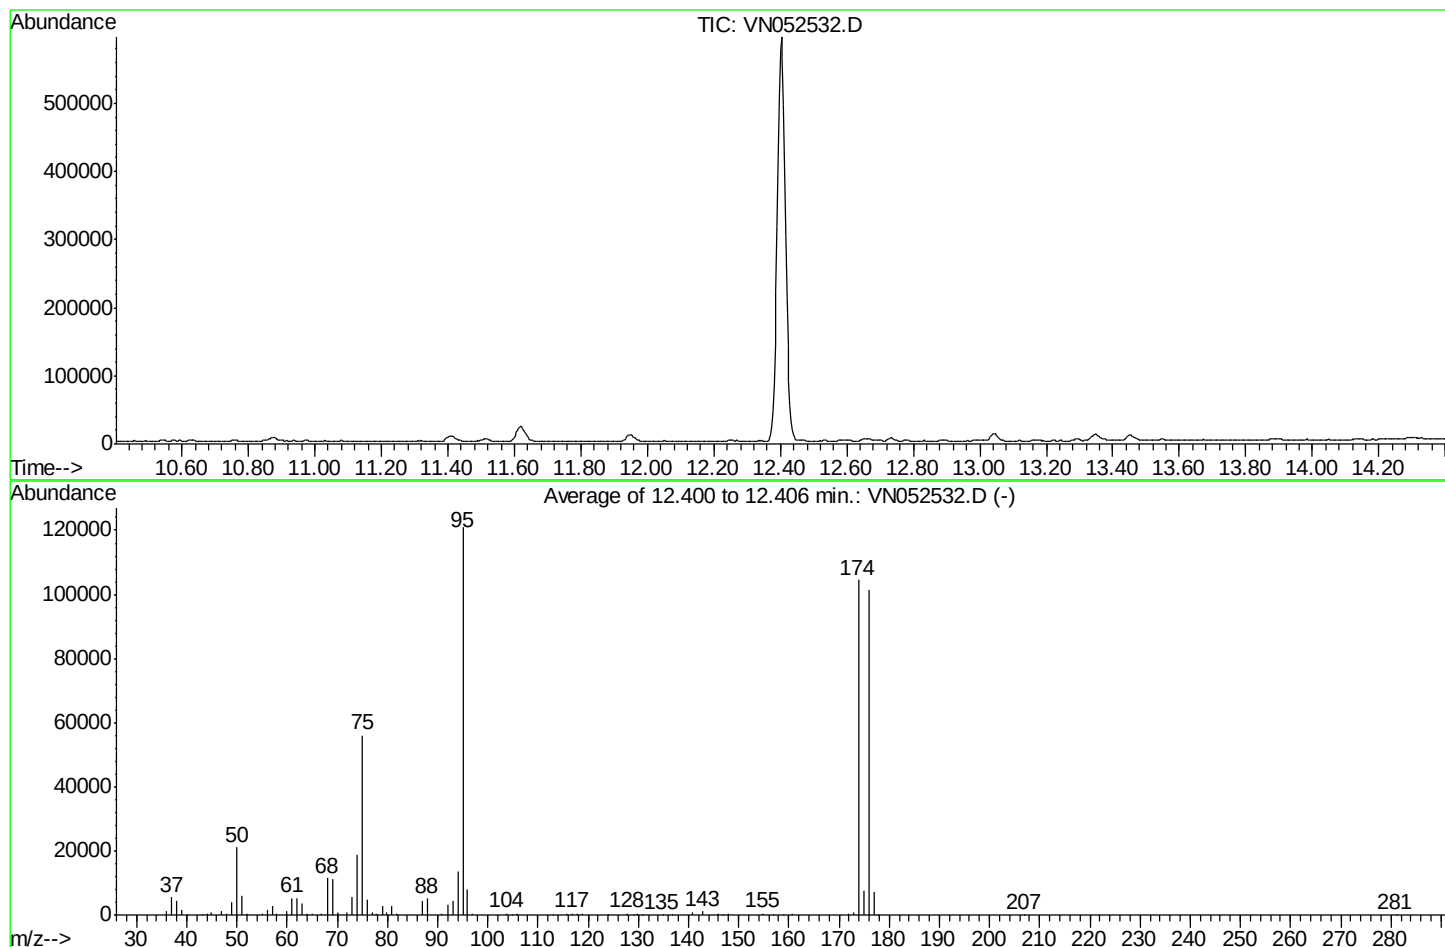

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	20976	PASS
75	95	30	60	46.3	56010	PASS
95	95	100	100	100.0	120922	PASS
96	95	5	9	6.7	8048	PASS
173	174	0.00	2	0.7	770	PASS
174	95	50	100	86.5	104568	PASS
175	174	5	9	7.1	7440	PASS
176	174	95	101	96.9	101309	PASS
177	176	5	9	7.1	7225	PASS