
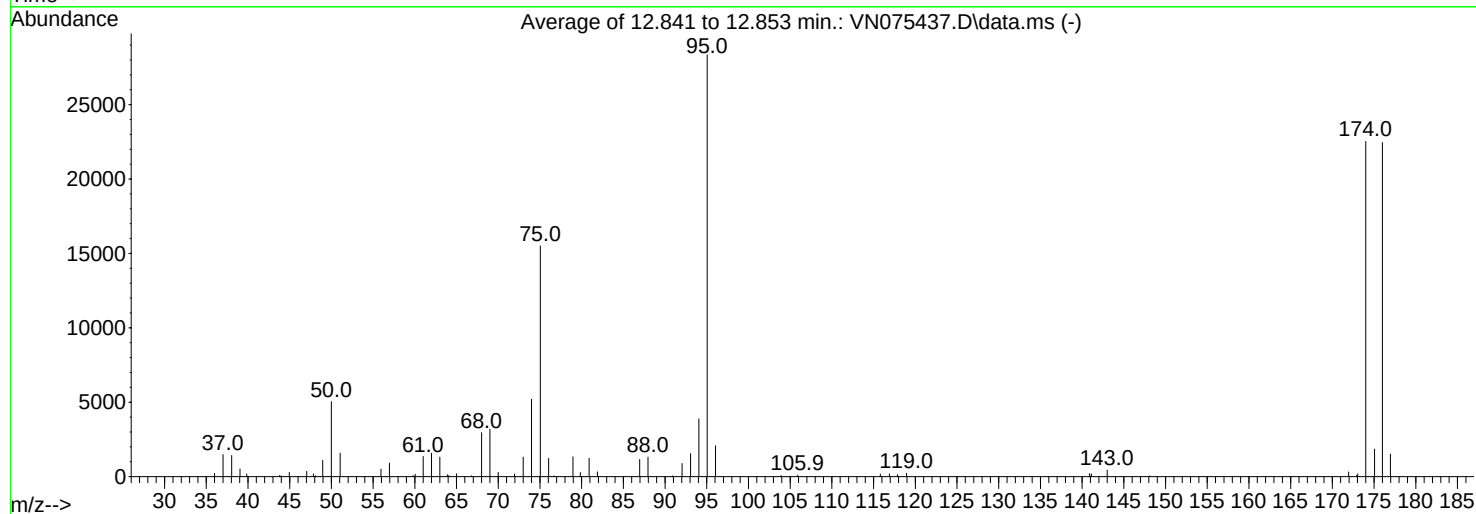


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112822\
Data File : VN075437.D
Acq On : 28 Nov 2022 10:02
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Title : SW846 8260
Last Update : Wed Nov 23 00:18:03 2022

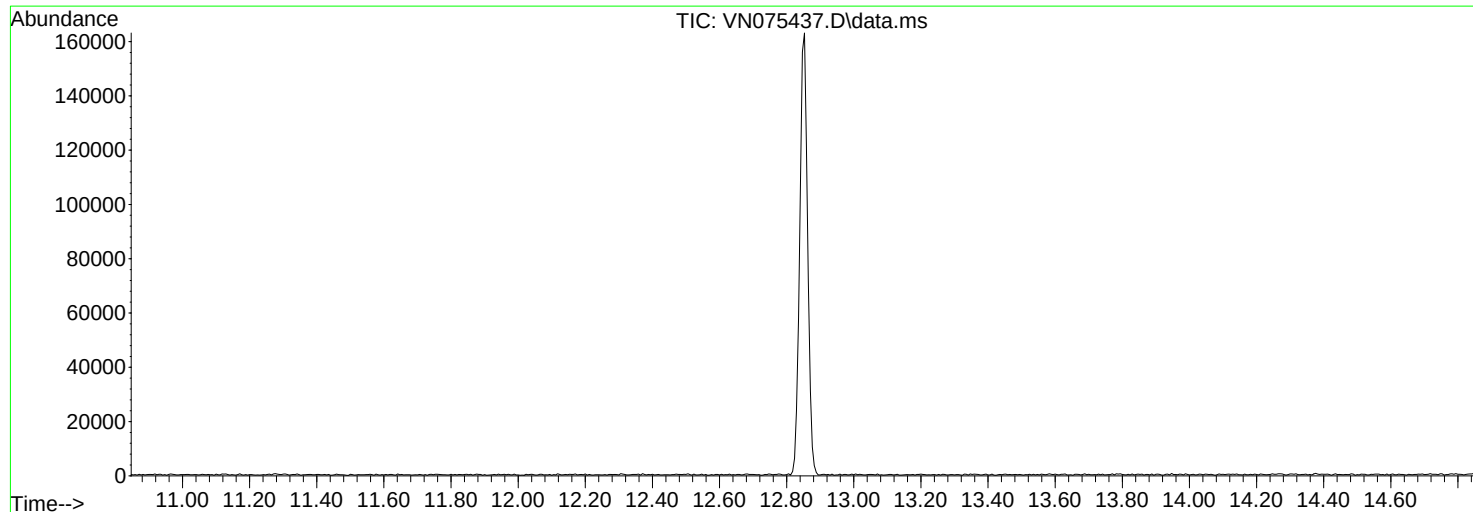

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	5045	PASS
75	95	30	60	54.7	15508	PASS
95	95	100	100	100.0	28347	PASS
96	95	5	9	7.3	2076	PASS
173	174	0.00	2	0.8	189	PASS
174	95	50	100	79.5	22531	PASS
175	174	5	9	8.2	1846	PASS
176	174	95	101	99.7	22456	PASS
177	176	5	9	6.8	1517	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	211	48.95	1095	64.10	73	76.70	51
37.00	1480	50.00	5045	65.00	189	78.95	133
38.05	1419	51.05	1577	66.80	56	79.85	28
39.05	515	55.95	503	68.00	2955	80.90	123
39.85	182	56.95	913	69.00	3191	81.90	323
43.80	90	59.80	71	70.00	287	86.95	1156
44.00	55	60.05	166	71.95	175	87.95	1317
44.95	293	61.00	1354	73.00	1307	90.90	53
47.05	357	62.00	1575	74.00	5209	92.05	886
47.85	179	63.00	1307	75.05	15508	93.05	1550
48.10	68	63.90	132	76.05	1237	94.05	3878

Average of 12.841 to 12.853 min.: VN075437.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.05	28347	148.10	50				
96.05	2076	171.95	316				
103.90	80	172.90	91				
105.90	106	173.05	189				
115.80	168	174.00	22531				
116.90	187	175.05	1846				
117.85	142	176.00	22456				
118.95	227	176.95	1517				
140.90	202						
141.10	186						
143.00	438						

Instrument :

MSVOA_N

ClientSampleId :

BFB