
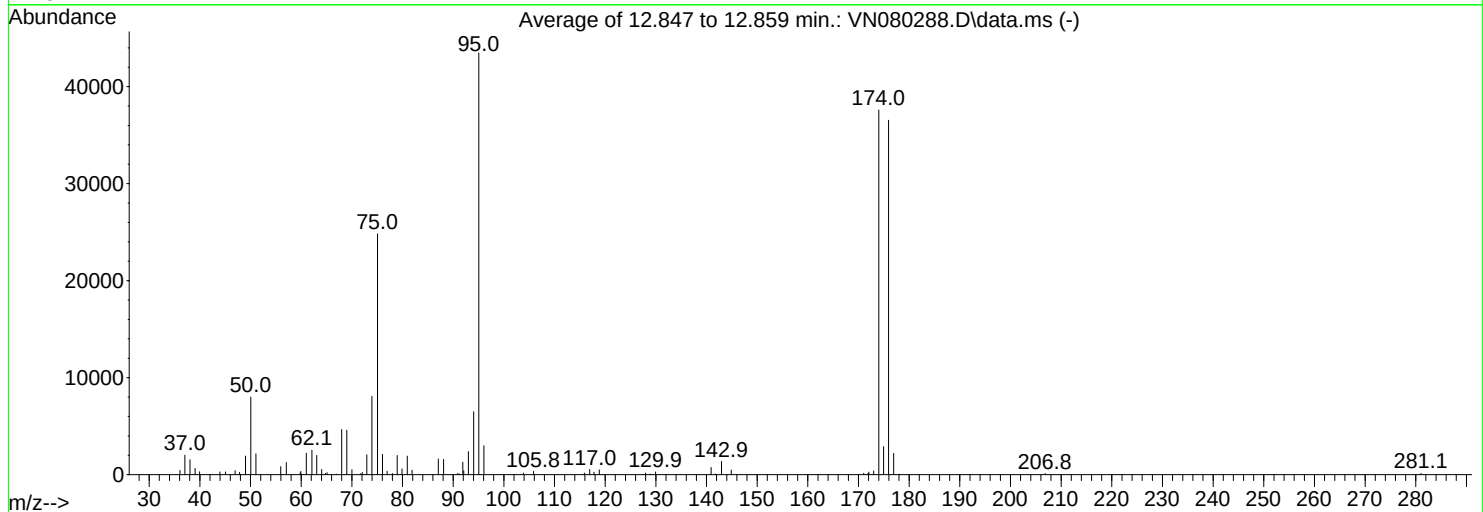


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112823\
Data File : VN080288.D
Acq On : 28 Nov 2023 10:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

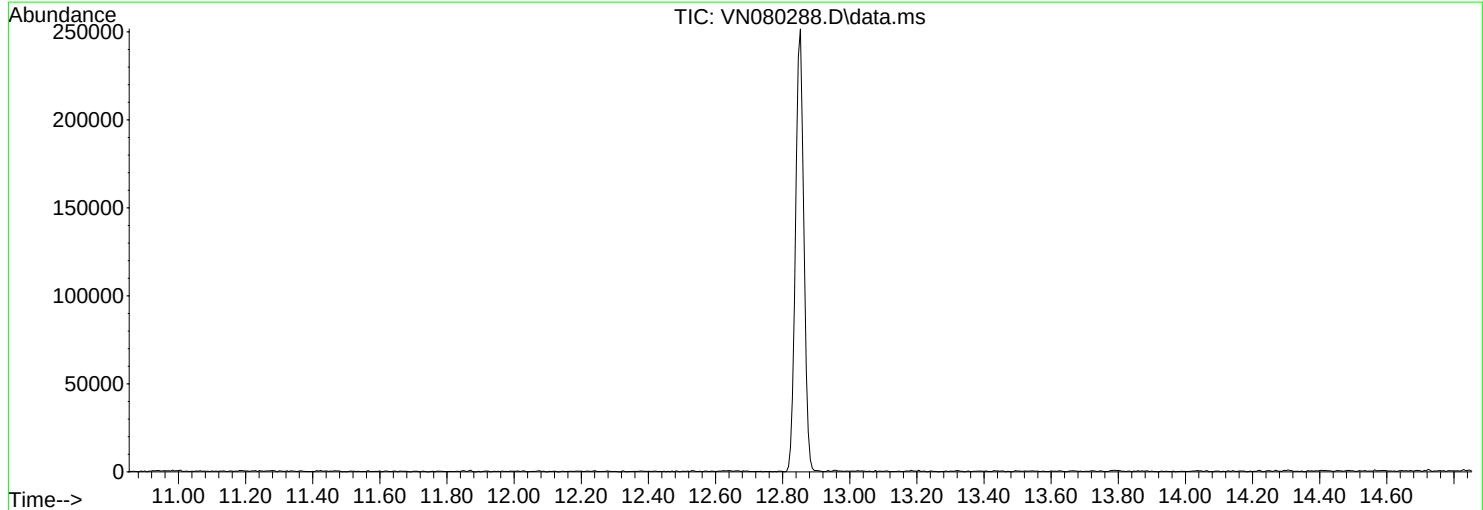

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	8000	PASS
75	95	30	60	57.1	24832	PASS
95	95	100	100	100.0	43485	PASS
96	95	5	9	6.9	2989	PASS
173	174	0.00	2	1.0	373	PASS
174	95	50	100	86.5	37597	PASS
175	174	5	9	7.7	2889	PASS
176	174	95	101	97.2	36531	PASS
177	176	5	9	6.0	2198	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	425	51.05	2143	66.90	51	78.00	10
37.05	2011	55.95	820	68.00	4656	78.95	198
38.05	1541	57.05	1259	69.00	4595	79.90	60
39.05	647	59.80	196	70.00	507	80.95	191
39.95	298	59.95	335	71.70	96	81.90	459
43.95	285	61.00	2212	72.05	228	87.05	1625
45.05	280	62.10	2532	72.95	2045	88.10	1565
46.95	414	63.05	1981	73.95	8065	90.90	121
47.85	231	64.05	532	75.05	24832	91.20	84
49.00	1912	64.80	133	76.05	2088	91.90	1288
50.05	8000	65.10	200	76.95	349	92.10	390

Average of 12.847 to 12.859 min.: VN080288.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	2381	128.90	55	174.95	2889		
94.05	6481	129.95	287	175.95	36531		
95.05	43485	140.90	750	176.95	2198		
96.05	2989	141.80	72	178.10	53		
103.85	168	142.95	1357	206.85	111		
105.85	325	144.90	486	281.05	133		
115.90	170	171.05	147				
116.95	528	171.90	144				
117.80	243	172.05	259				
118.85	502	173.00	373				
127.95	160	174.00	37597				