


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112918\
 Data File : VN052551.D
 Acq On : 29 Nov 2018 8:44
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
 Title : SW846 8260
 Last Update : Wed Nov 28 01:11:38 2018

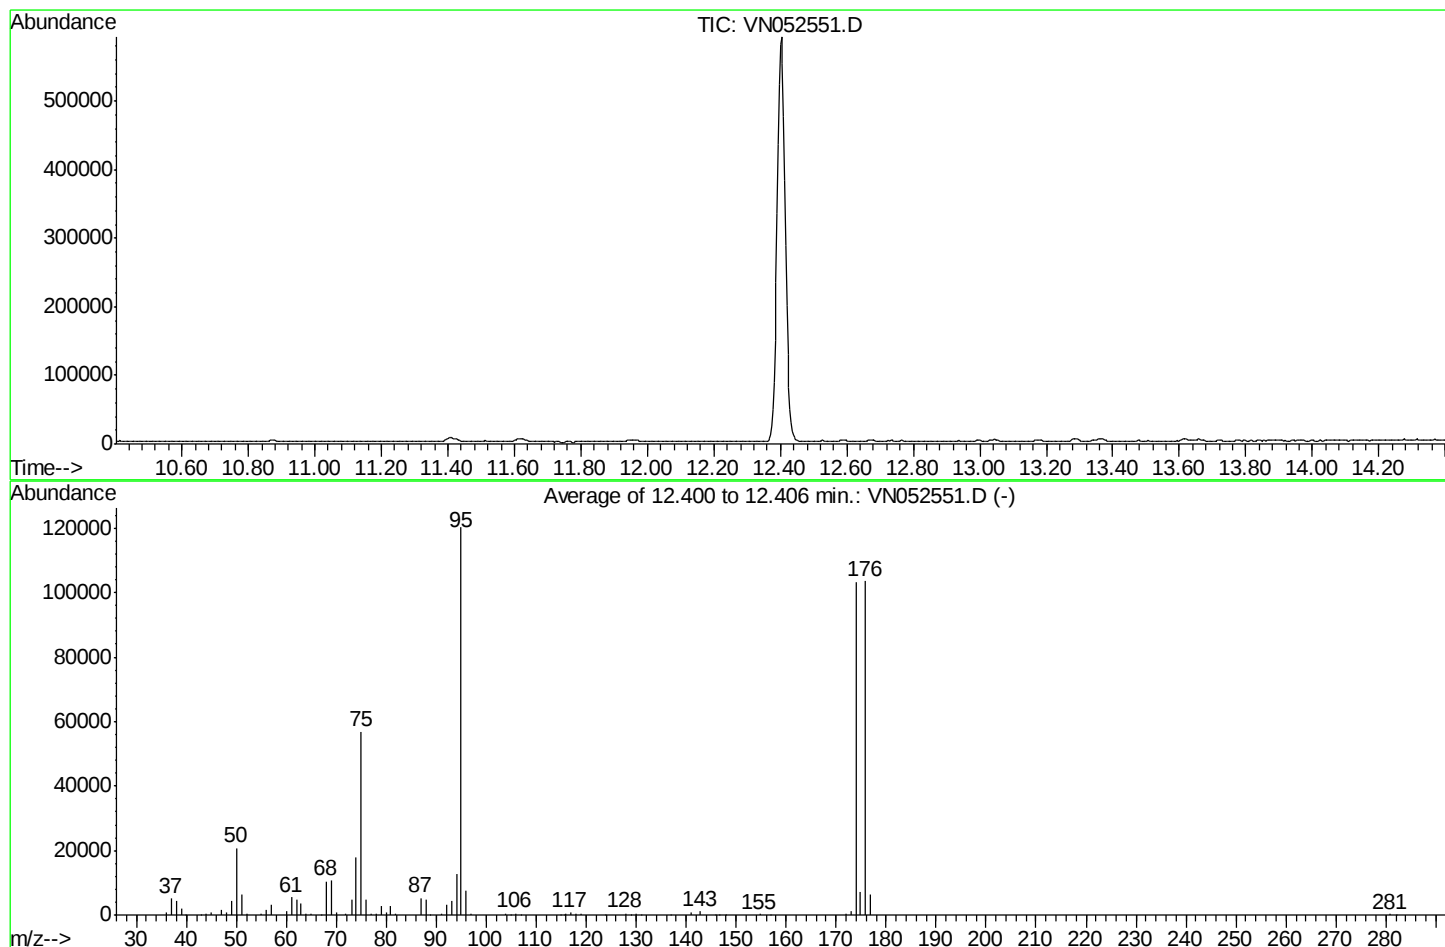

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	20672	PASS
75	95	30	60	47.3	56888	PASS
95	95	100	100	100.0	120253	PASS
96	95	5	9	6.4	7703	PASS
173	174	0.00	2	1.0	1013	PASS
174	95	50	100	85.9	103264	PASS
175	174	5	9	6.9	7142	PASS
176	174	95	101	100.2	103477	PASS
177	176	5	9	6.1	6292	PASS