

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112921\
 Data File : VN069659.D
 Acq On : 29 Nov 2021 12:21
 Operator : JC/MD
 Sample : VN1129MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 30 04:15:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 09 18:18:22 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	1404375	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2431003	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2412287	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	879995	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	1032634	50.712	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 101.420%			
35) Dibromofluoromethane	8.021	113	715320	49.061	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 98.120%			
50) Toluene-d8	10.440	98	3088009	53.851	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 107.700%			
62) 4-Bromofluorobenzene	12.731	95	1085904	51.548	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 103.100%			
Target Compounds						
					Qvalue	
5) Bromomethane	2.882	94	4887	0.432	ug/l #	81
13) Acrolein	4.046	56	910	Below Cal	#	46
16) Acetone	4.293	43	5644	0.514	ug/l	97
29) Tetrahydrofuran	7.694	42	2118	0.232	ug/l #	68
31) Cyclohexane	8.083	56	35934	1.292	ug/l #	7
36) 1,1-Dichloropropene	8.086	75	118702	5.803	ug/l #	49
38) Carbon Tetrachloride	8.086	117	144378	7.311	ug/l #	16
49) 1,4-Dioxane	9.574	88	1219	41.887	ug/l #	49
51) 4-Methyl-2-Pentanone	10.330	43	15201	0.530	ug/l	94
53) t-1,3-Dichloropropene	10.719	75	816	2.667	ug/l #	36
54) cis-1,3-Dichloropropene	10.199	75	377	1.746	ug/l #	58
56) Ethyl methacrylate	10.757	69	2921	2.147	ug/l	87
58) 2-Chloroethyl Vinyl ether	10.049	63	229	22.797	ug/l #	45
59) 2-Hexanone	11.095	43	30278	9.153	ug/l	92
60) Dibromochloromethane	11.240	129	528	2.446	ug/l	60
61) 1,2-Dibromoethane	11.341	107	412	1.094	ug/l #	48
70) Styrene	12.294	104	4552	1.601	ug/l #	87
71) Bromoform	12.457	173	858	3.487	ug/l #	29
74) N-amyl acetate	12.401	43	17367	0.585	ug/l #	90
76) 1,2,3-Trichloropropane	12.731	75	595543	29.325	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	595543	82.975	ug/l #	5
82) 4-Chlorotoluene	13.106	91	9575	0.206	ug/l	87
87) 1,3-Dichlorobenzene	13.616	146	7335	0.264	ug/l	95
88) 1,4-Dichlorobenzene	13.616	146	7335	0.269	ug/l	94
89) n-Butylbenzene	13.946	91	17354	0.378	ug/l	96
90) Hexachloroethane	14.214	117	25	2.164	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.597	75	1010	2.018	ug/l #	59
93) 1,2,4-Trichlorobenzene	15.262	180	14710	4.109	ug/l	97
94) Hexachlorobutadiene	15.372	225	1882	0.274	ug/l	71
95) Naphthalene	15.509	128	54248	5.716	ug/l	97
96) 1,2,3-Trichlorobenzene	15.705	180	17176	4.384	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: Nov 30 04:15:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 09 18:18:22 2021
Response via : Initial Calibration








#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 1404375
Ion Ratio Lower Upper
168 100
99 61.2 41.3 61.9

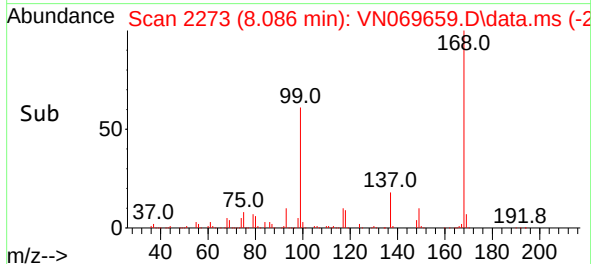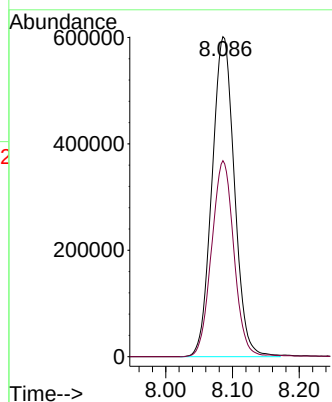

#5
Bromomethane
Concen: 0.432 ug/l
RT: 2.882 min Scan# 333
Delta R.T. 0.037 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Tgt Ion: 94 Resp: 4887
Ion Ratio Lower Upper
94 100
96 73.7 73.8 110.8#


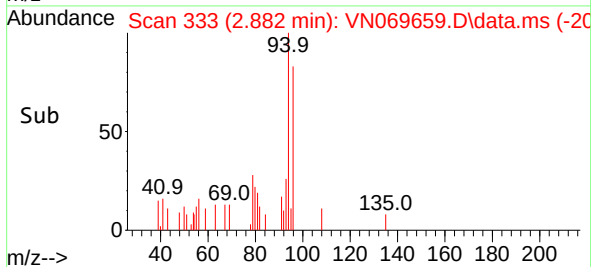
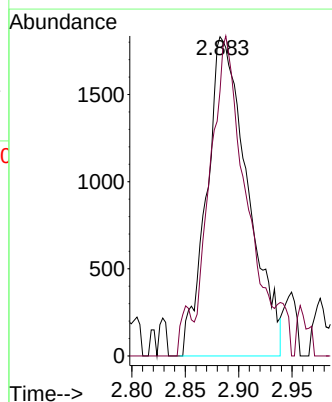
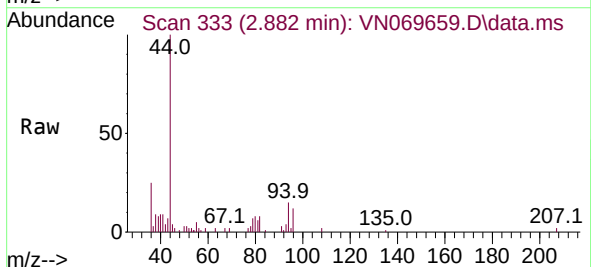




#13
Acrolein
Concen: Below Cal
RT: 4.046 min Scan# 765
Delta R.T. 0.005 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 910
Ion Ratio Lower Upper
56 100
55 25.8 56.6 85.0#

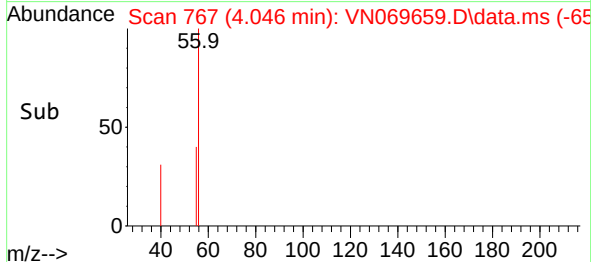

#16
Acetone
Concen: 0.514 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.005 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Tgt Ion: 43 Resp: 5644
Ion Ratio Lower Upper
43 100
58 30.5 23.1 34.7

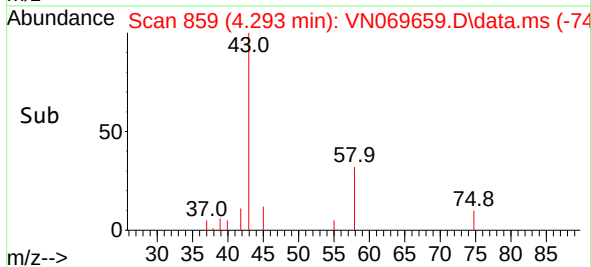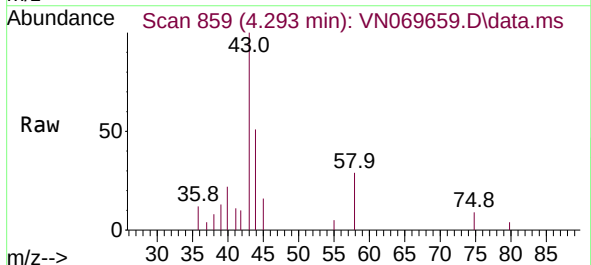

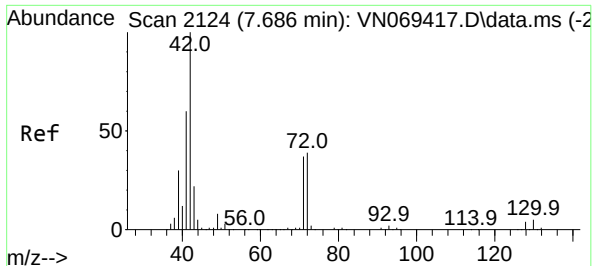

#29

Tetrahydrofuran

Concen: 0.232 ug/l

RT: 7.694 min Scan# 2124

Delta R.T. 0.008 min

Lab File: VN069659.D





Acq: 29 Nov 2021 12:21

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:	42	Resp:	2118
Ion	Ratio	Lower	Upper
42	100		
72	55.4	36.3	54.5#
71	12.0	34.7	52.1#

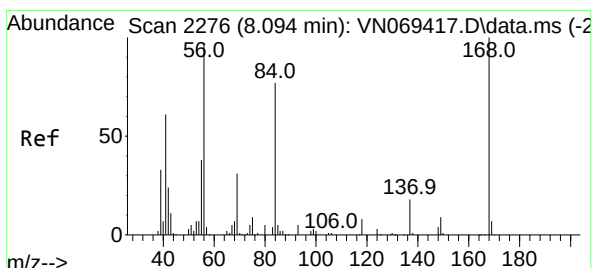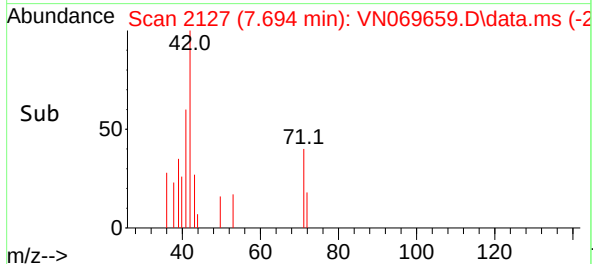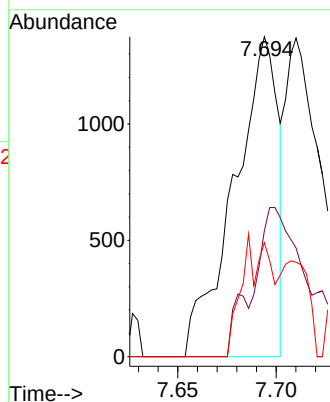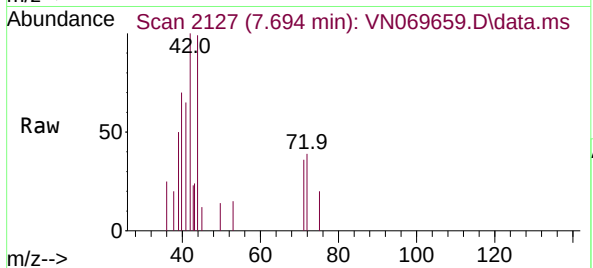

#31

Cyclohexane

Concen: 1.292 ug/l




RT: 8.083 min Scan# 2272


Delta R.T. -0.011 min

Lab File: VN069659.D

Acq: 29 Nov 2021 12:21


Tgt Ion:	56	Resp:	35934
Ion	Ratio	Lower	Upper
56	100		
69	170.6	27.1	40.7#
84	128.9	73.4	110.0#

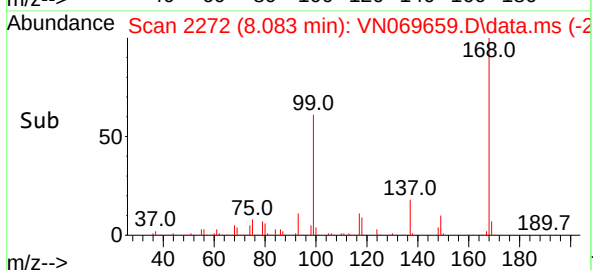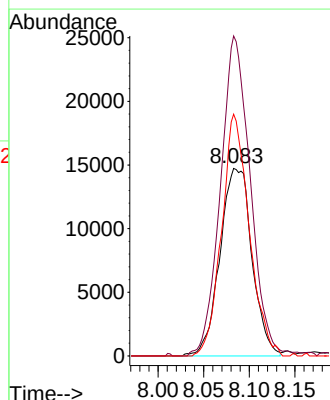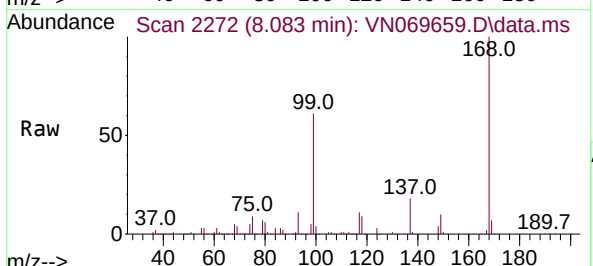






#33
 1,2-Dichloroethane-d4
 Concen: 50.712 ug/l
 RT: 8.437 min Scan# 2405
 Delta R.T. -0.003 min
 Lab File: VN069659.D
 Acq: 29 Nov 2021 12:21

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion: 65 Resp: 1032634
 Ion Ratio Lower Upper
 65 100
 67 51.0 0.0 103.0

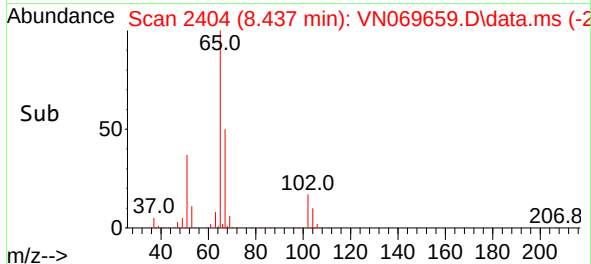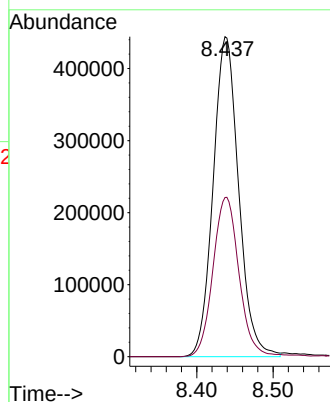

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.968 min Scan# 2602
 Delta R.T. -0.000 min
 Lab File: VN069659.D
 Acq: 29 Nov 2021 12:21


Tgt Ion: 114 Resp: 2431003
 Ion Ratio Lower Upper
 114 100
 63 23.0 0.0 37.8
 88 15.9 0.0 27.4

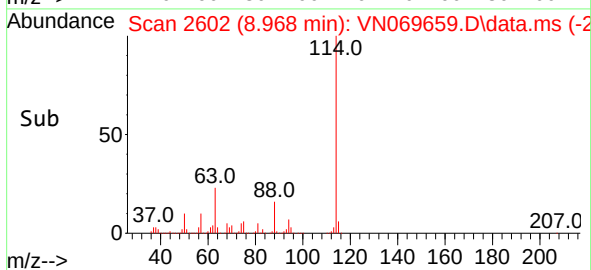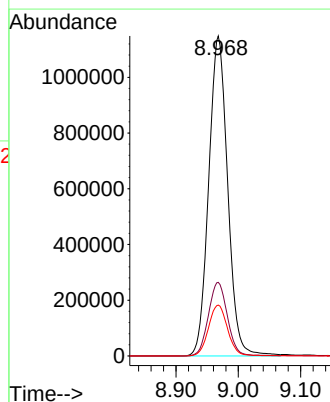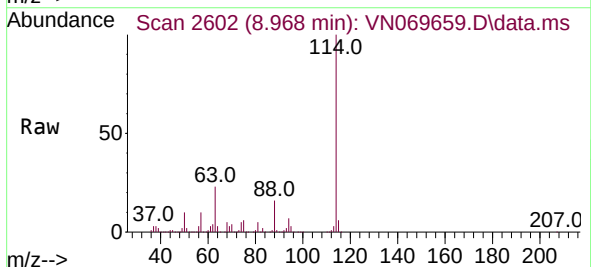



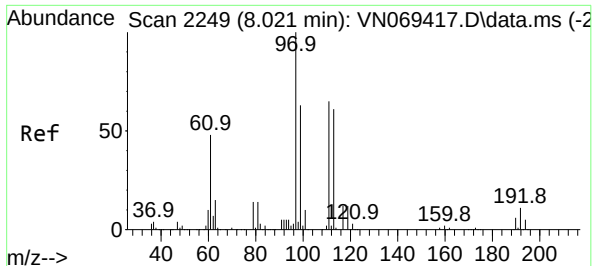


#35
 Dibromofluoromethane
 Concen: 49.061 ug/l
 RT: 8.021 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VN069659.D
 Acq: 29 Nov 2021 12:21

Instrument :
 MSVOA_N
 ClientSampleId :



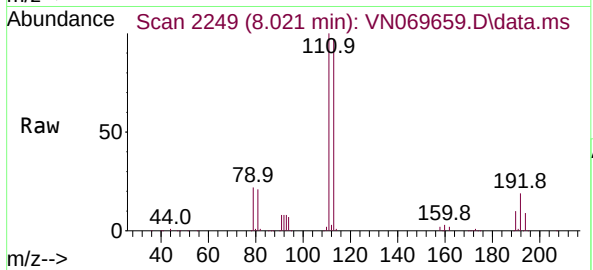



Tgt Ion:113 Resp: 715320
 Ion Ratio Lower Upper
 113 100
 111 104.6 82.2 123.2
 192 19.0 16.9 25.3

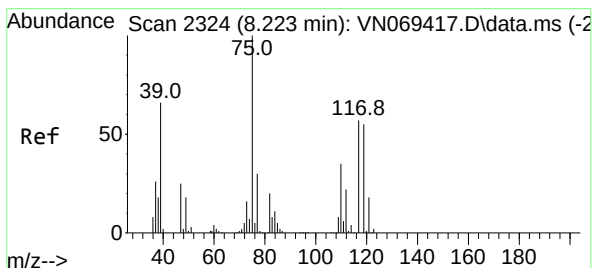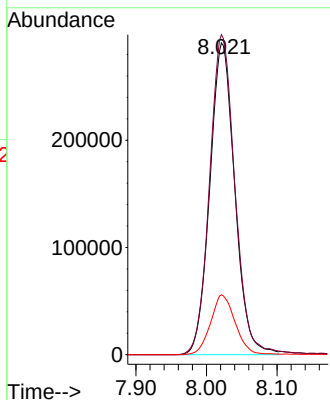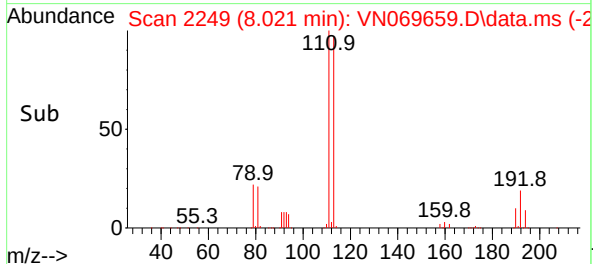

#36
 1,1-Dichloropropene
 Concen: 5.803 ug/l
 RT: 8.086 min Scan# 2273
 Delta R.T. -0.137 min
 Lab File: VN069659.D
 Acq: 29 Nov 2021 12:21


Tgt Ion: 75 Resp: 118702
 Ion Ratio Lower Upper
 75 100
 110 9.2 18.4 55.2#
 77 0.1 24.4 36.6#

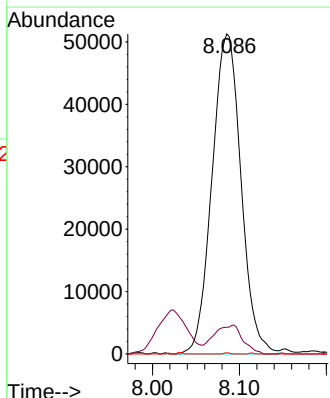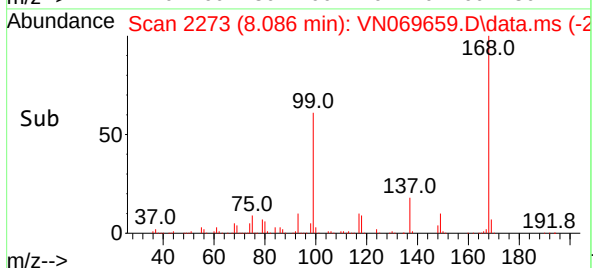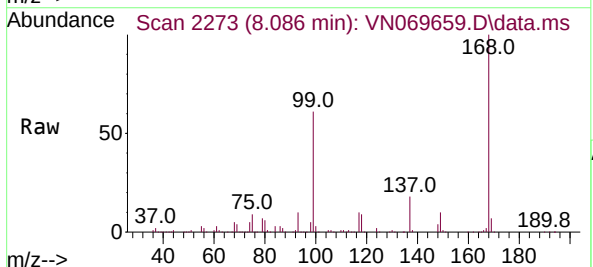



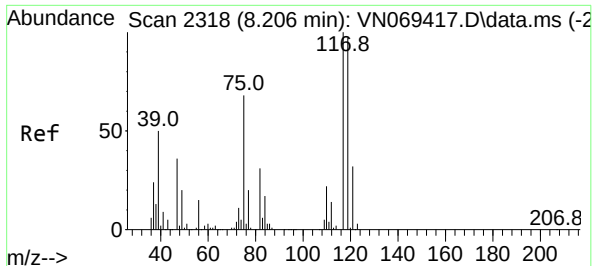


#38
Carbon Tetrachloride
Concen: 7.311 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.120 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Instrument :
MSVOA_N
ClientSampleId :



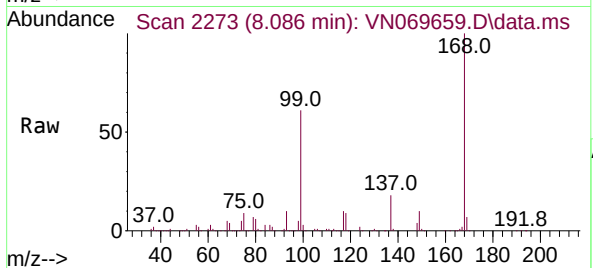



Tgt Ion:117 Resp: 144378
Ion Ratio Lower Upper
117 100
119 4.6 76.1 114.1#
121 0.0 24.2 36.2#

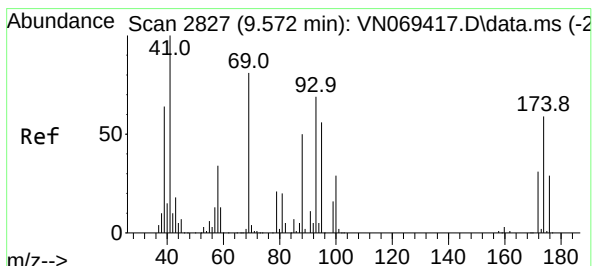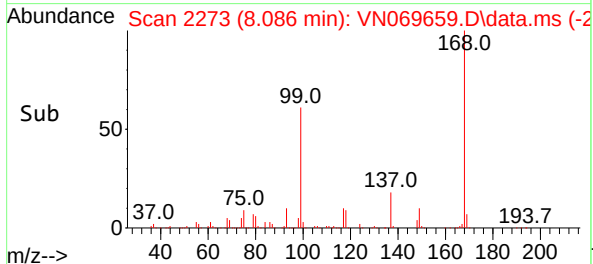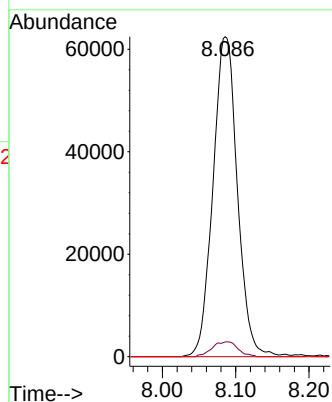

#49
1,4-Dioxane
Concen: 41.887 ug/l
RT: 9.574 min Scan# 2828
Delta R.T. 0.002 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Tgt Ion: 88 Resp: 1219
Ion Ratio Lower Upper
88 100
43 77.9 23.4 35.2#
58 38.3 50.6 75.8#


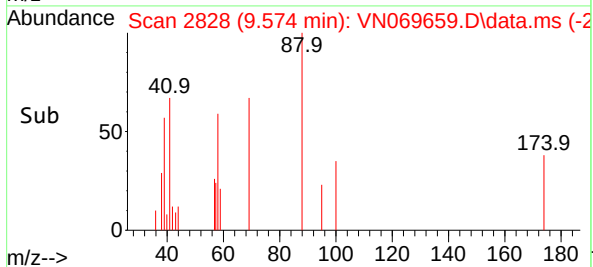

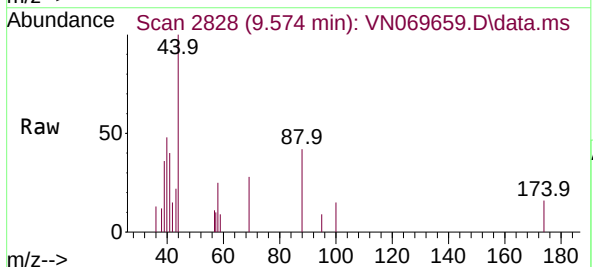




#50
Toluene-d8
Concen: 53.851 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. -0.001 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 3088009
Ion Ratio Lower Upper
98 100
100 63.4 50.4 75.6

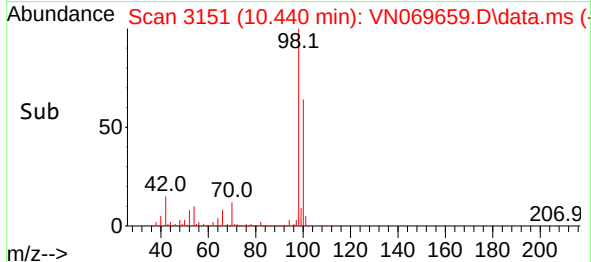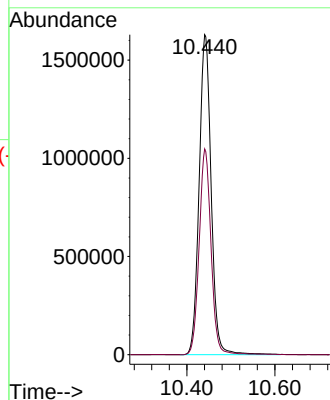

#51
4-Methyl-2-Pentanone
Concen: 0.530 ug/l
RT: 10.330 min Scan# 3110
Delta R.T. -0.001 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Tgt Ion: 43 Resp: 15201
Ion Ratio Lower Upper
43 100
58 34.6 30.4 45.6


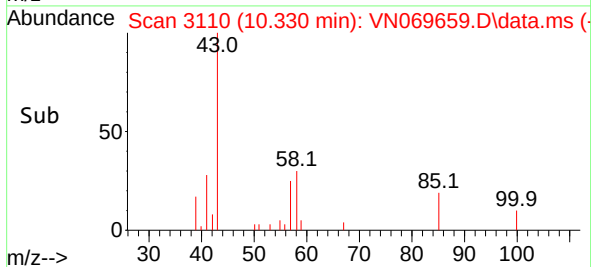
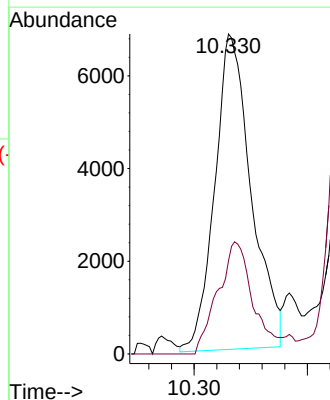
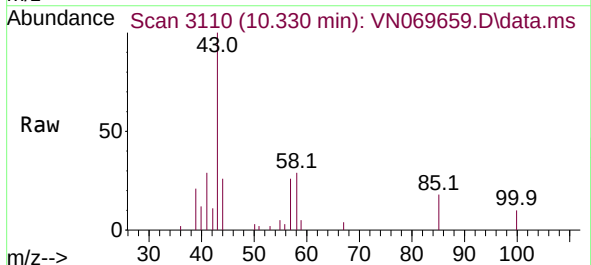


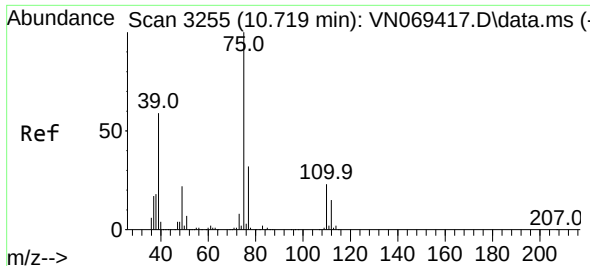

#53
t-1,3-Dichloropropene
Concen: 2.667 ug/l
RT: 10.719 min Scan# 31
Delta R.T. 0.000 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 816
Ion Ratio Lower Upper
75 100
77 67.4 25.6 38.4#

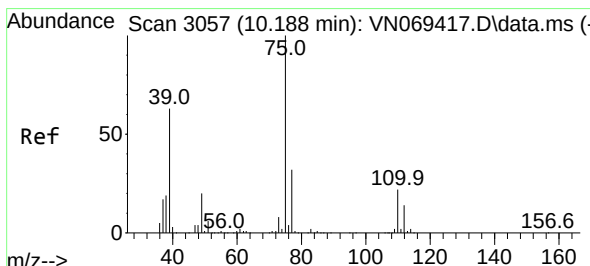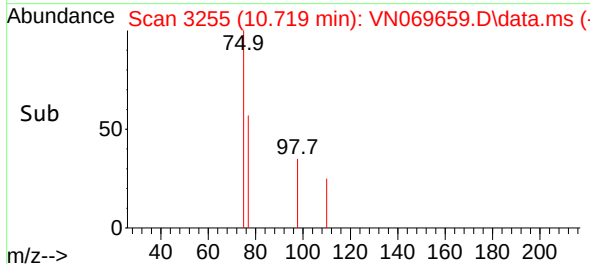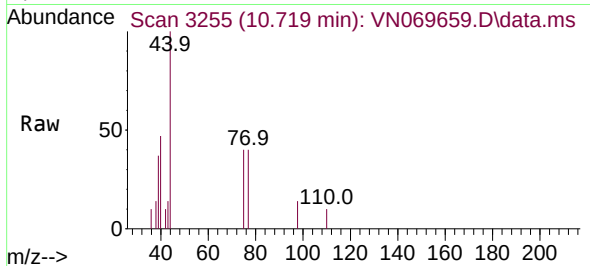

#54
cis-1,3-Dichloropropene
Concen: 1.746 ug/l
RT: 10.199 min Scan# 3061
Delta R.T. 0.011 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Tgt Ion: 75 Resp: 377
Ion Ratio Lower Upper
75 100
77 44.1 26.4 39.6#
39 13.0 42.5 63.7#


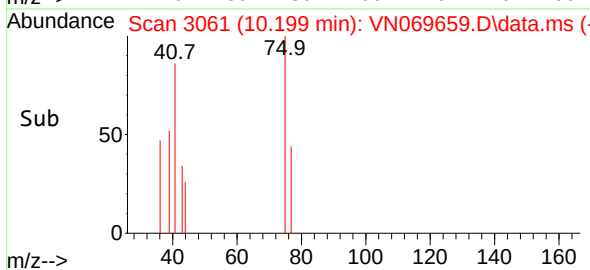

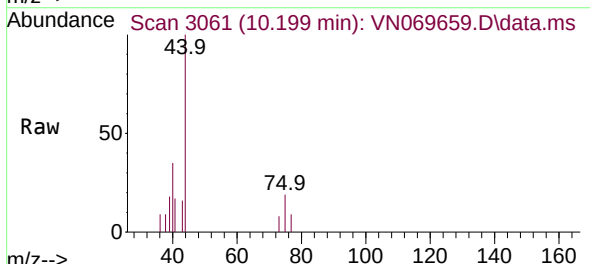




#56
Ethyl methacrylate
Concen: 2.147 ug/l
RT: 10.757 min Scan# 31
Delta R.T. -0.005 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 69	Resp: 2921
Ion Ratio	Lower Upper
69 100	
41 52.7	51.4 77.0
39 50.8	34.6 52.0

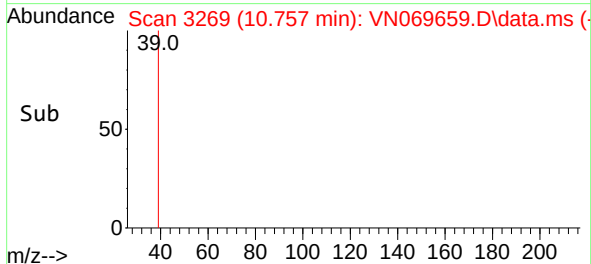

#58
2-Chloroethyl Vinyl ether
Concen: 22.797 ug/l
RT: 10.049 min Scan# 3005
Delta R.T. 0.008 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Tgt Ion: 63	Resp: 229		
Ion Ratio	Lower	Upper	
63 100			
106 0.0	23.9	35.9#	


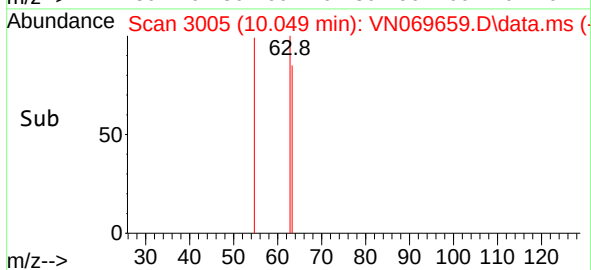

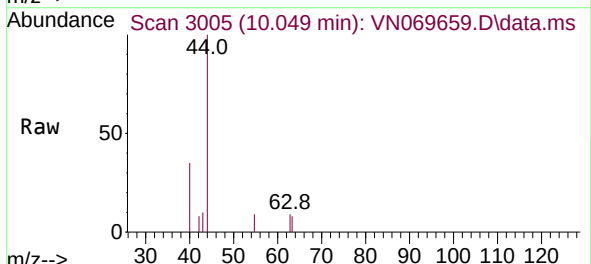




#59
2-Hexanone
Concen: 9.153 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 30278
Ion Ratio Lower Upper
43 100
58 48.0 26.9 80.7

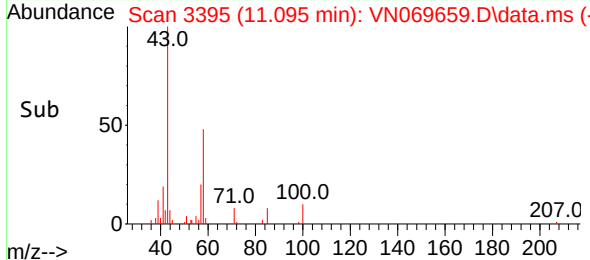

#60
Dibromochloromethane
Concen: 2.446 ug/l
RT: 11.240 min Scan# 3449
Delta R.T. -0.000 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21


Tgt Ion:129 Resp: 528
Ion Ratio Lower Upper
129 100
127 42.4 38.6 116.0

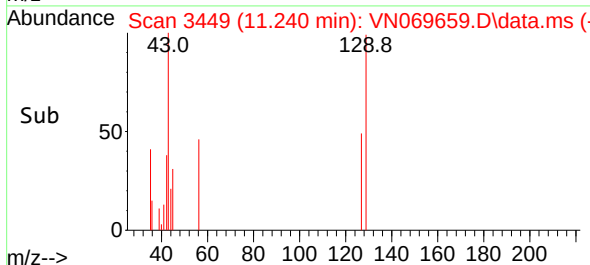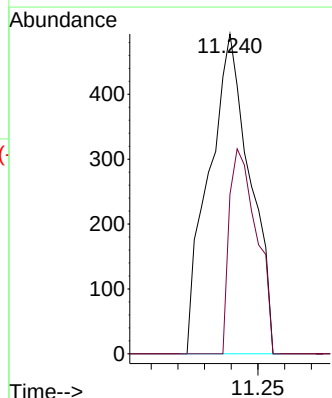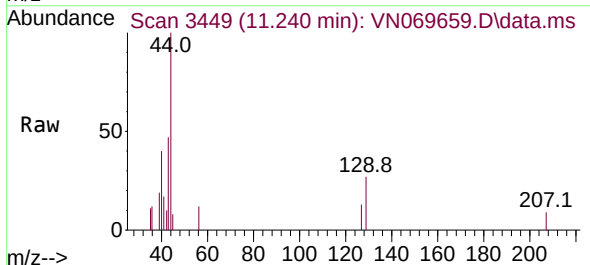






#61
1,2-Dibromoethane
Concen: 1.094 ug/l
RT: 11.341 min Scan# 3487
Delta R.T. -0.006 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:107 Resp: 412
Ion Ratio Lower Upper
107 100
109 44.7 75.7 113.5#

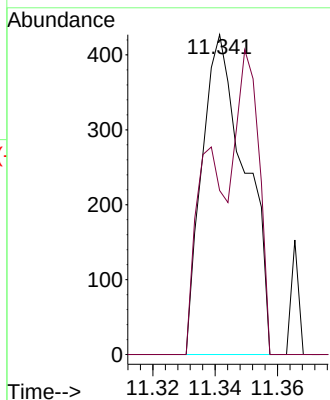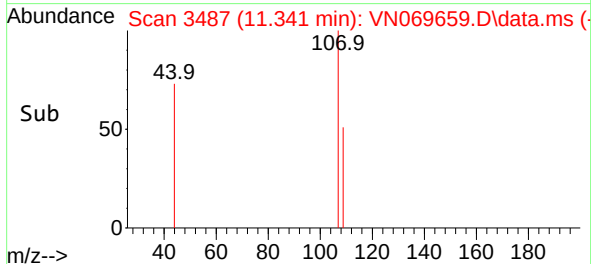

#62
4-Bromofluorobenzene
Concen: 51.548 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.003 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21


Tgt Ion: 95 Resp: 1085904
Ion Ratio Lower Upper
95 100
174 75.0 0.0 187.2
176 72.1 0.0 181.4

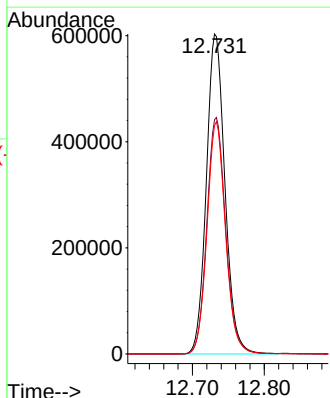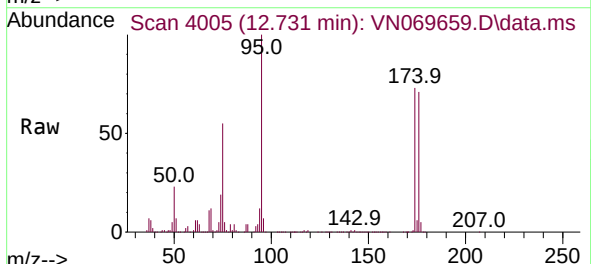

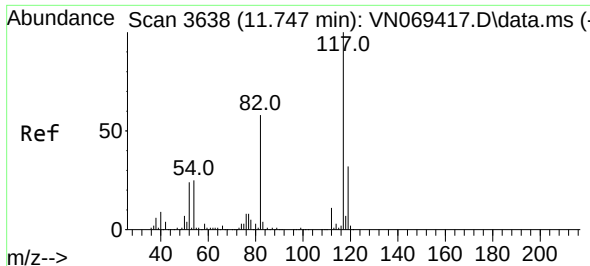




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.003 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:117 Resp: 2412287




Ion	Ratio	Lower	Upper
117	100		
82	59.2	42.4	63.6
119	32.0	25.4	38.2

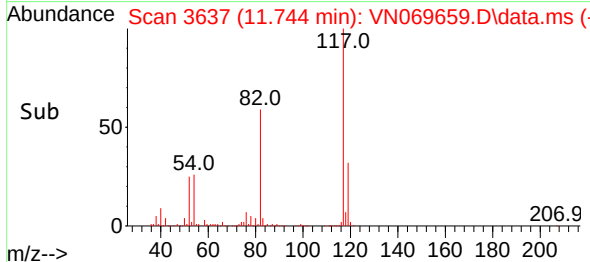


#70
Styrene
Concen: 1.601 ug/l
RT: 12.294 min Scan# 3842
Delta R.T. -0.000 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Tgt Ion:104 Resp: 4552

Ion	Ratio	Lower	Upper
104	100		
78	50.3	38.7	58.1
103	40.6	45.0	67.6


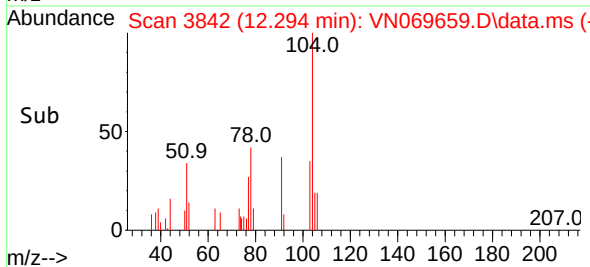
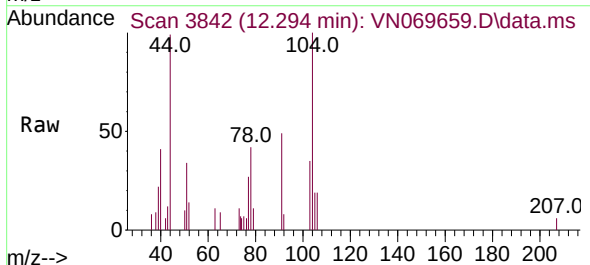



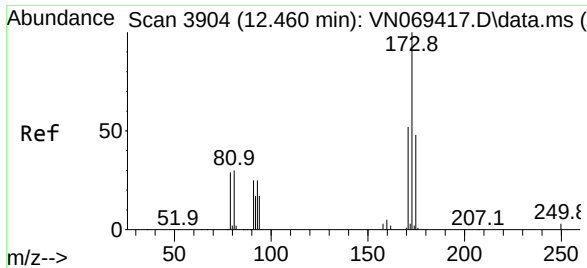

#71
Bromoform
Concen: 3.487 ug/l
RT: 12.457 min Scan# 3903
Delta R.T. -0.003 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 858
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

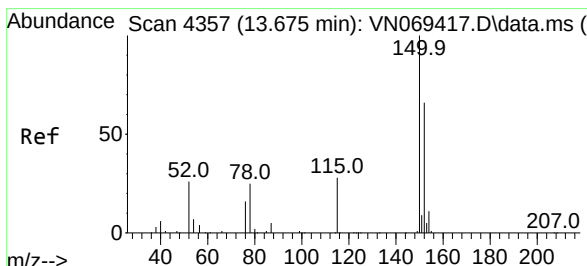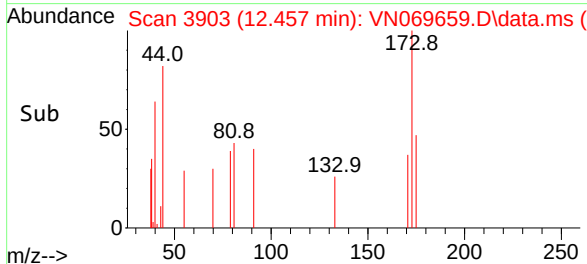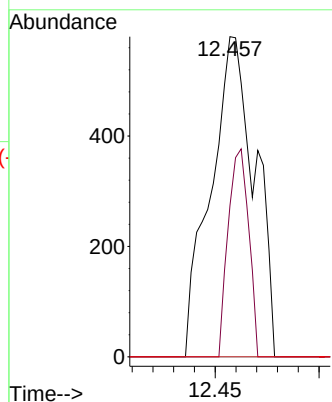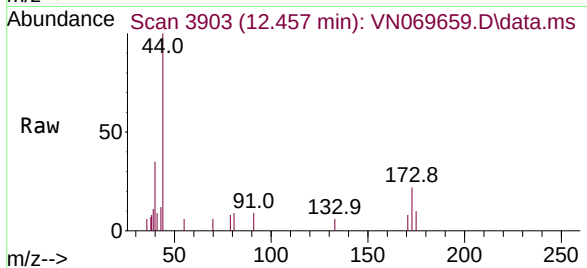

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.000 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21


Tgt Ion:152 Resp: 879995
Ion Ratio Lower Upper
152 100
115 60.2 27.5 82.5
150 156.8 0.0 344.4

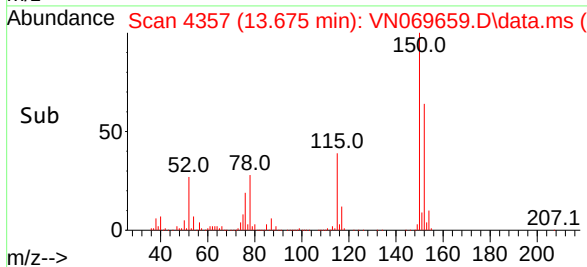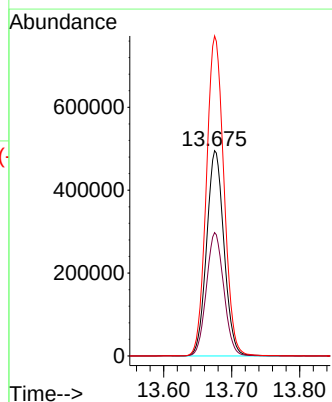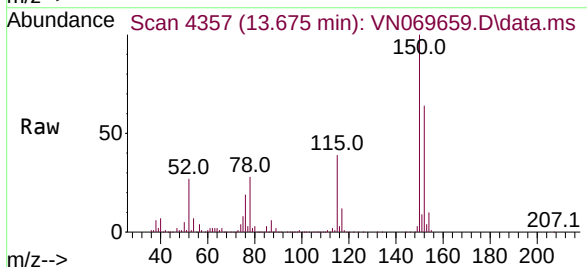



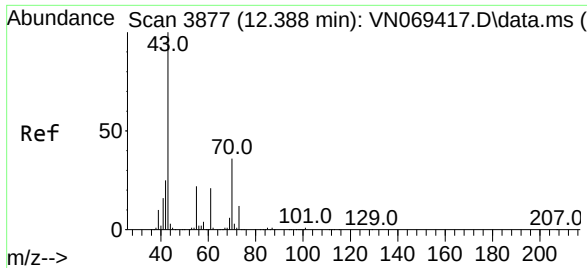


#74
N-amy1 acetate
Concen: 0.585 ug/l
RT: 12.401 min Scan# 3882
Delta R.T. 0.013 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Instrument :
MSVOA_N
ClientSampleId :



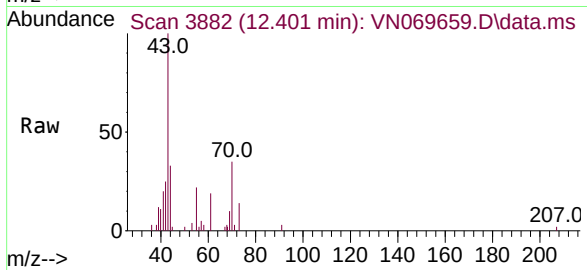



Tgt Ion: 43	Resp: 17367
Ion Ratio	Lower Upper
43	100
70	36.8 33.4 50.0
55	14.9 19.3 28.9#
61	21.2 18.5 27.7

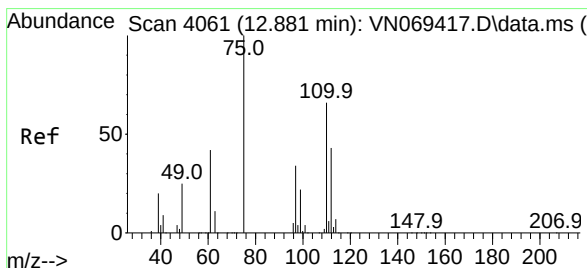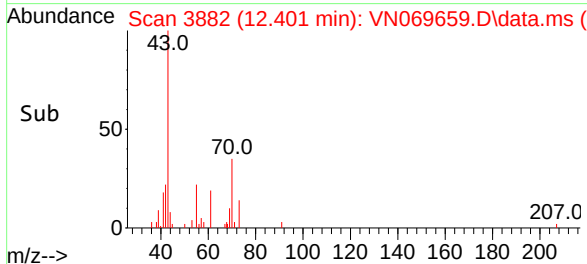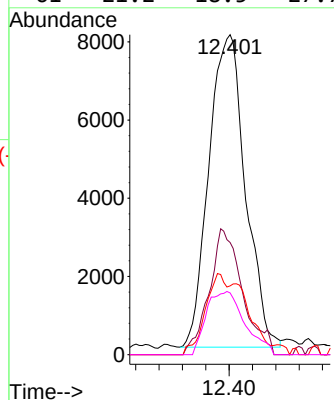

#76
1,2,3-Trichloropropane
Concen: 29.325 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Tgt Ion: 75	Resp: 595543
Ion Ratio	Lower Upper
75	100
77	1.0 82.6 247.8#


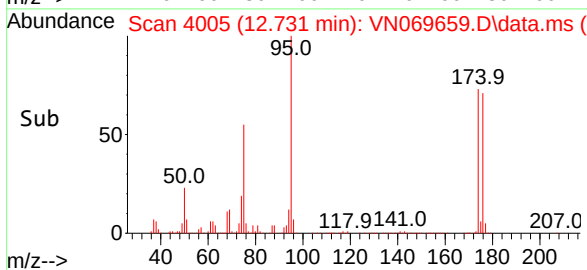
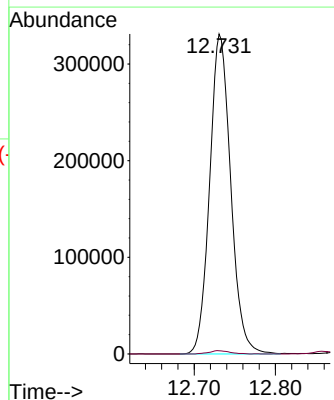
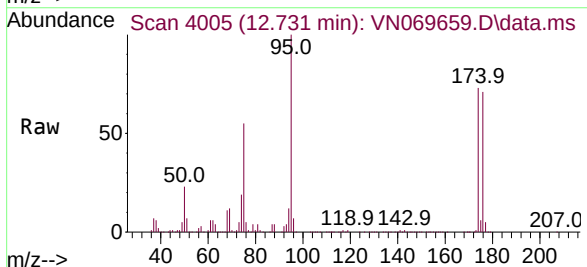


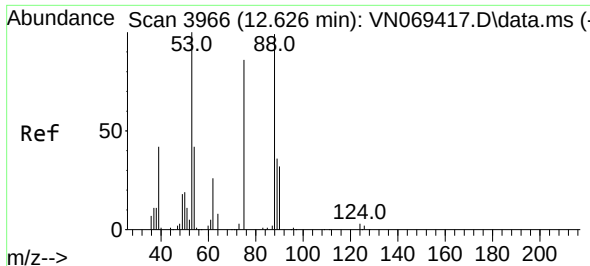

#81
trans-1,4-Dichloro-2-butene
Concen: 82.975 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 595543
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

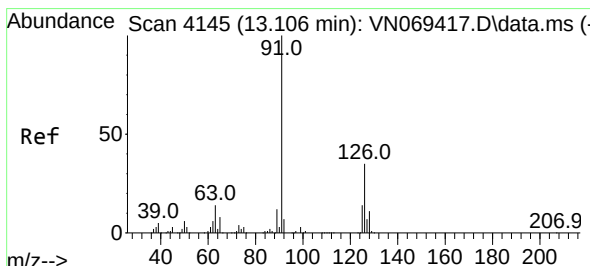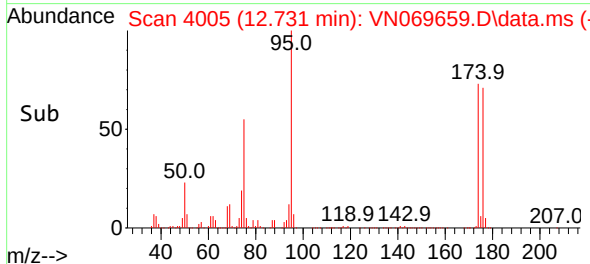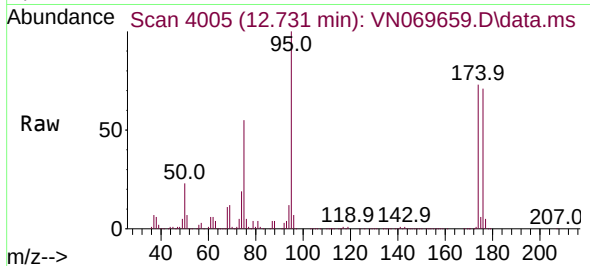

#82
4-Chlorotoluene
Concen: 0.206 ug/l
RT: 13.106 min Scan# 4145
Delta R.T. 0.000 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21


Tgt Ion: 91 Resp: 9575
Ion Ratio Lower Upper
91 100
126 28.7 18.2 54.6

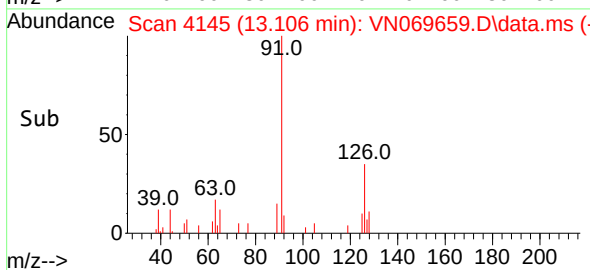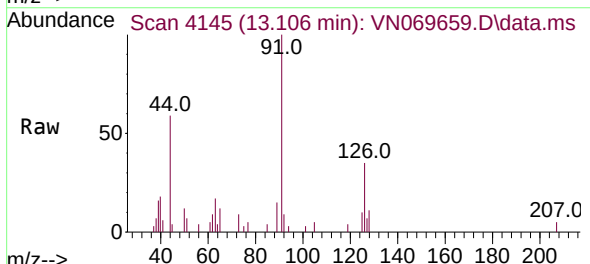






#87
 1,3-Dichlorobenzene
 Concen: 0.264 ug/l
 RT: 13.616 min Scan# 4335
 Delta R.T. -0.000 min
 Lab File: VN069659.D
 Acq: 29 Nov 2021 12:21


Instrument :
 MSVOA_N
 ClientSampleId :

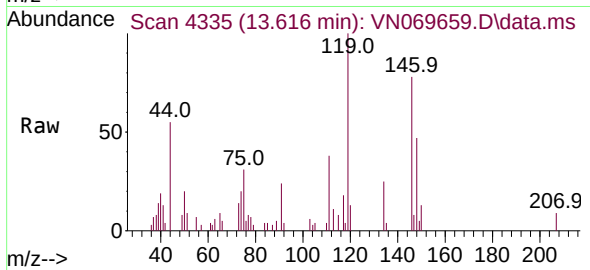



Tgt Ion:146	Resp:	7335
Ion	Ratio	Lower Upper
146	100	
111	43.4	18.6 55.6
148	62.0	31.6 95.0

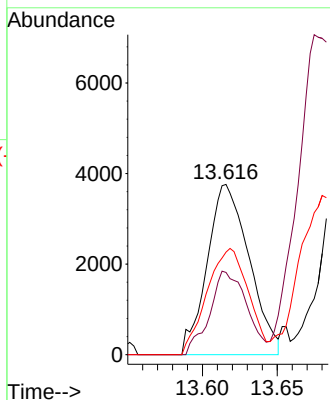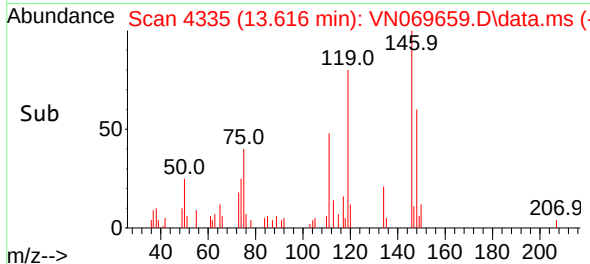


#88
 1,4-Dichlorobenzene
 Concen: 0.269 ug/l
 RT: 13.616 min Scan# 4335
 Delta R.T. -0.080 min
 Lab File: VN069659.D
 Acq: 29 Nov 2021 12:21

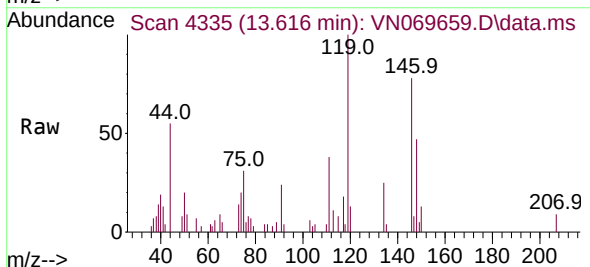

Tgt Ion:146	Resp:	7335
Ion	Ratio	Lower Upper
146	100	
111	43.4	18.3 54.8
148	62.0	31.8 95.4



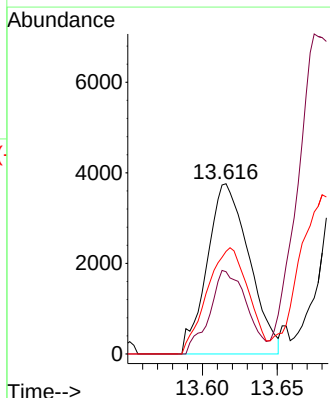



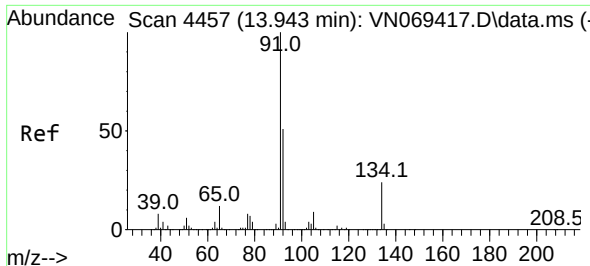

#89
n-Butylbenzene
Concen: 0.378 ug/l
RT: 13.946 min Scan# 4458
Delta R.T. 0.003 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 17354
Ion Ratio Lower Upper
91 100
92 51.2 25.4 76.0
134 22.4 13.6 40.8

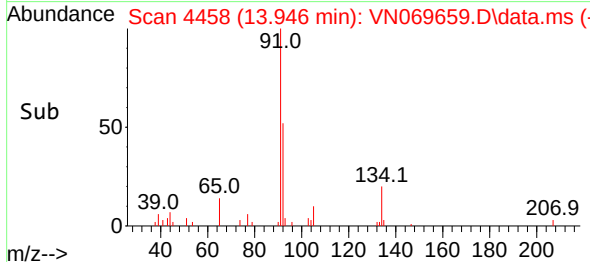

#90
Hexachloroethane
Concen: 2.164 ug/l
RT: 14.214 min Scan# 4558
Delta R.T. 0.003 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

Tgt Ion: 117 Resp: 25
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#


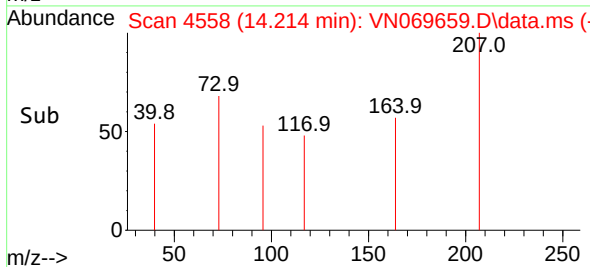

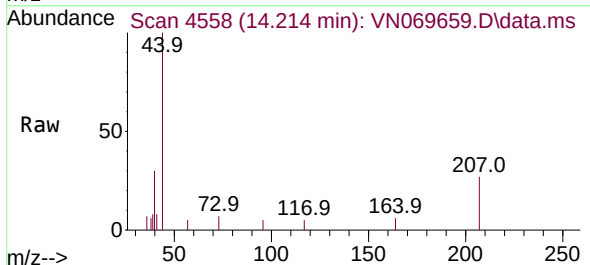


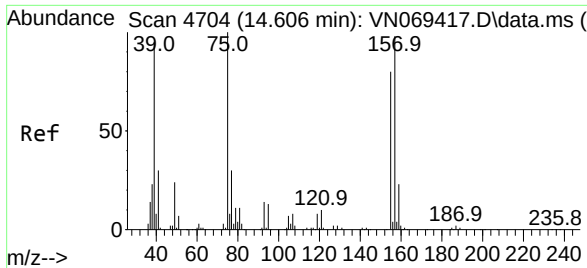

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 2.018 ug/l
 RT: 14.597 min Scan# 41
 Delta R.T. -0.009 min
 Lab File: VN069659.D
 Acq: 29 Nov 2021 12:21




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 1010
 Ion Ratio Lower Upper
 75 100
 155 143.7 46.9 140.7#
 157 157.0 60.6 181.7

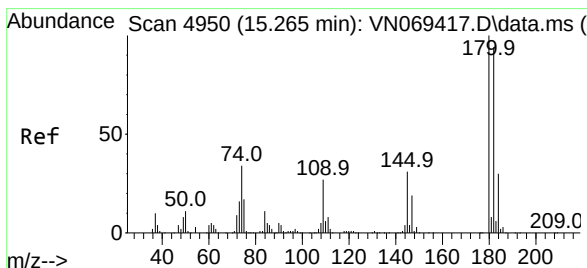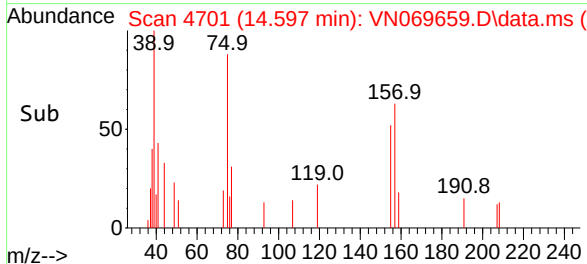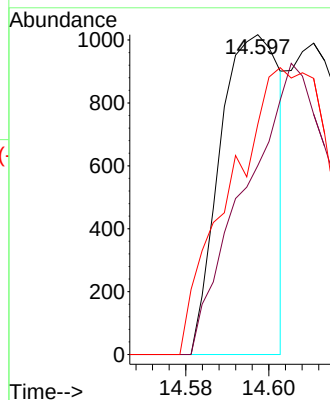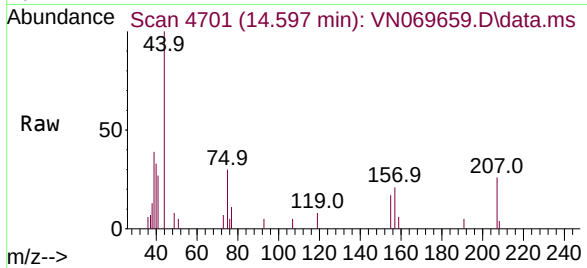

#93
 1,2,4-Trichlorobenzene
 Concen: 4.109 ug/l
 RT: 15.262 min Scan# 4949
 Delta R.T. -0.003 min
 Lab File: VN069659.D
 Acq: 29 Nov 2021 12:21


Tgt Ion:180 Resp: 14710
 Ion Ratio Lower Upper
 180 100
 182 92.6 48.3 144.9
 145 29.4 14.5 43.5

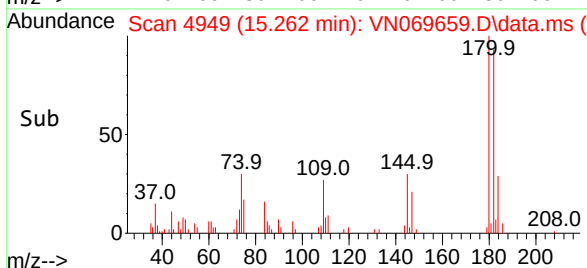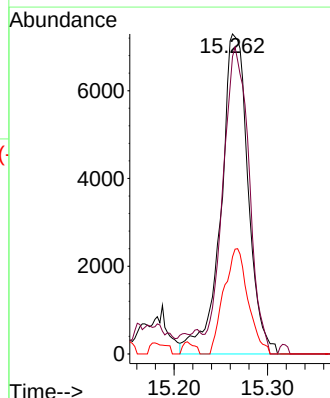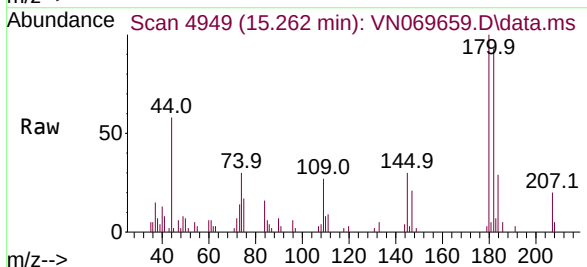






#94
Hexachlorobutadiene
Concen: 0.274 ug/l
RT: 15.372 min Scan# 4989
Delta R.T. 0.002 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21


Instrument :
MSVOA_N
ClientSampleId :

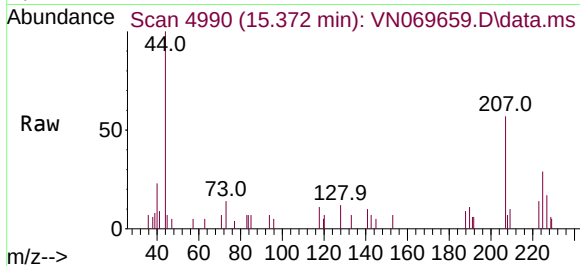



Tgt Ion:225 Resp: 1882
Ion Ratio Lower Upper
225 100
223 37.8 31.9 95.7
227 44.2 32.1 96.3

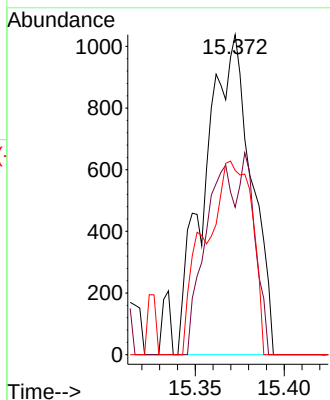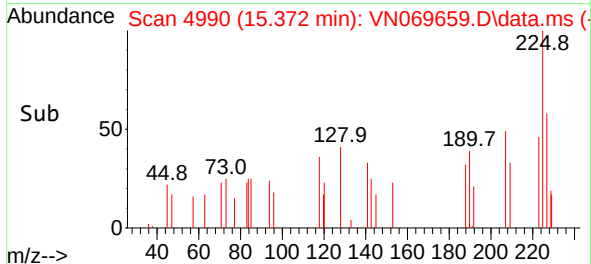


#95
Naphthalene
Concen: 5.716 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN069659.D
Acq: 29 Nov 2021 12:21

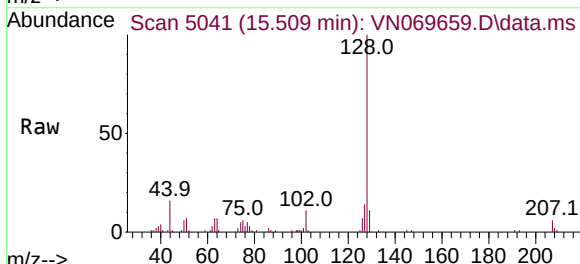


Tgt Ion:128 Resp: 54248
Ion Ratio Lower Upper
128 100
127 14.8 10.5 15.7
129 11.7 8.7 13.1

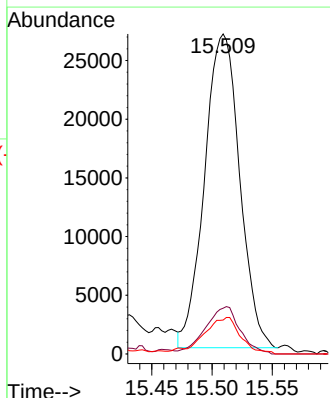



#96
 1,2,3-Trichlorobenzene
 Concen: 4.384 ug/l
 RT: 15.705 min Scan# 51
 Delta R.T. 0.005 min
 Lab File: VN069659.D
 Acq: 29 Nov 2021 12:21

Instrument :
 MSVOA_N
 ClientSampleId :

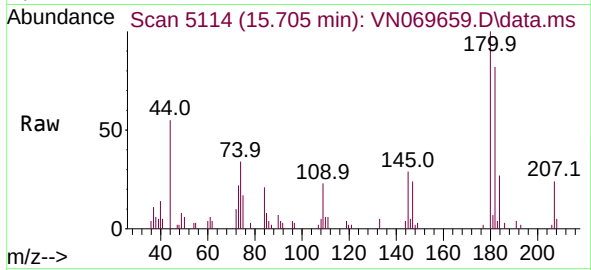

Tgt Ion:	180	Resp:	17176
Ion Ratio	Lower	Upper	
180	100		
182	94.8	47.4	142.2
145	34.7	15.0	45.1

