
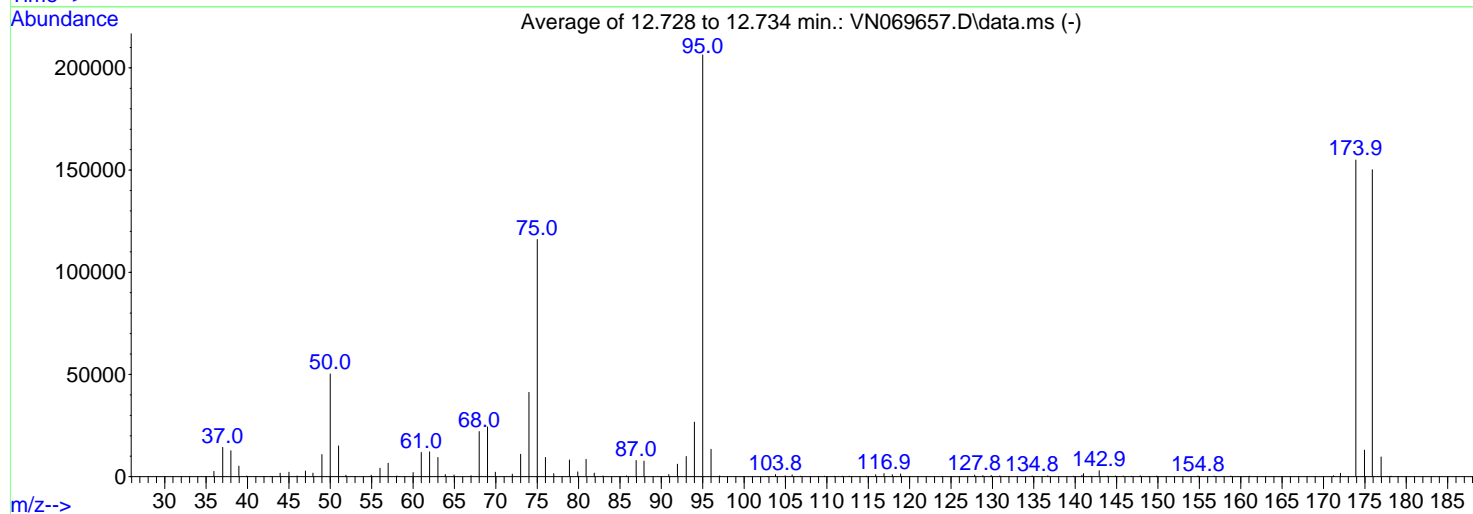


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112921\
 Data File : VN069657.D
 Acq On : 29 Nov 2021 9:43
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Title : SW846 8260
 Last Update : Tue Nov 09 18:18:22 2021

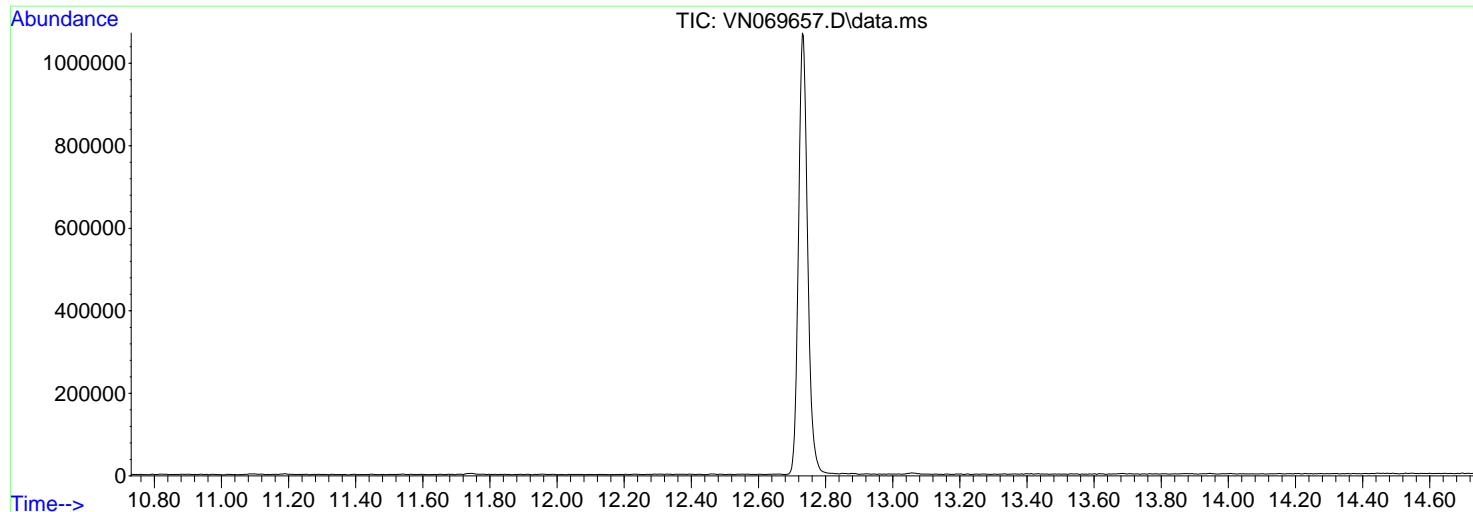

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3987

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result |
|-------------|--------------|--------------|--------------|-----------|---------|--------|
| 50 | 95 | 15 | 40 | 24.3 | 50235 | PASS |
| 75 | 95 | 30 | 60 | 56.2 | 116051 | PASS |
| 95 | 95 | 100 | 100 | 100.0 | 206379 | PASS |
| 96 | 95 | 5 | 9 | 6.5 | 13355 | PASS |
| 173 | 174 | 0.00 | 2 | 0.0 | 0 | PASS |
| 174 | 95 | 50 | 100 | 75.1 | 154901 | PASS |
| 175 | 174 | 5 | 9 | 8.4 | 12995 | PASS |
| 176 | 174 | 95 | 101 | 96.9 | 150144 | PASS |
| 177 | 176 | 5 | 9 | 6.4 | 9621 | PASS |