

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112922\
 Data File : VN075468.D
 Acq On : 29 Nov 2022 12:04
 Operator : JC\MD
 Sample : N5800-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RW9-PT-IN01-11282022

Quant Time: Nov 30 02:26:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	147642	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	247503	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	212166	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	84211	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	45236	57.079	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	114.160%
35) Dibromofluoromethane	8.171	113	53467	54.992	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	109.980%
50) Toluene-d8	10.565	98	112867	51.541	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.080%
62) 4-Bromofluorobenzene	12.847	95	83913	51.916	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	103.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112922\
Data File : VN075468.D
Acq On : 29 Nov 2022 12:04
Operator : JC\MD
Sample : N5800-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RW9-PT-IN01-11282022

Quant Time: Nov 30 02:26:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration




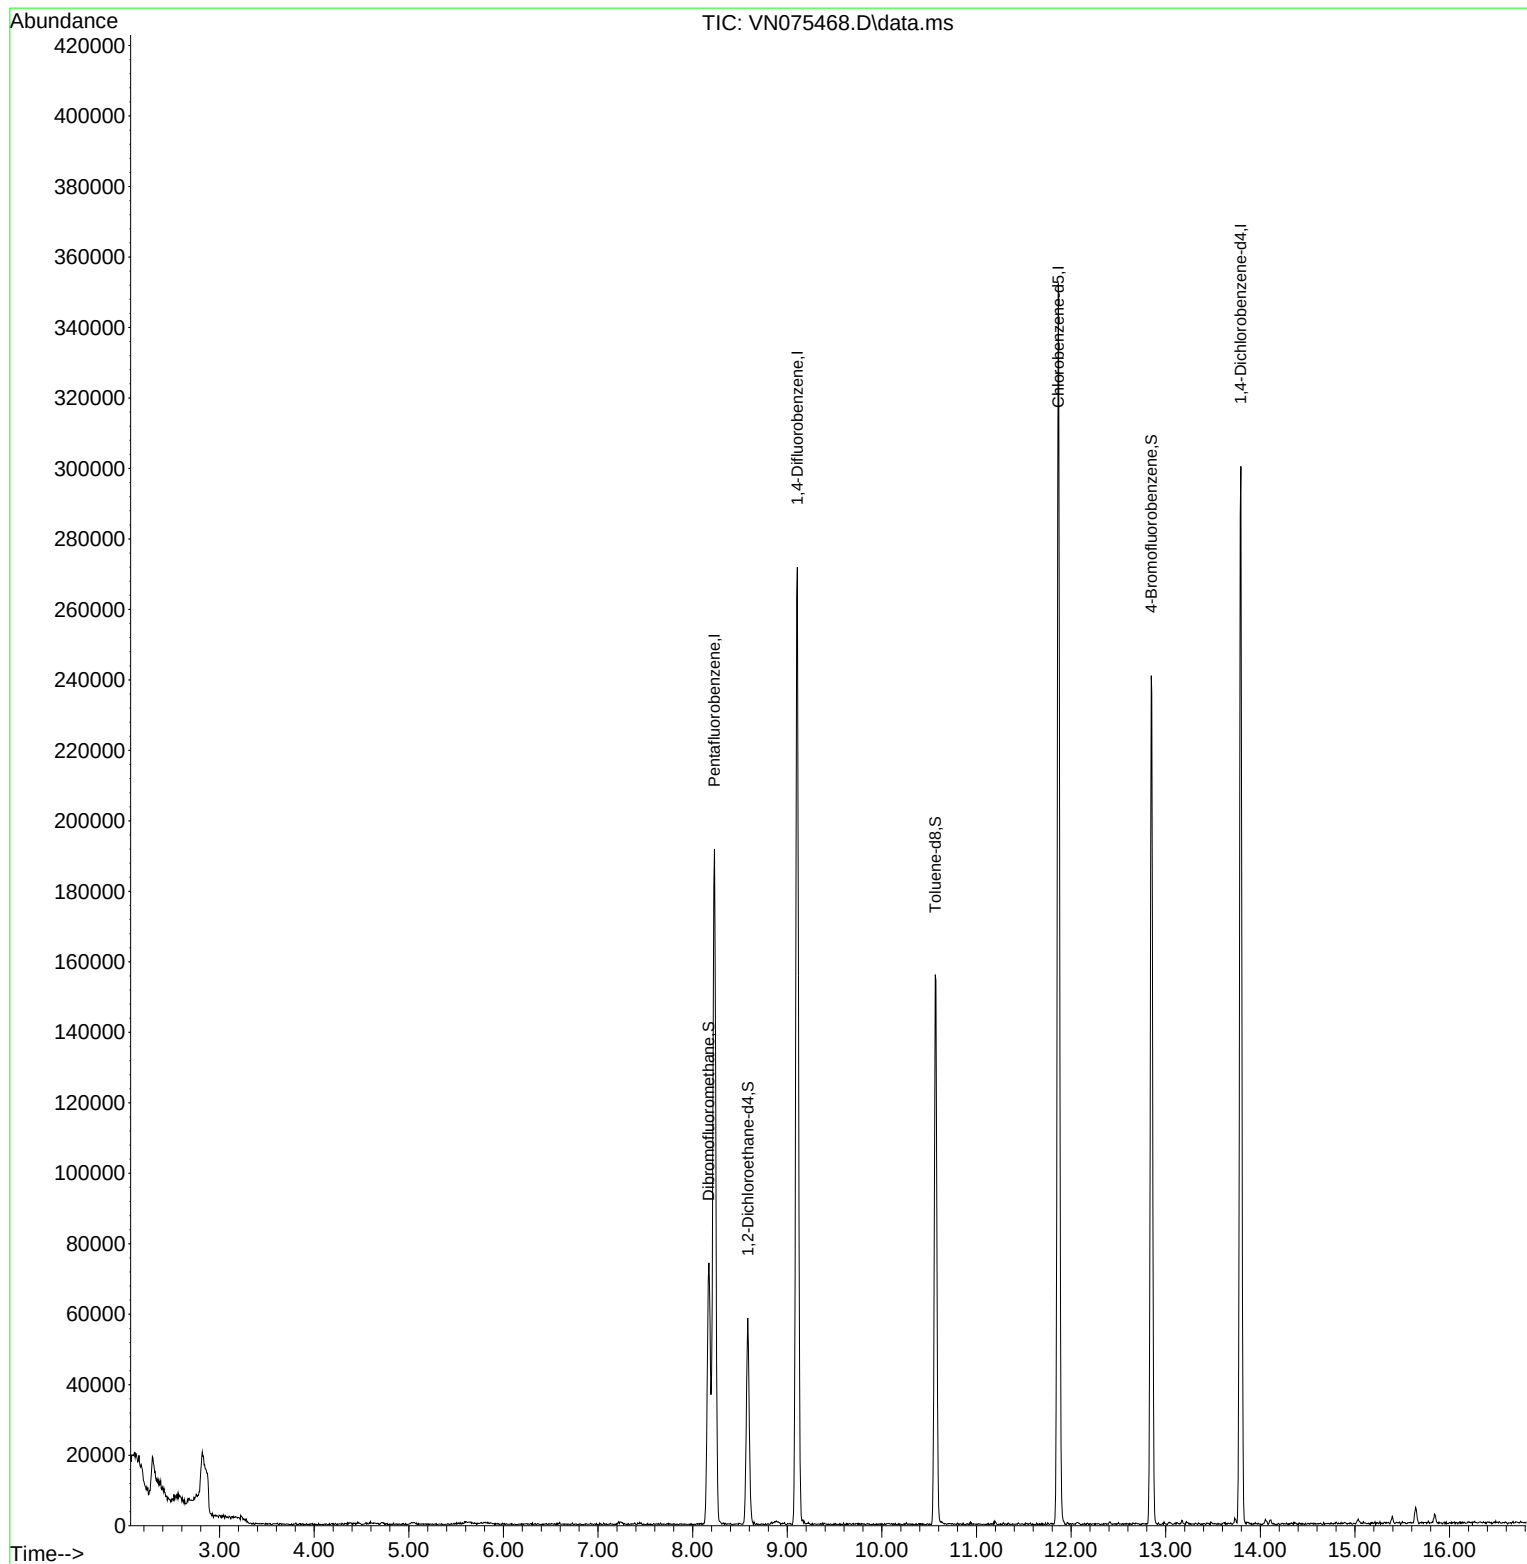


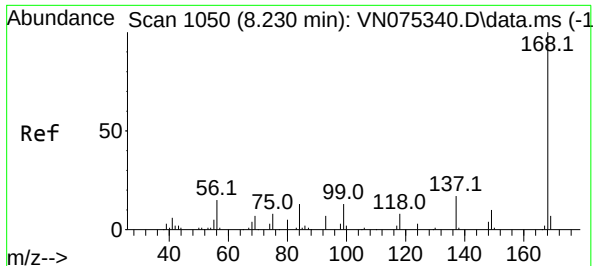

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1105
Delta R.T. -0.000 min
Lab File: VN075468.D
Acq: 29 Nov 2022 12:04




Instrument :
MSVOA_N
ClientSampleId :
RW9-PT-IN01-11282022


Tgt Ion:168 Resp: 147642
Ion Ratio Lower Upper
168 100
99 56.2 51.6 77.4

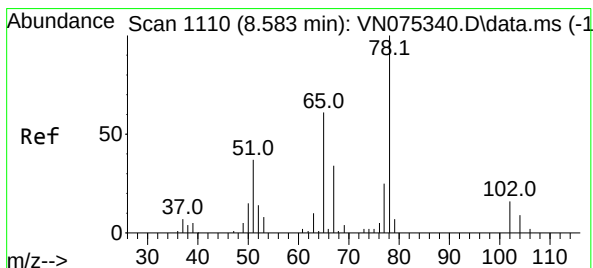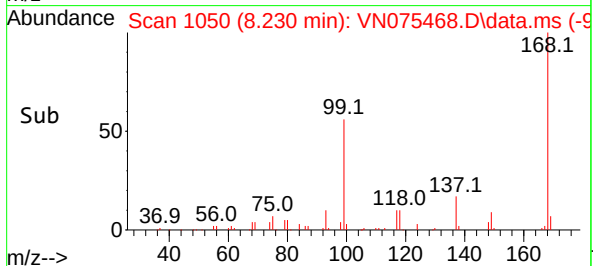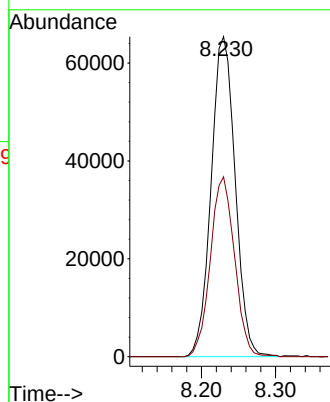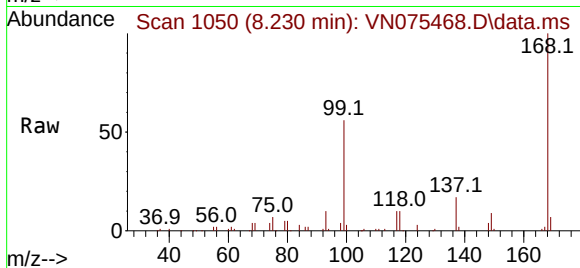

#33
1,2-Dichloroethane-d4
Concen: 57.079 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. -0.000 min
Lab File: VN075468.D
Acq: 29 Nov 2022 12:04

Tgt Ion: 65 Resp: 45236
Ion Ratio Lower Upper
65 100
67 50.9 0.0 102.0

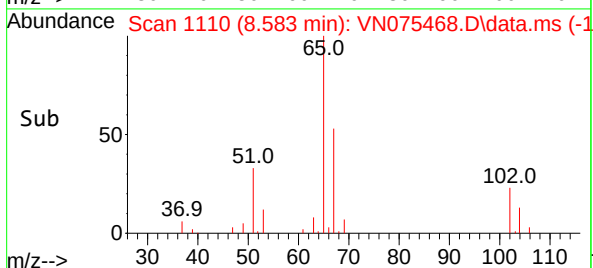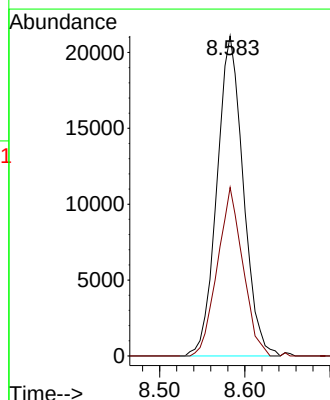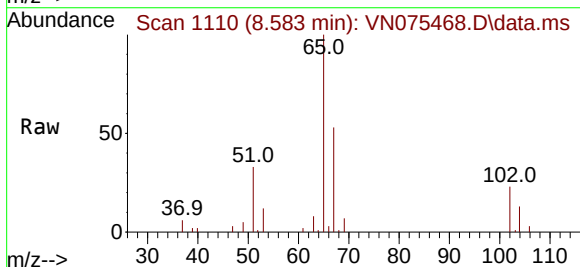

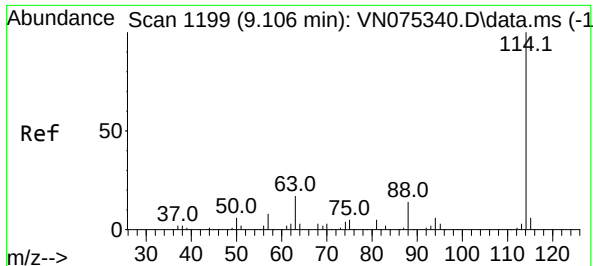

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075468.D

Acq: 29 Nov 2022 12:04

Instrument :

MSVOA_N

ClientSampleId :

RW9-PT-IN01-11282022





Tgt Ion:114 Resp: 247503

Ion Ratio Lower Upper

114 100

63 17.3 0.0 39.6

88 14.6 0.0 29.0

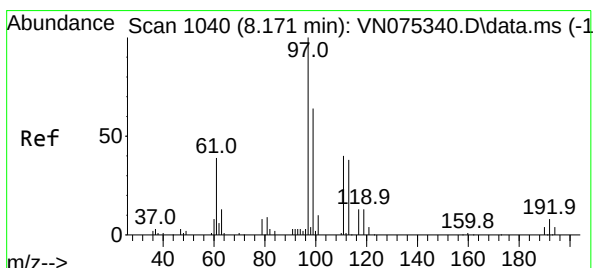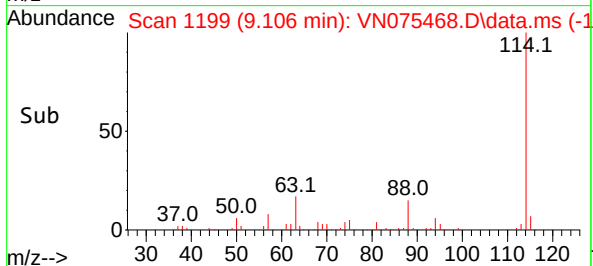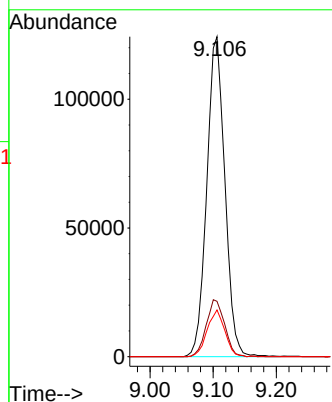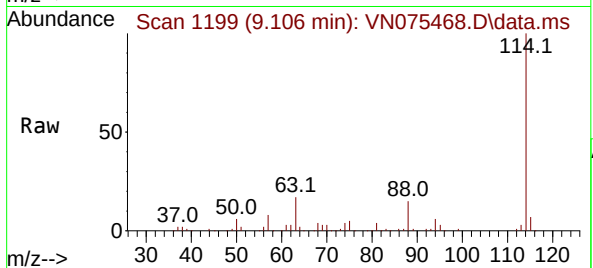

#35

Dibromofluoromethane

Concen: 54.992 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN075468.D

Acq: 29 Nov 2022 12:04




Tgt Ion:113 Resp: 53467


Ion Ratio Lower Upper

113 100

111 104.0 80.5 120.7

192 19.2 13.2 19.8


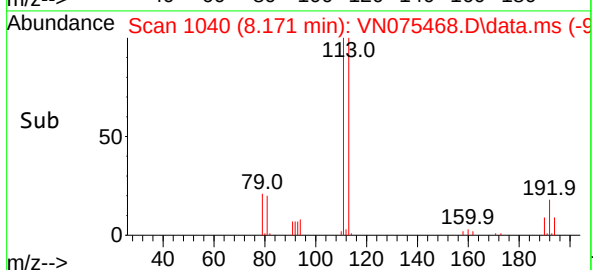
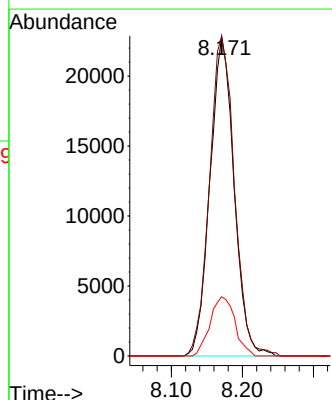
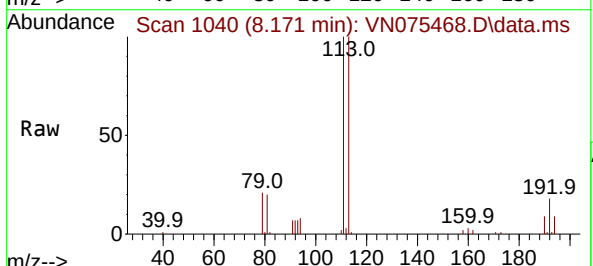


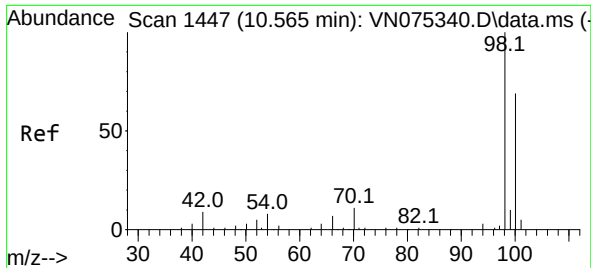

#50
Toluene-d8
Concen: 51.541 ug/l
RT: 10.565 min Scan# 1447
Delta R.T. -0.000 min
Lab File: VN075468.D
Acq: 29 Nov 2022 12:04




Instrument :
MSVOA_N
ClientSampleId :
RW9-PT-IN01-11282022


Tgt Ion: 98 Resp: 112867
Ion Ratio Lower Upper
98 100
100 67.0 53.0 79.6

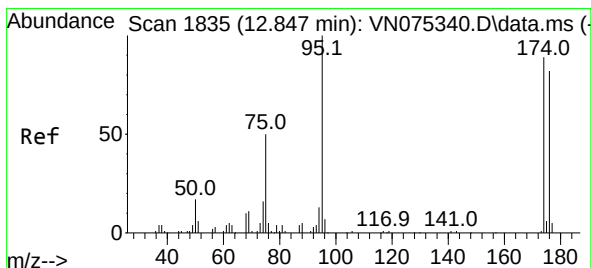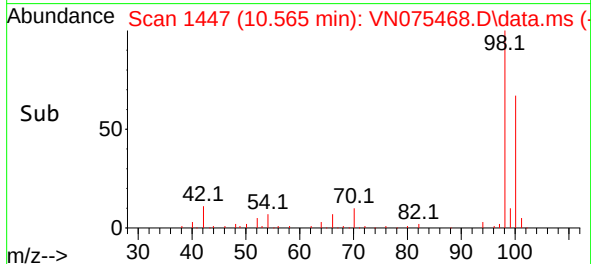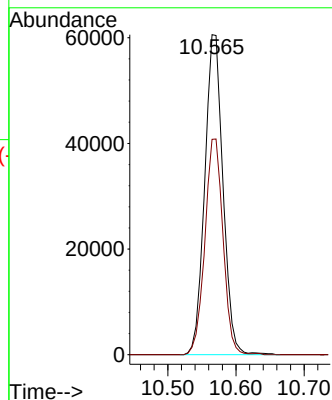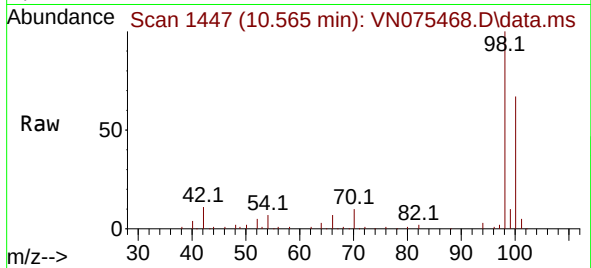

#62
4-Bromofluorobenzene
Concen: 51.916 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.000 min
Lab File: VN075468.D
Acq: 29 Nov 2022 12:04

Tgt Ion: 95 Resp: 83913
Ion Ratio Lower Upper
95 100
174 82.2 0.0 147.4
176 80.3 0.0 142.2


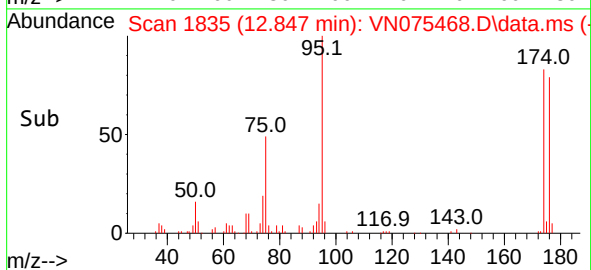
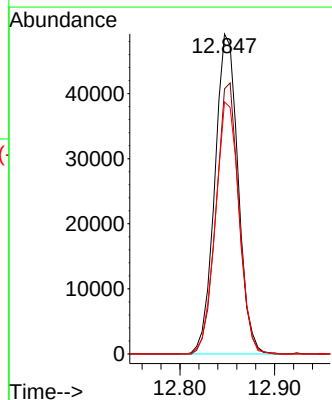
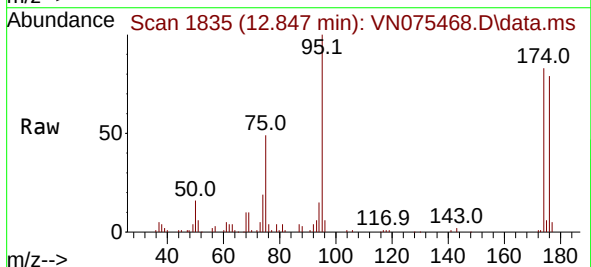


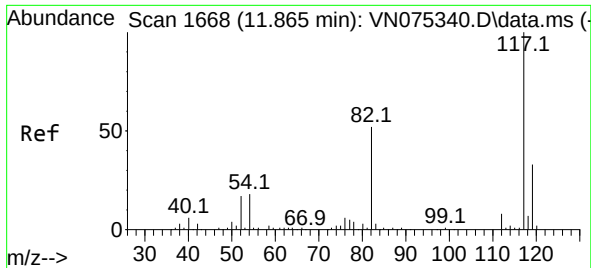

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN075468.D
Acq: 29 Nov 2022 12:04

Instrument :
MSVOA_N
ClientSampleId :
RW9-PT-IN01-11282022

Tgt Ion:117 Resp: 212166
Ion Ratio Lower Upper
117 100
82 54.3 43.1 64.7
119 33.4 25.5 38.3

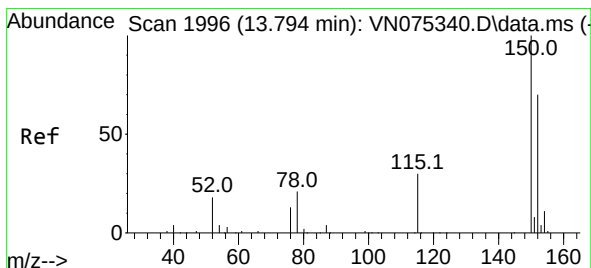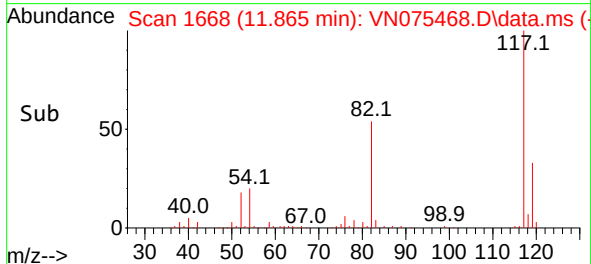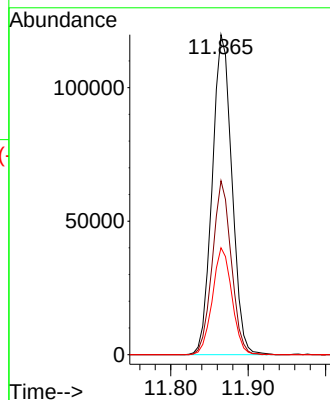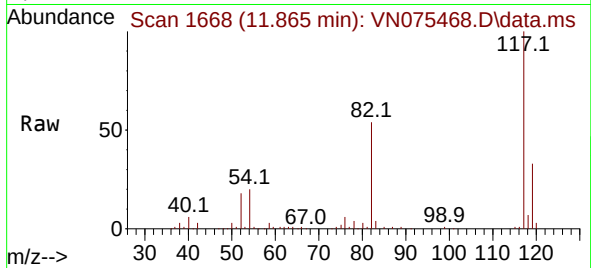

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN075468.D
Acq: 29 Nov 2022 12:04

Tgt Ion:152 Resp: 84211
Ion Ratio Lower Upper
152 100
115 59.7 30.2 90.6
150 159.6 0.0 348.4

