

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112922\
 Data File : VN075471.D
 Acq On : 29 Nov 2022 13:16
 Operator : JC\MD
 Sample : N5800-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TB01-11282022

Quant Time: Nov 30 02:26:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	123027	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	209809	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	178946	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	69976	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	33728	51.073	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	102.140%
35) Dibromofluoromethane	8.171	113	41681	50.572	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.140%
50) Toluene-d8	10.571	98	85263	45.931	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	91.860%
62) 4-Bromofluorobenzene	12.853	95	61111	44.601	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112922\
Data File : VN075471.D
Acq On : 29 Nov 2022 13:16
Operator : JC\MD
Sample : N5800-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB01-11282022

Quant Time: Nov 30 02:26:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration




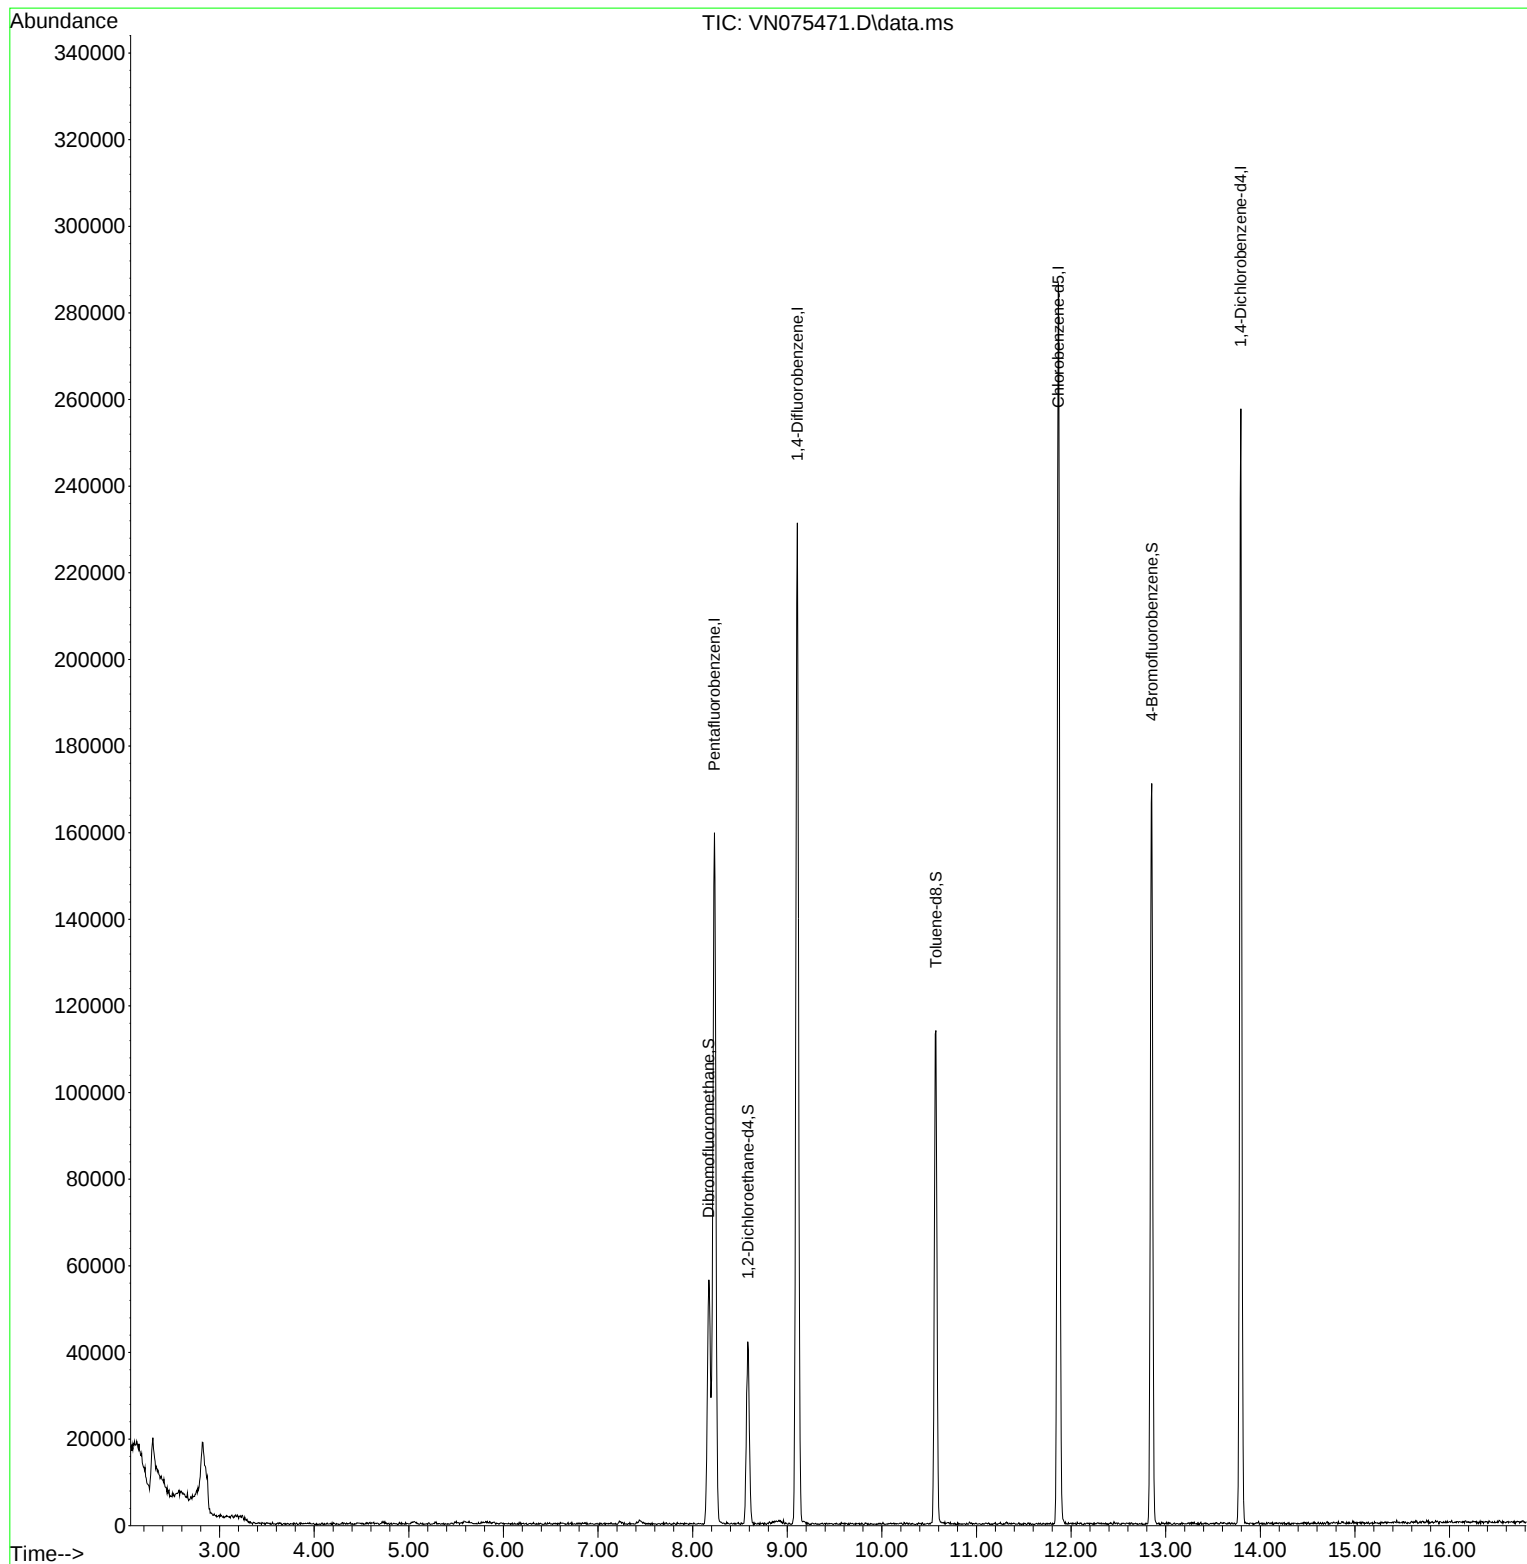


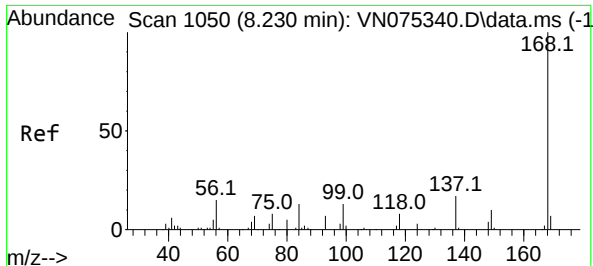

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 110
Delta R.T. -0.000 min
Lab File: VN075471.D
Acq: 29 Nov 2022 13:16




Instrument :
MSVOA_N
ClientSampleId :
TB01-11282022


Tgt Ion:168 Resp: 123027
Ion Ratio Lower Upper
168 100
99 56.8 51.6 77.4

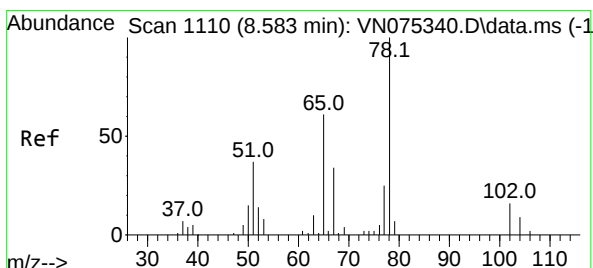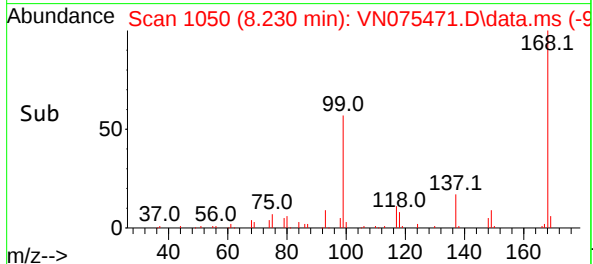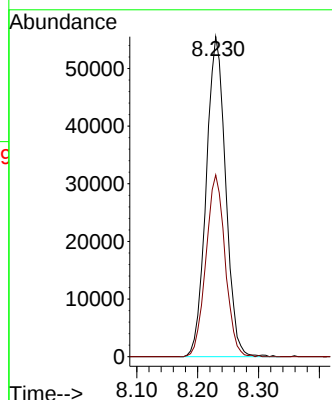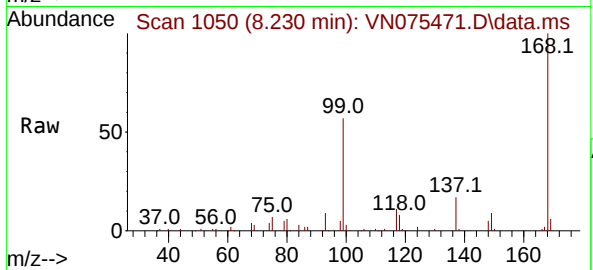

#33
1,2-Dichloroethane-d4
Concen: 51.073 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. -0.000 min
Lab File: VN075471.D
Acq: 29 Nov 2022 13:16

Tgt Ion: 65 Resp: 33728
Ion Ratio Lower Upper
65 100
67 52.8 0.0 102.0

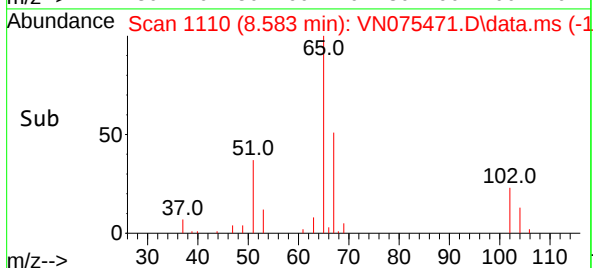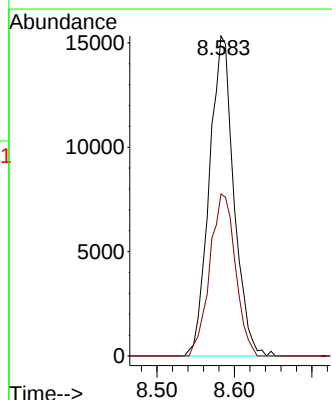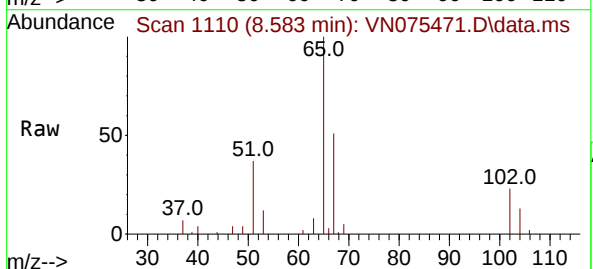

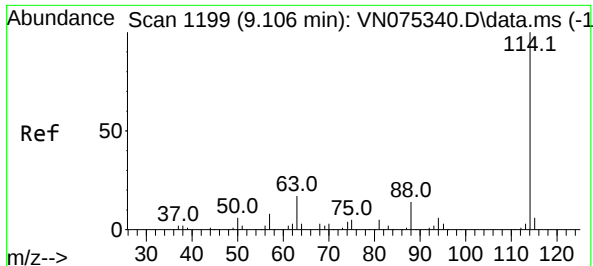

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075471.D

Acq: 29 Nov 2022 13:16

Instrument :

MSVOA_N

ClientSampleId :

TB01-11282022





Tgt Ion:114 Resp: 209809

Ion Ratio Lower Upper

114 100

63 17.7 0.0 39.6

88 13.5 0.0 29.0

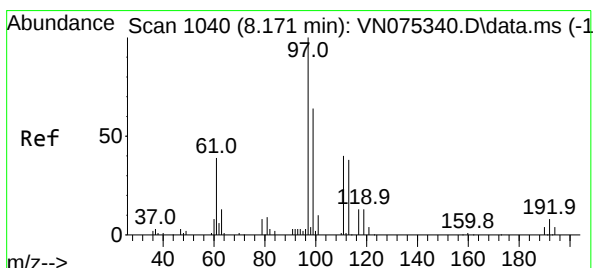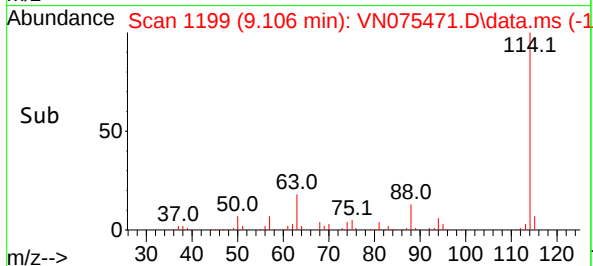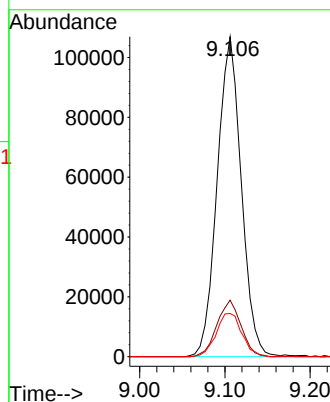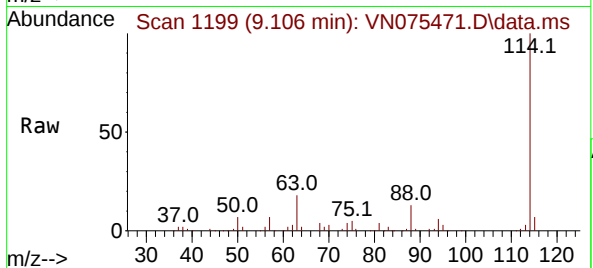

#35

Dibromofluoromethane

Concen: 50.572 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN075471.D

Acq: 29 Nov 2022 13:16




Tgt Ion:113 Resp: 41681


Ion Ratio Lower Upper

113 100

111 99.7 80.5 120.7

192 19.1 13.2 19.8


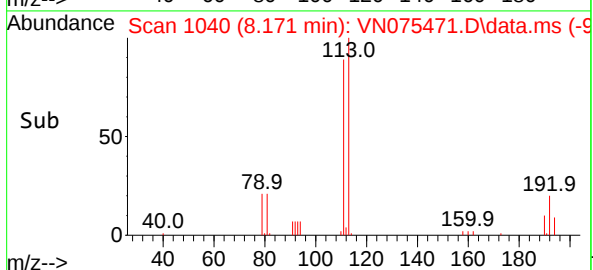
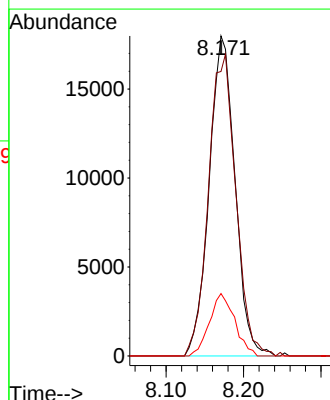
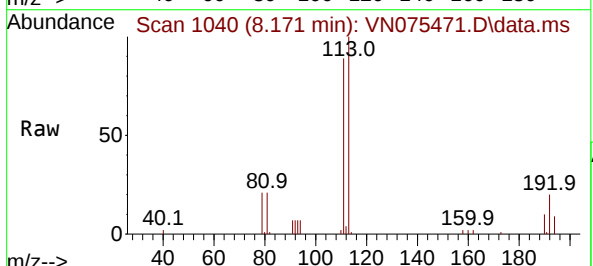


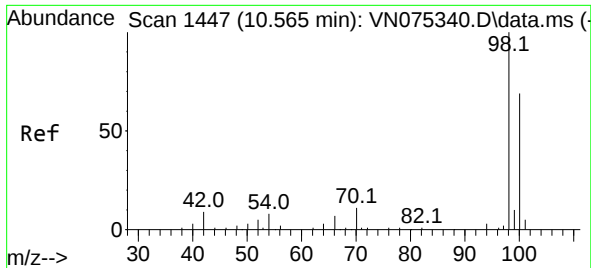

#50
Toluene-d8
Concen: 45.931 ug/l
RT: 10.571 min Scan# 1447
Delta R.T. 0.006 min
Lab File: VN075471.D
Acq: 29 Nov 2022 13:16




Instrument :
MSVOA_N
ClientSampleId :
TB01-11282022


Tgt Ion: 98 Resp: 85263
Ion Ratio Lower Upper
98 100
100 65.2 53.0 79.6

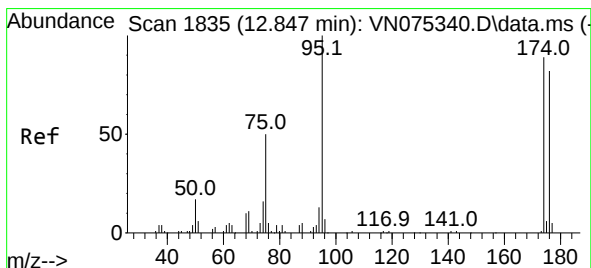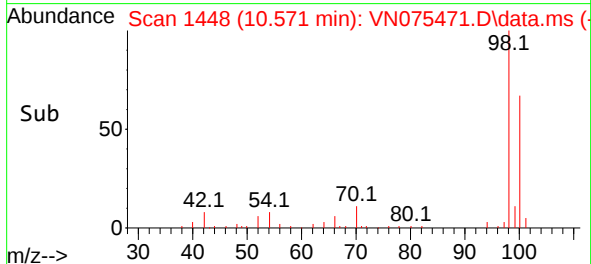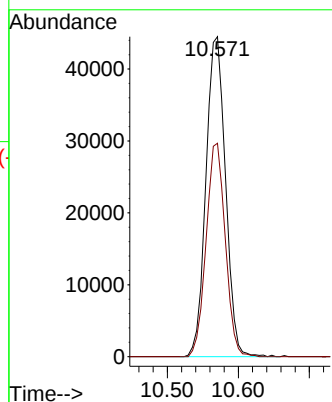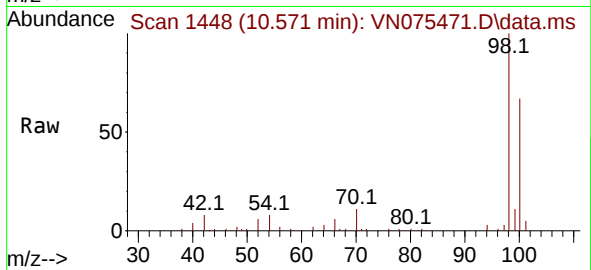

#62
4-Bromofluorobenzene
Concen: 44.601 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN075471.D
Acq: 29 Nov 2022 13:16

Tgt Ion: 95 Resp: 61111
Ion Ratio Lower Upper
95 100
174 80.2 0.0 147.4
176 77.2 0.0 142.2


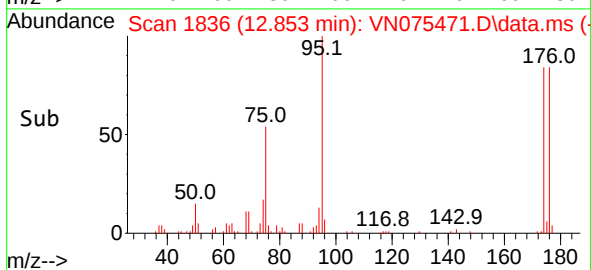
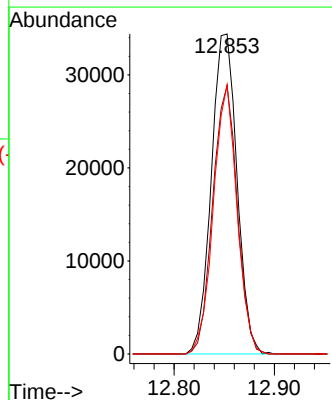
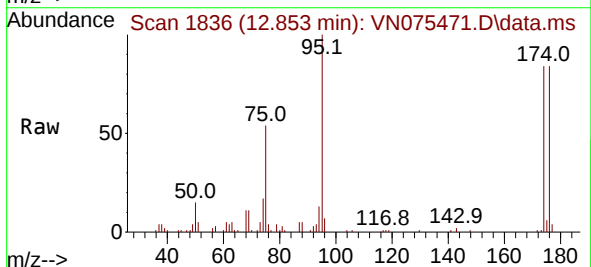


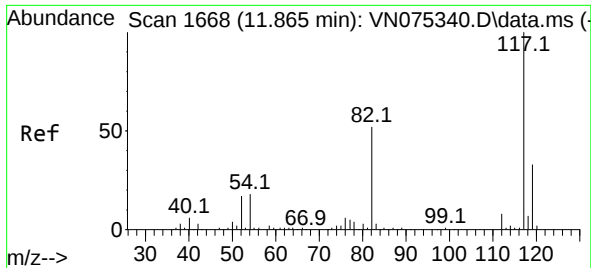

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN075471.D
Acq: 29 Nov 2022 13:16

Instrument :
MSVOA_N
ClientSampleId :
TB01-11282022

Tgt Ion:117 Resp: 178946
Ion Ratio Lower Upper
117 100
82 51.9 43.1 64.7
119 32.5 25.5 38.3

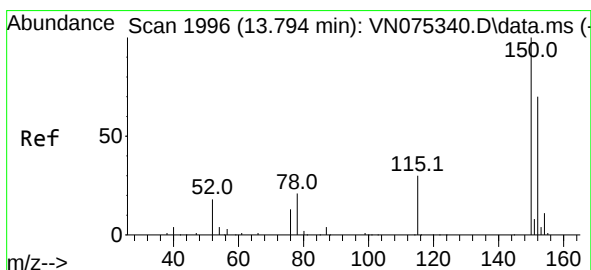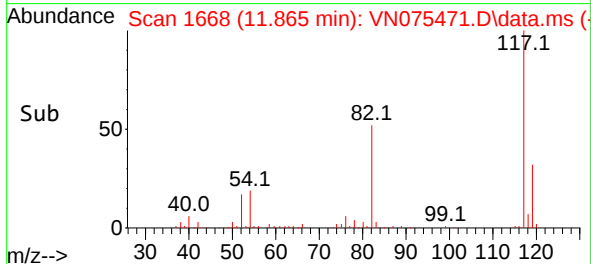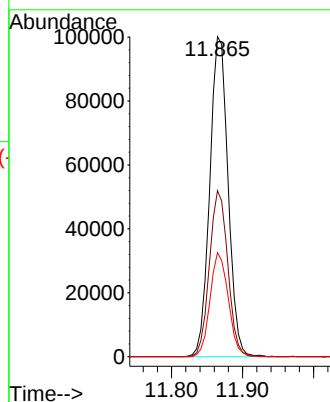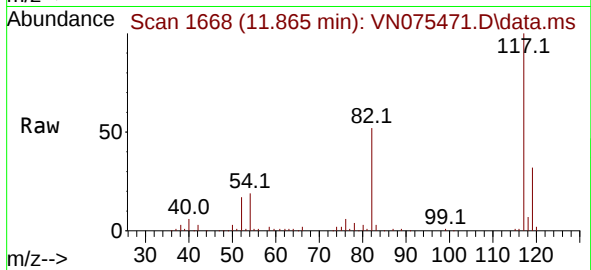

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075471.D
Acq: 29 Nov 2022 13:16

Tgt Ion:152 Resp: 69976
Ion Ratio Lower Upper
152 100
115 58.8 30.2 90.6
150 156.7 0.0 348.4

