


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112922\
Data File : VN075462.D
Acq On : 29 Nov 2022 08:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Title : SW846 8260
Last Update : Wed Nov 23 00:18:03 2022

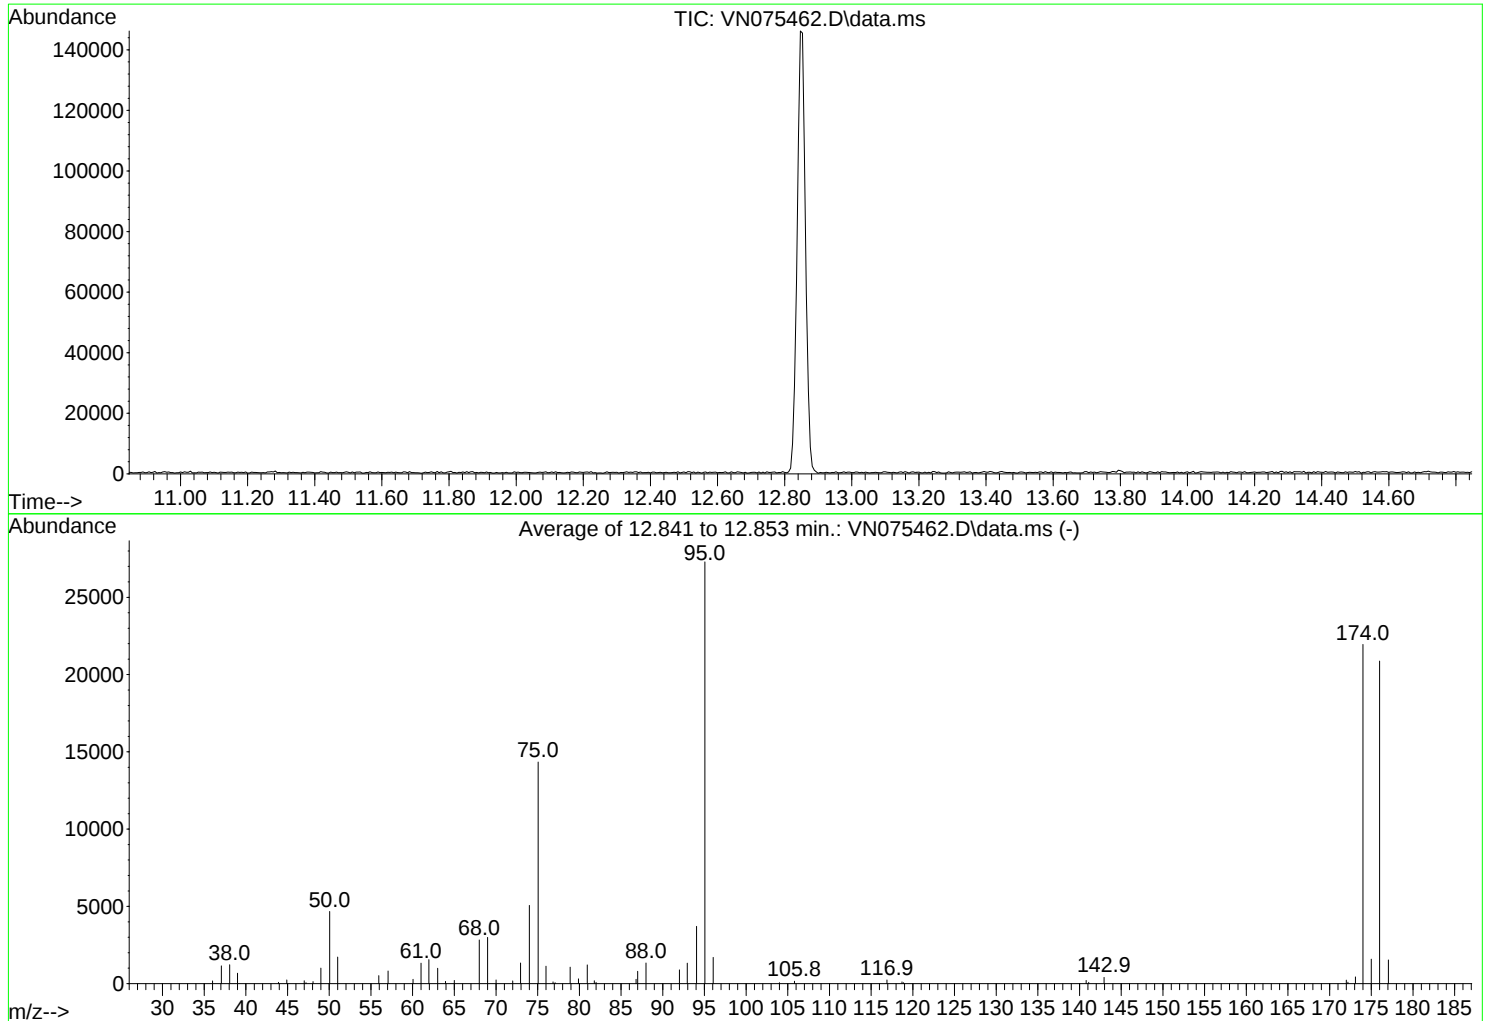

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	4672	PASS
75	95	30	60	52.5	14339	PASS
95	95	100	100	100.0	27296	PASS
96	95	5	9	6.2	1703	PASS
173	174	0.00	2	2.0	434	PASS
174	95	50	100	80.4	21949	PASS
175	174	5	9	7.2	1587	PASS
176	174	95	101	95.1	20875	PASS
177	176	5	9	7.3	1530	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	174	51.00	1721	70.00	243	81.80	19
37.05	1150	55.95	515	72.00	174	82.00	8
38.05	1227	57.05	823	72.95	1339	86.80	27
39.00	670	60.05	279	74.00	5065	87.00	80
43.90	83	61.00	1321	75.05	14339	88.00	1334
44.90	235	61.95	1551	76.00	1126	92.00	891
47.00	182	63.00	998	76.85	113	92.95	1321
47.20	62	63.95	146	77.10	67	94.05	3703
48.05	134	65.00	203	78.90	1065	95.05	27296
49.00	1009	68.00	2825	79.90	314	96.05	1703
50.05	4672	69.00	2994	80.95	1212	104.00	61

Average of 12.841 to 12.853 min.: VN075462.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.80	156	175.00	1587				
116.90	237	176.00	20875				
118.70	119	177.05	1530				
118.90	63						
140.80	212						
141.10	87						
142.95	405						
172.00	227						
172.20	91						
173.10	434						
174.00	21949						