
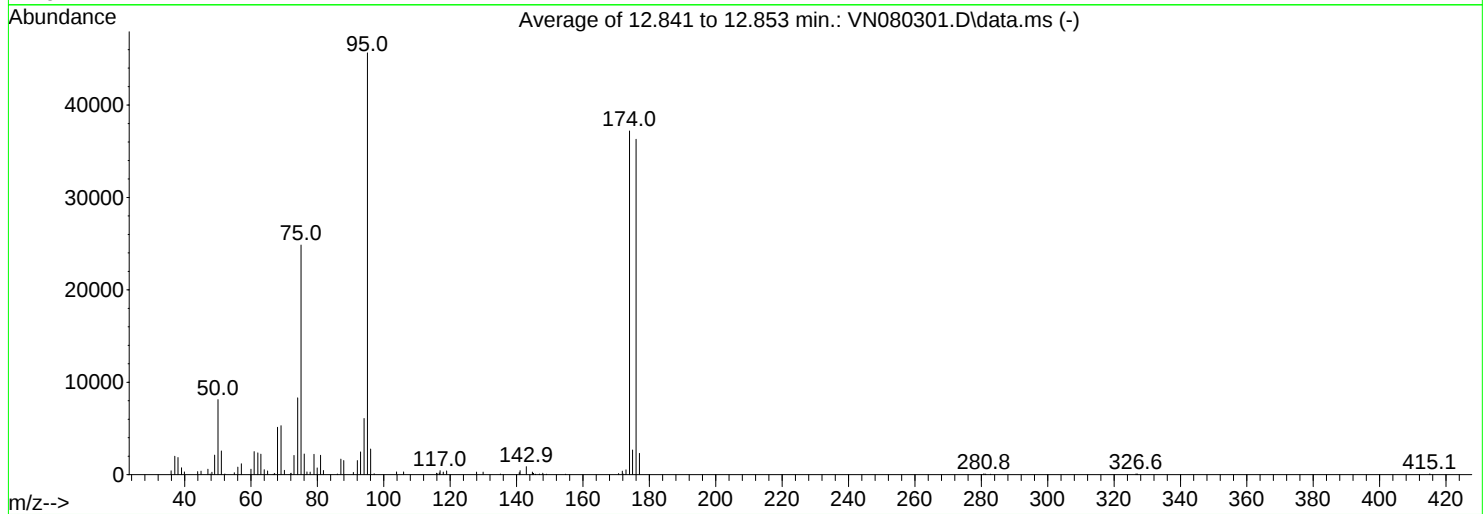


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112923\
Data File : VN080301.D
Acq On : 29 Nov 2023 08:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

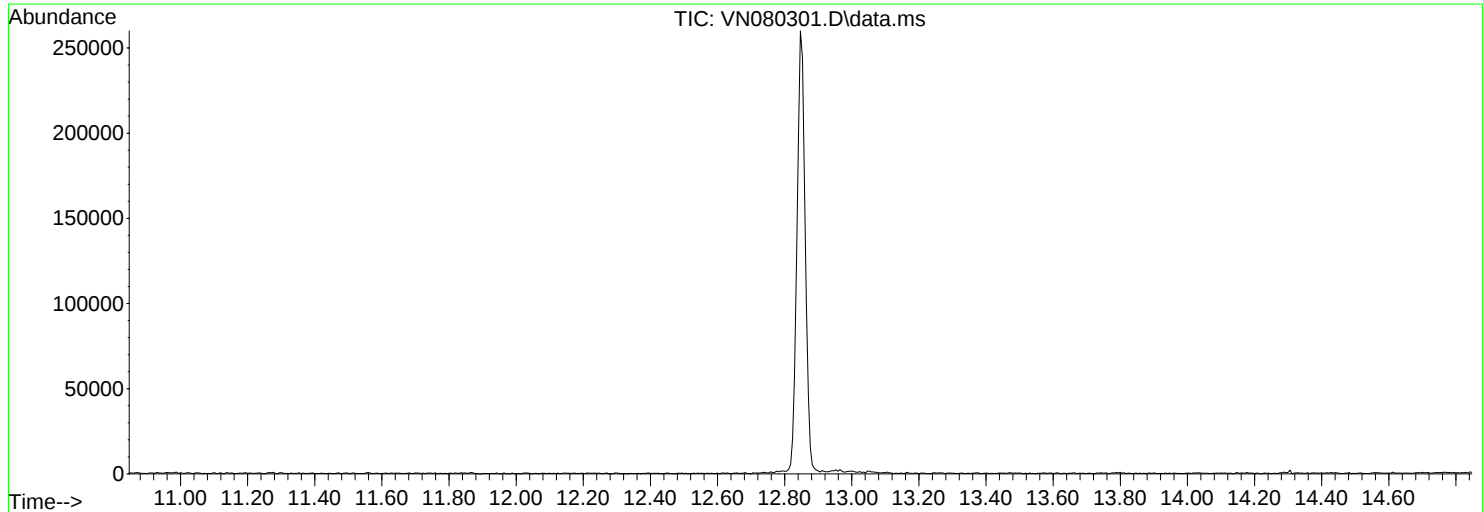

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	8126	PASS
75	95	30	60	54.5	24859	PASS
95	95	100	100	100.0	45653	PASS
96	95	5	9	6.1	2775	PASS
173	174	0.00	2	1.4	513	PASS
174	95	50	100	81.5	37208	PASS
175	174	5	9	7.2	2674	PASS
176	174	95	101	97.6	36299	PASS
177	176	5	9	6.4	2313	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	408	50.05	8126	65.00	405	76.05	2231
37.05	1994	51.05	2556	66.70	54	76.85	291
38.00	1857	52.10	72	67.10	136	77.80	281
39.05	750	54.95	200	68.00	5132	78.95	2201
39.95	291	56.05	816	69.05	5295	79.95	722
43.95	336	57.10	1177	70.05	462	80.95	2094
44.95	384	60.00	586	71.90	102	81.80	455
47.00	594	60.95	2487	72.10	165	86.00	74
47.70	75	62.05	2363	72.95	2080	87.05	1675
48.20	262	62.95	2221	74.05	8317	87.95	1525
49.05	2121	64.00	537	75.05	24859	90.85	239

Average of 12.841 to 12.853 min.: VN080301.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.05	1521	116.95	436	145.10	134	174.95	2674
93.00	2461	117.90	280	145.70	51	176.00	36299
94.05	6078	118.95	395	146.90	72	177.00	2313
95.05	45653	127.95	275	147.90	156	280.80	106
96.05	2775	129.90	282	149.00	52	281.30	74
97.10	111	135.10	73	154.80	60	282.80	60
103.85	301	140.80	230	170.75	115	326.60	87
105.95	298	141.05	443	171.85	375	327.00	77
115.90	152	142.95	873	172.10	75	415.10	95
116.20	84	144.75	272	172.95	513		
116.70	189	144.90	107	174.00	37208		

Instrument :

MSVOA_N

ClientSampleId :

BFB