


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN113018\
Data File : VN052592.D
Acq On : 30 Nov 2018 8:25
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Title : SW846 8260
Last Update : Mon Dec 03 03:24:02 2018

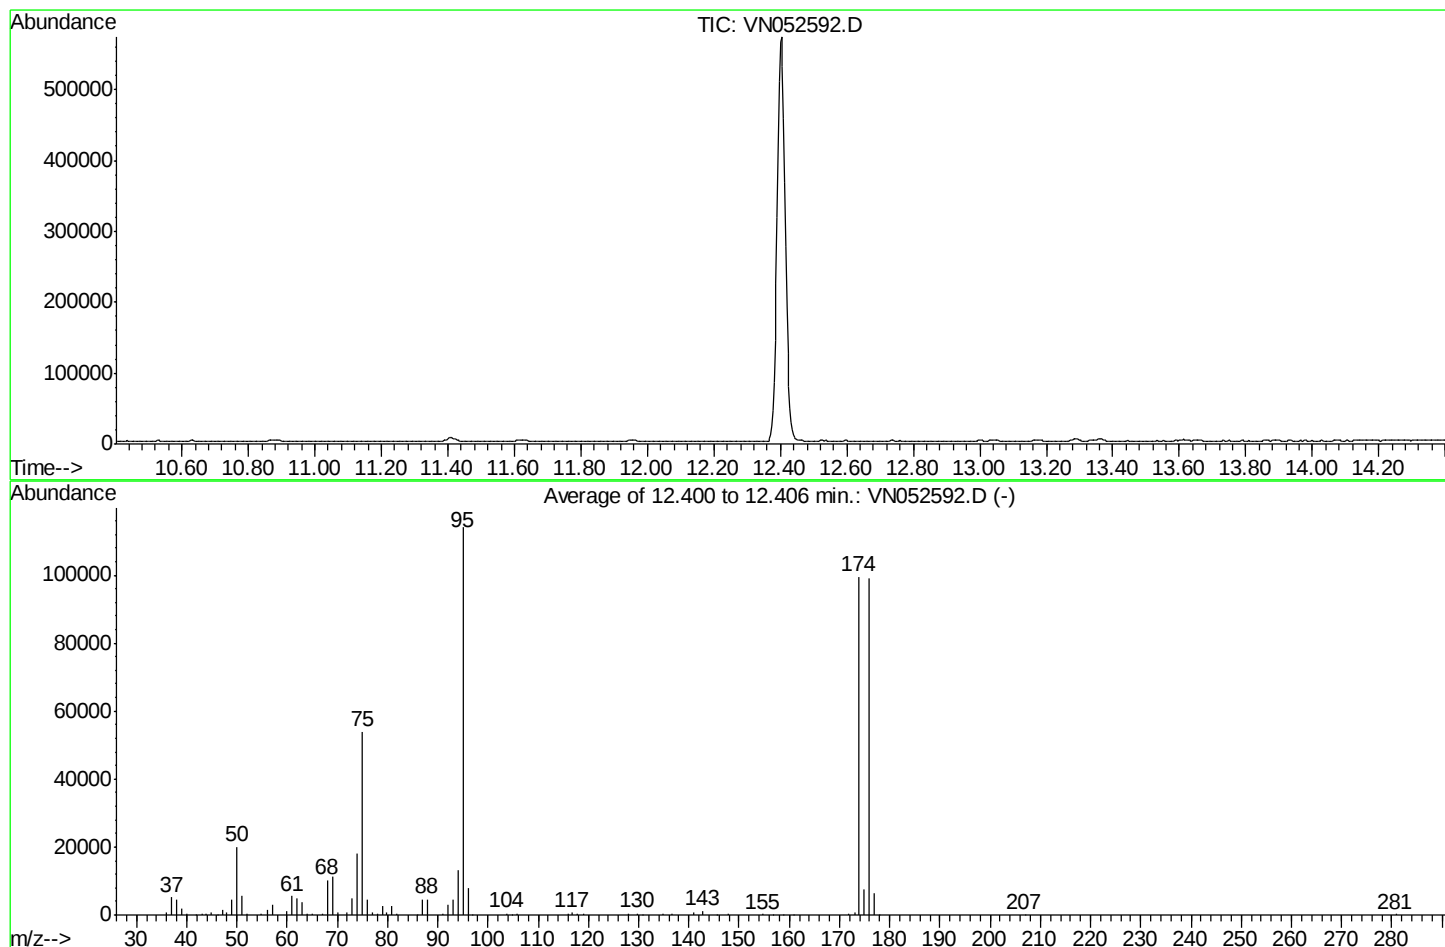

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	20114	PASS
75	95	30	60	47.2	53877	PASS
95	95	100	100	100.0	114072	PASS
96	95	5	9	7.0	7978	PASS
173	174	0.00	2	0.9	908	PASS
174	95	50	100	87.3	99530	PASS
175	174	5	9	7.4	7378	PASS
176	174	95	101	99.6	99149	PASS
177	176	5	9	6.5	6398	PASS