


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN113020\
 Data File : VN064861.D
 Acq On : 30 Nov 2020 10:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
 Title : SW846 8260
 Last Update : Mon Nov 23 13:54:12 2020

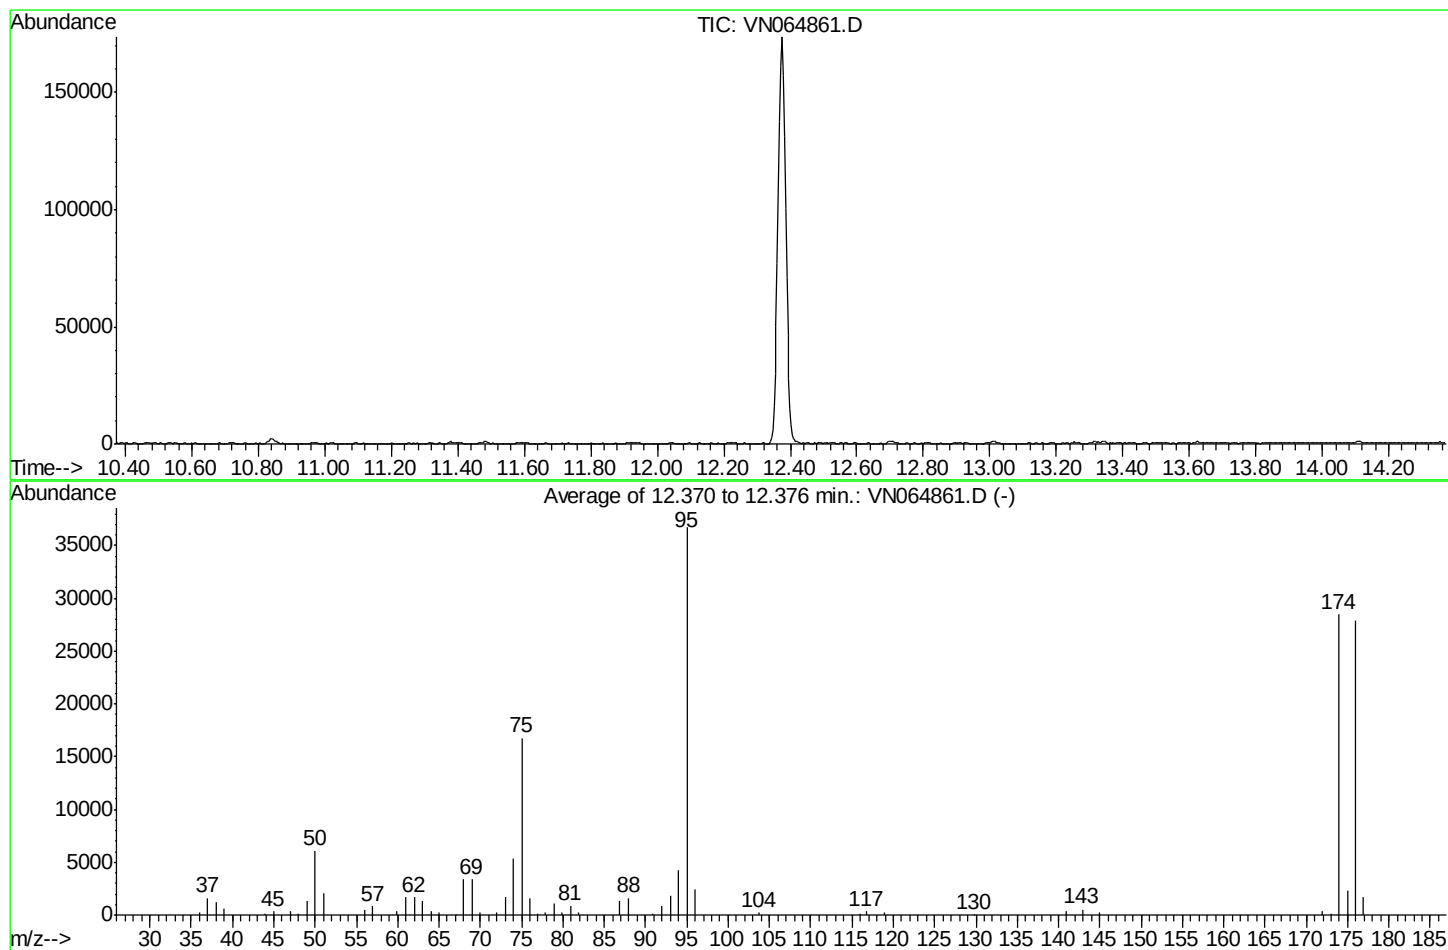

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	6118	PASS
75	95	30	60	45.7	16785	PASS
95	95	100	100	100.0	36720	PASS
96	95	5	9	6.5	2392	PASS
173	174	0.00	2	0.4	117	PASS
174	95	50	100	77.6	28482	PASS
175	174	5	9	8.1	2305	PASS
176	174	95	101	98.1	27944	PASS
177	176	5	9	6.2	1720	PASS