


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN113021\
Data File : VN069676.D
Acq On : 30 Nov 2021 9:50
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
Title : SW846 8260
Last Update : Tue Nov 09 18:18:22 2021

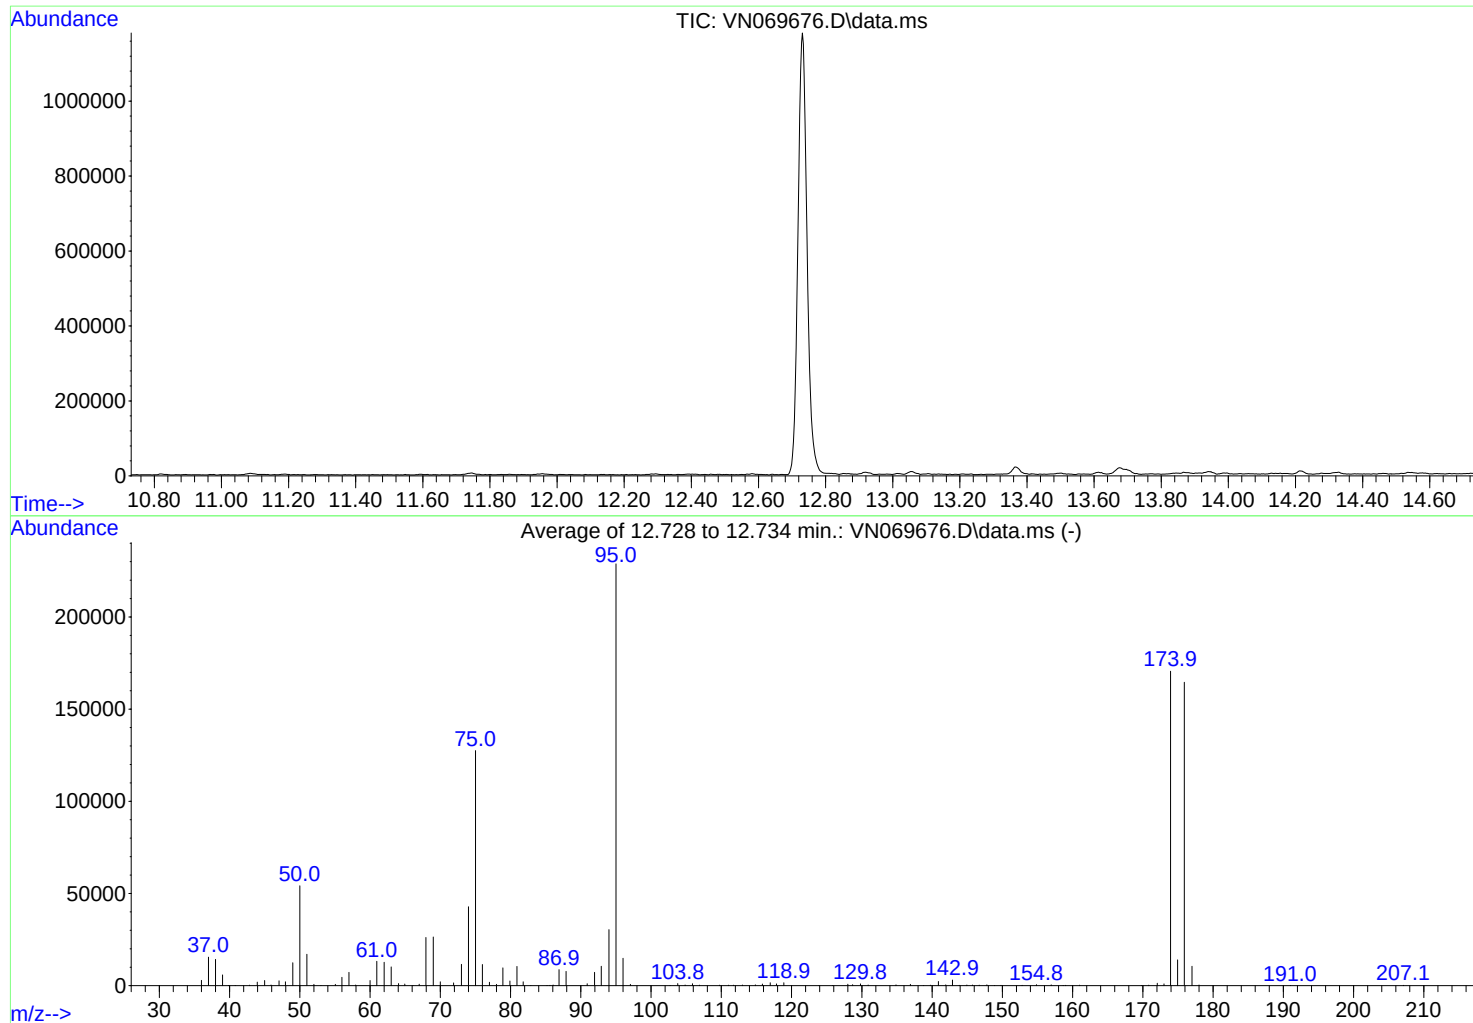

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.7	54203	PASS
75	95	30	60	55.7	127565	PASS
95	95	100	100	100.0	228843	PASS
96	95	5	9	6.5	14822	PASS
173	174	0.00	2	0.6	978	PASS
174	95	50	100	74.5	170560	PASS
175	174	5	9	8.2	13984	PASS
176	174	95	101	96.5	164587	PASS
177	176	5	9	6.4	10509	PASS