
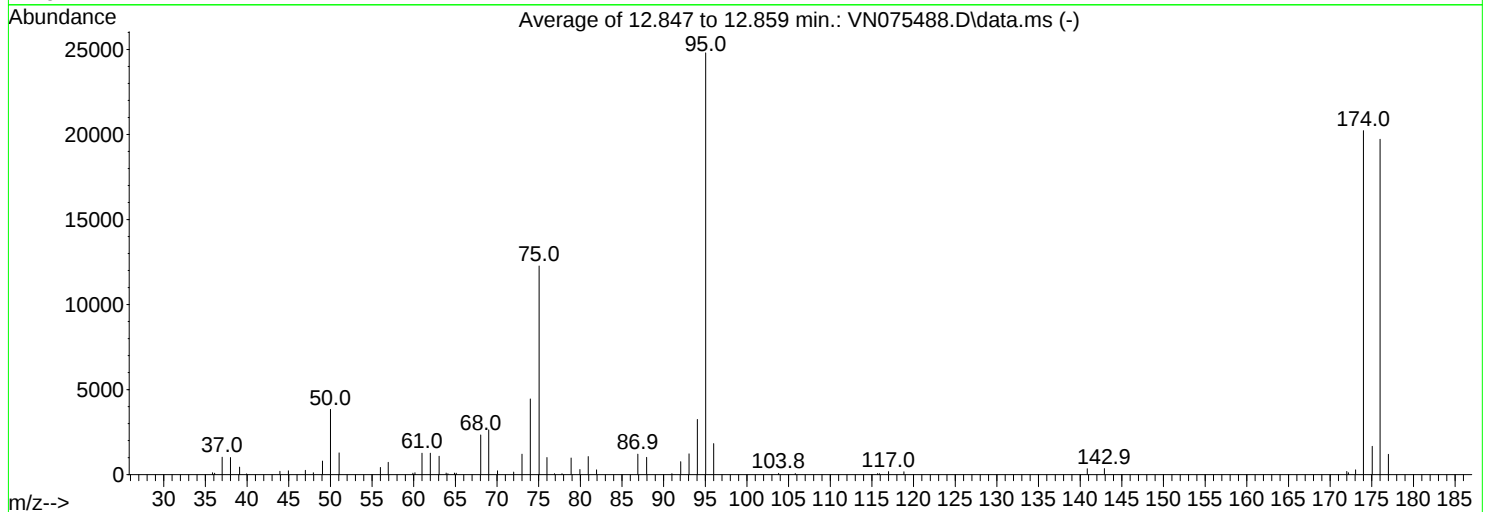


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN113022\
Data File : VN075488.D
Acq On : 30 Nov 2022 08:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Title : SW846 8260
Last Update : Wed Nov 23 00:18:03 2022

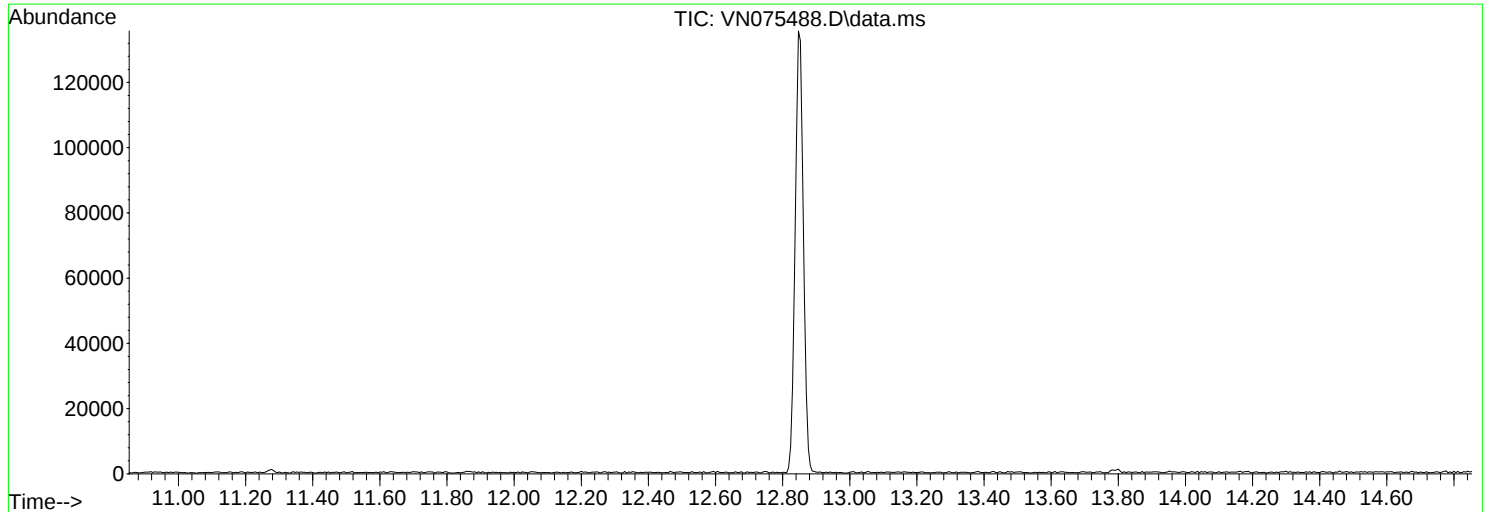

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	3835	PASS
75	95	30	60	49.5	12271	PASS
95	95	100	100	100.0	24800	PASS
96	95	5	9	7.4	1826	PASS
173	174	0.00	2	1.4	278	PASS
174	95	50	100	81.5	20224	PASS
175	174	5	9	8.2	1663	PASS
176	174	95	101	97.5	19715	PASS
177	176	5	9	6.1	1193	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	115	50.00	3835	64.90	92	77.80	51
36.10	88	51.05	1284	65.10	83	78.90	97
37.00	1025	56.00	425	68.05	2329	79.95	30
38.00	1004	56.95	726	69.00	2630	80.95	106
39.10	442	59.90	85	70.05	228	81.95	287
39.95	50	60.15	112	72.00	152	86.90	1206
43.95	198	61.00	1263	73.00	1201	87.95	1014
44.95	224	62.00	1264	74.00	4446	91.00	60
47.00	259	63.05	1081	75.05	12271	92.05	767
47.95	115	63.90	93	76.00	1005	93.05	1219
49.05	799	64.10	60	76.90	59	94.05	3243

Average of 12.847 to 12.859 min.: VN075488.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.05	24800	172.20	109				
96.00	1826	173.05	278				
103.80	76	174.00	20224				
105.80	69	175.05	1663				
115.70	67	176.00	19715				
115.90	53	177.00	1193				
117.00	180						
118.85	173						
140.85	349						
142.90	360						
172.00	186						

Instrument :

MSVOA_N

ClientSampleId :

BFB