
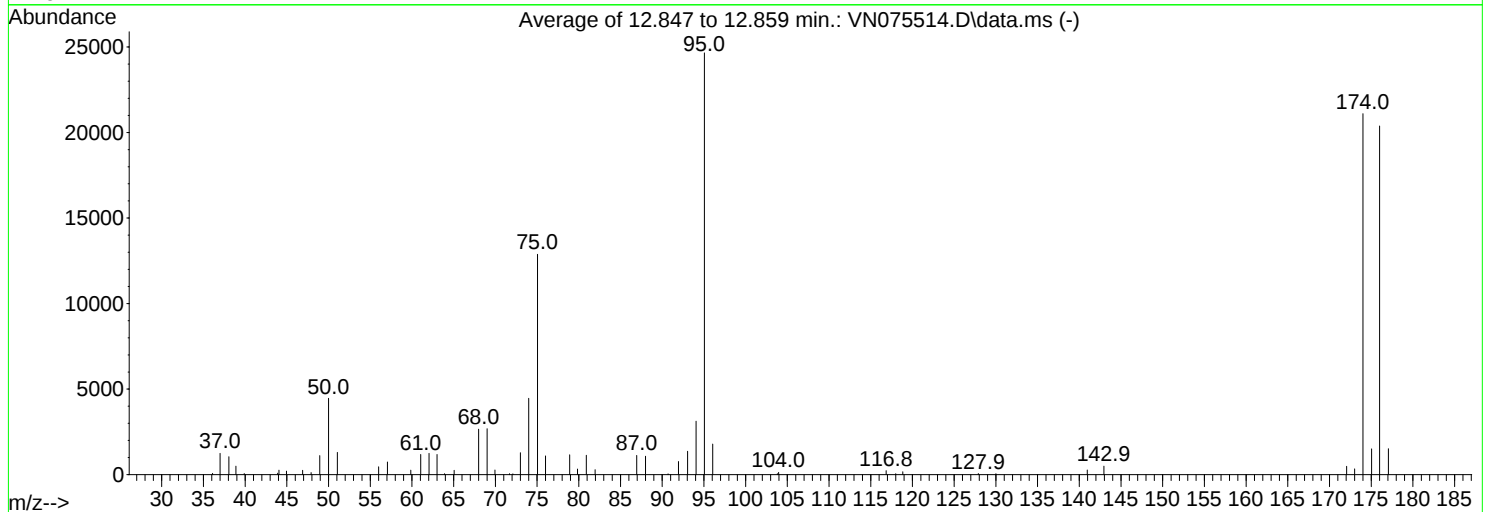


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120122\
Data File : VN075514.D
Acq On : 01 Dec 2022 09:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Title : SW846 8260
Last Update : Wed Nov 23 00:18:03 2022

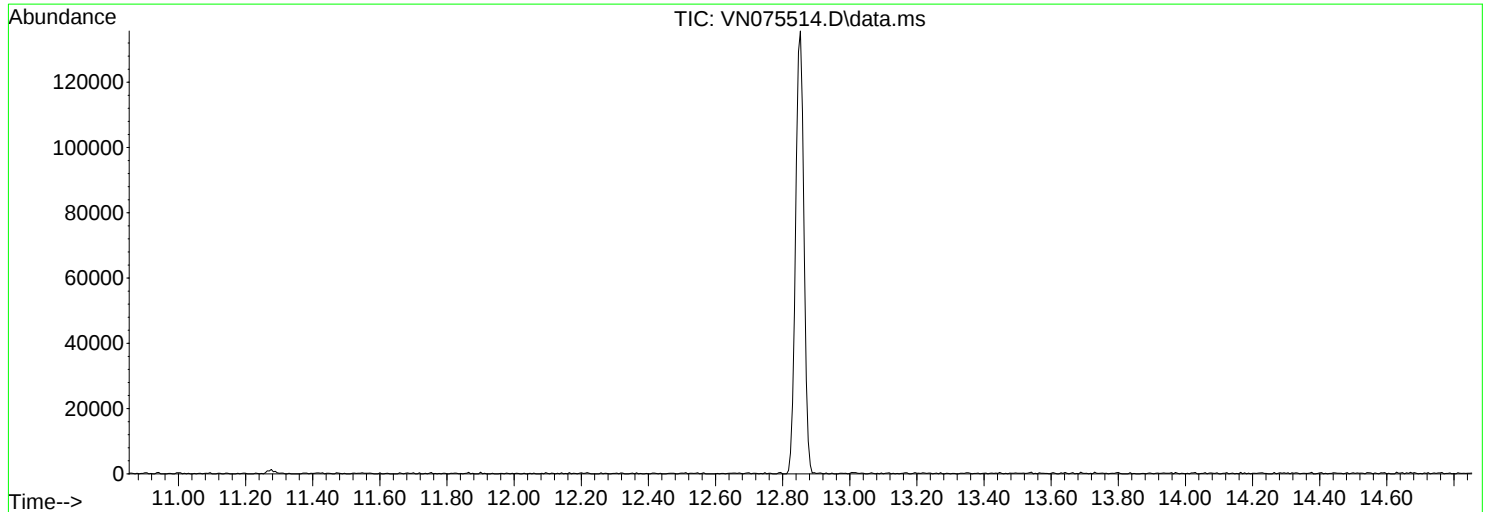

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	4458	PASS
75	95	30	60	52.3	12883	PASS
95	95	100	100	100.0	24656	PASS
96	95	5	9	7.3	1791	PASS
173	174	0.00	2	1.6	333	PASS
174	95	50	100	85.6	21096	PASS
175	174	5	9	7.1	1506	PASS
176	174	95	101	96.6	20376	PASS
177	176	5	9	7.5	1519	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	77	50.00	4458	69.00	2683	81.95	294
37.00	1245	51.05	1302	69.95	269	86.95	112
38.05	1045	56.00	456	71.70	55	88.00	107
38.90	498	57.05	738	72.10	51	90.70	5
39.90	62	59.85	261	73.00	1285	91.95	764
43.90	89	61.05	1175	74.00	4460	93.05	1368
44.05	264	62.05	1240	75.05	12883	94.05	3123
44.95	202	63.00	1175	76.00	1094	95.05	24656
46.90	252	63.90	52	78.90	1156	96.05	1791
47.90	120	65.05	254	79.85	323	103.80	53
48.95	1110	68.00	2654	80.90	1133	103.95	132

Average of 12.847 to 12.859 min.: VN075514.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.85	231	176.00	20376				
118.00	56	177.05	1519				
118.85	169						
127.90	66						
130.00	59						
140.95	271						
142.95	500						
172.05	488						
173.00	333						
174.00	21096						
175.05	1506						

Instrument :

MSVOA_N

ClientSampleId :

BFB