
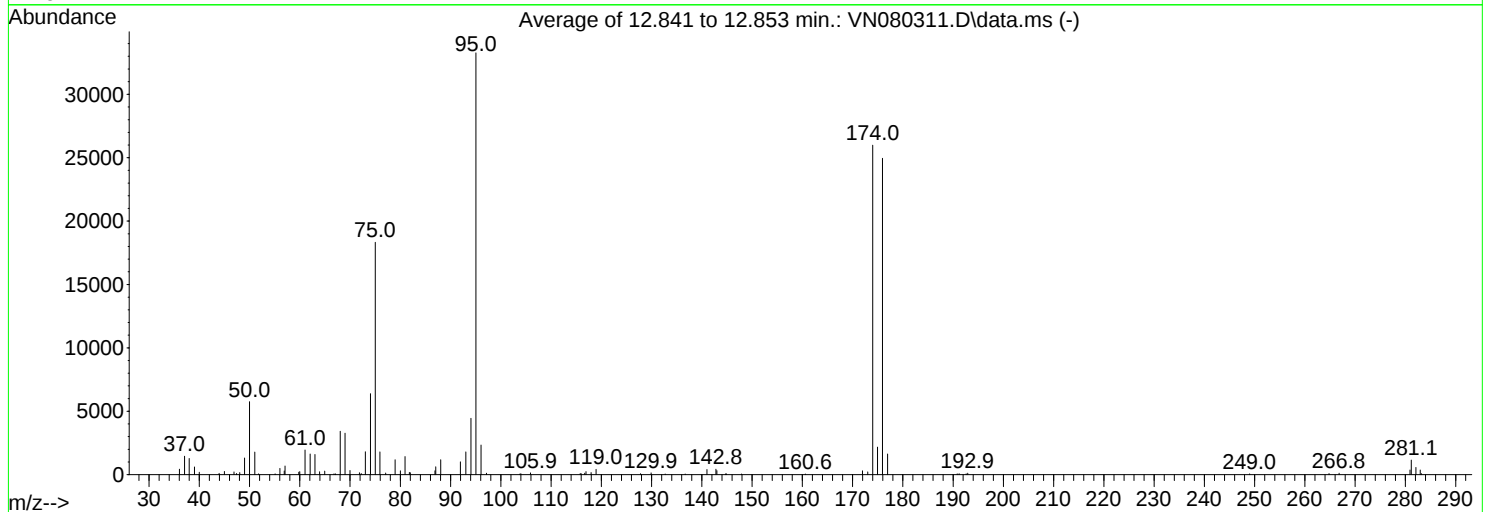


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120123\
Data File : VN080311.D
Acq On : 01 Dec 2023 09:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

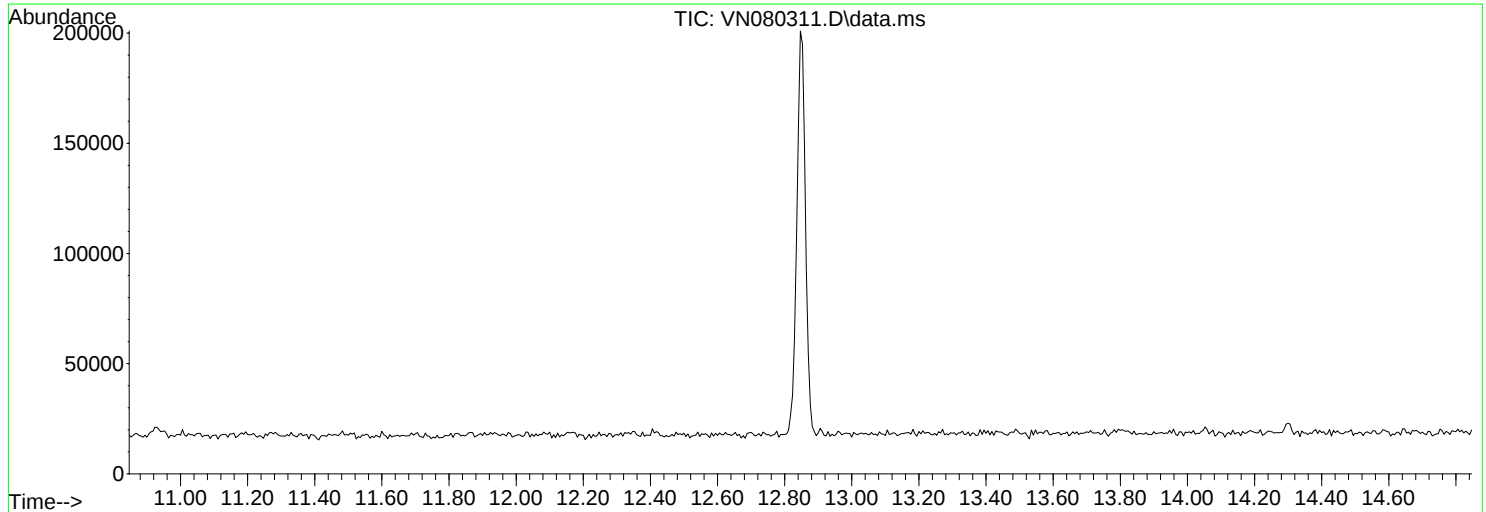

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	5763	PASS
75	95	30	60	55.1	18333	PASS
95	95	100	100	100.0	33272	PASS
96	95	5	9	7.0	2335	PASS
173	174	0.00	2	0.8	216	PASS
174	95	50	100	78.1	25995	PASS
175	174	5	9	8.4	2171	PASS
176	174	95	101	96.0	24955	PASS
177	176	5	9	6.5	1630	PASS

Average of 12.841 to 12.853 min.: VN080311.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	431	50.00	5763	63.00	1596	74.05	638
37.05	1449	51.05	1777	63.95	230	75.00	1833
38.00	1279	51.80	61	64.95	281	75.95	179
39.05	602	55.10	62	66.80	62	77.10	13
40.00	192	56.05	496	67.10	67	78.95	1181
43.95	97	56.90	289	68.05	3427	80.00	304
45.00	256	57.05	681	69.00	3269	80.95	1429
46.90	216	59.80	190	70.00	324	81.80	179
47.40	91	60.00	235	71.85	149	82.00	159
48.05	171	61.05	1947	72.20	87	86.90	300
49.00	1316	62.05	1633	73.05	1811	87.05	616

Average of 12.841 to 12.853 min.: VN080311.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.05	1170	116.00	71	143.00	312	190.80	64
91.95	1014	116.70	110	144.70	63	191.20	79
93.05	1789	116.95	234	144.90	66	192.60	59
94.05	4442	117.95	170	147.90	54	192.90	111
95.05	33272	118.95	420	160.60	54	249.00	65
96.05	2335	127.80	77	171.95	299	264.80	93
97.15	114	129.90	143	173.00	216	266.80	121
103.80	55	132.70	51	174.00	25995	280.90	371
104.00	73	136.70	57	174.95	2171	281.15	1152
105.90	141	141.00	411	175.95	24955	282.10	574
115.80	88	142.80	427	176.95	1630	282.95	362

Average of 12.841 to 12.853 min.: VN080311.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
283.20	72						

Instrument :

MSVOA_N

ClientSampleId :

BFB