

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120222\
 Data File : VN075548.D
 Acq On : 02 Dec 2022 21:40
 Operator : JC\MD
 Sample : N5865-11
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DUP-01

Manual Integrations
 APPROVED

Reviewed By :John Carlone 12/05/2022
 Supervised By :Mahesh Dadoda 12/05/2022

Quant Time: Dec 03 00:39:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.235	168	154271	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	256524	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	237699	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	109232	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	44871	54.185	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 108.380%			
35) Dibromofluoromethane	8.177	113	61002	60.535	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 121.080%			
50) Toluene-d8	10.571	98	119521	52.661	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 105.320%			
62) 4-Bromofluorobenzene	12.853	95	91063	54.358	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 108.720%			
Target Compounds					Qvalue	
3) Chloromethane	2.371	50	2233	1.521	ug/l	100
4) Vinyl Chloride	2.524	62	32907	17.789	ug/l #	86
12) 1,1-Dichloroethene	4.359	96	319551	223.676	ug/l	90
16) Acetone	4.459	43	4737	6.133	ug/l	96
17) Carbon Disulfide	4.730	76	28725	7.737	ug/l	97
21) trans-1,2-Dichloroethene	5.800	96	680728	418.104	ug/l	97
24) 1,1-Dichloroethane	6.583	63	37648	13.909	ug/l	97
27) cis-1,2-Dichloroethene	7.465	96	56086330m	30464.955	ug/l	
30) Chloroform	7.977	83	42234	13.587	ug/l	97
32) 1,1,1-Trichloroethane	8.177	97	633483	224.451	ug/l	92
44) Trichloroethene	9.347	130	38443935m	20881.612	ug/l	
52) Toluene	10.635	92	491868	113.443	ug/l	100
55) 1,1,2-Trichloroethane	11.023	97	2469	1.398	ug/l #	85
64) Tetrachloroethene	11.106	164	55039	30.321	ug/l	93
67) Ethyl Benzene	11.965	91	569667	68.021	ug/l	99
68) m/p-Xylenes	12.070	106	748637	220.127	ug/l	99
69) o-Xylene	12.400	106	351286	103.960	ug/l	96
73) Isopropylbenzene	12.700	105	8101	1.015	ug/l	94
78) n-propylbenzene	13.041	91	8734	0.981	ug/l	97
80) 1,3,5-Trimethylbenzene	13.176	105	22625	3.412	ug/l	100
83) tert-Butylbenzene	13.441	119	1636	0.271	ug/l	92
84) 1,2,4-Trimethylbenzene	13.482	105	66944	10.066	ug/l	97
85) sec-Butylbenzene	13.617	105	4005	0.488	ug/l #	59
86) p-Isopropyltoluene	13.729	119	4423m	0.641	ug/l	
89) n-Butylbenzene	14.059	91	3150	0.540	ug/l #	73
95) Naphthalene	15.647	128	60610	10.332	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120222\
Data File : VN075548.D
Acq On : 02 Dec 2022 21:40
Operator : JC\MD
Sample : N5865-11
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
DUP-01

Manual Integrations
APPROVED

Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022


Quant Time: Dec 03 00:39:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration

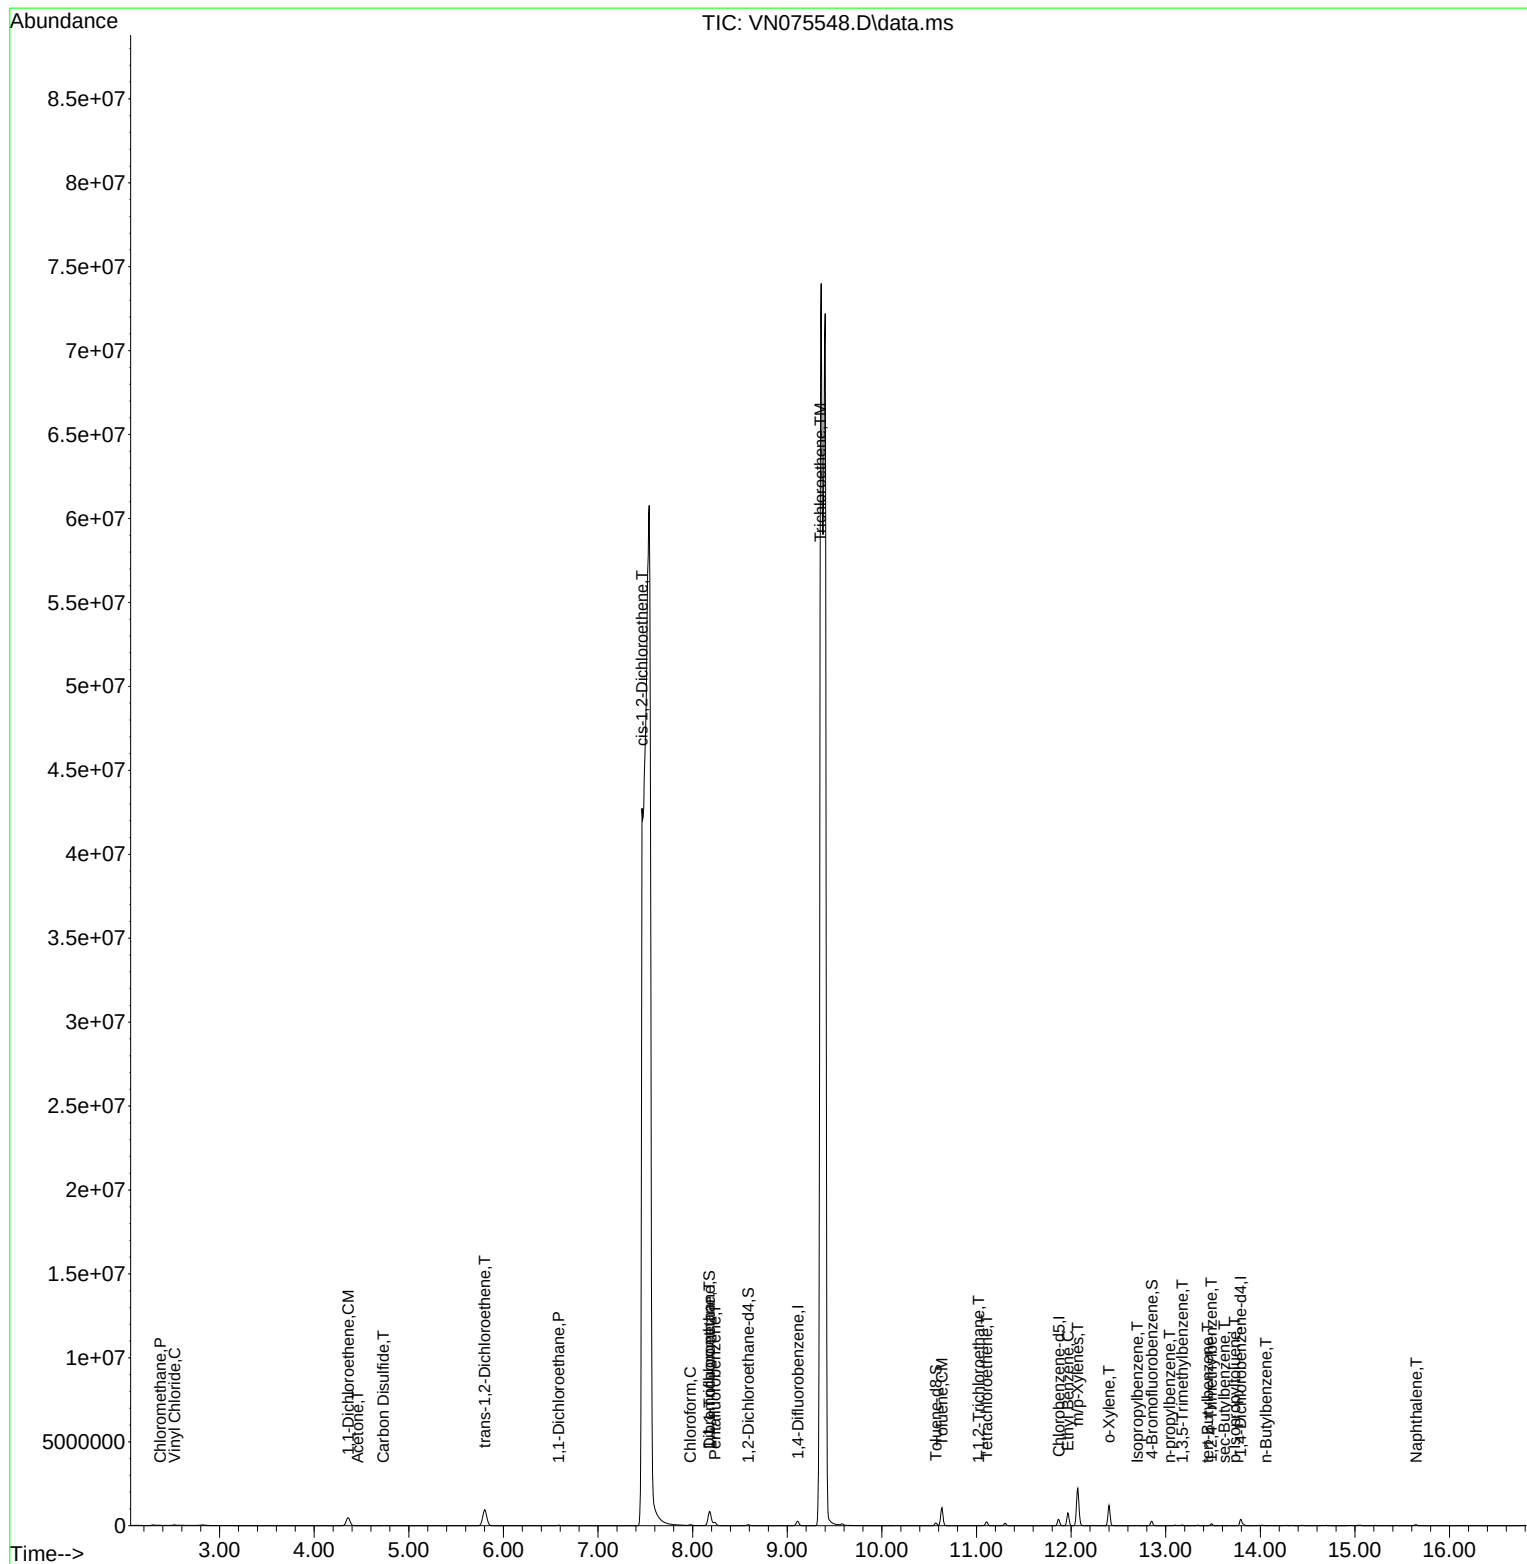



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1050
Delta R.T. 0.005 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01



Tgt Ion:168 Resp: 15427
Ion Ratio Lower Upper
168 100
99 56.3 51.6 77.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

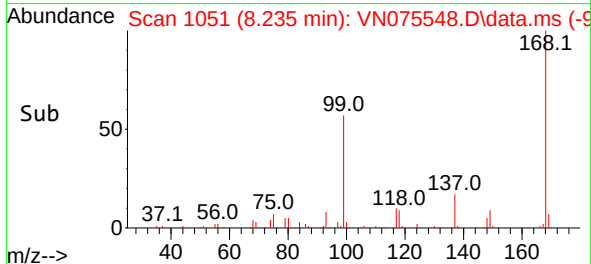

#3
Chloromethane
Concen: 1.521 ug/l
RT: 2.371 min Scan# 54
Delta R.T. 0.000 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40


Tgt Ion: 50 Resp: 2233
Ion Ratio Lower Upper
50 100
52 32.2 25.8 38.6

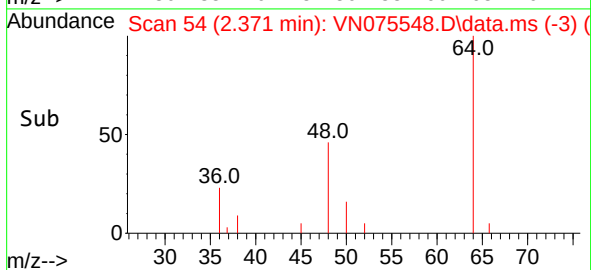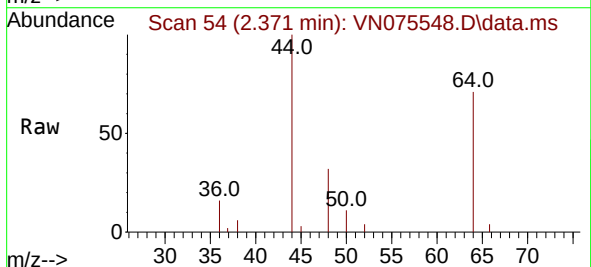



#4
 Vinyl Chloride
 Concen: 17.789 ug/l
 RT: 2.524 min Scan# 80
 Delta R.T. 0.000 min
 Lab File: VN075548.D
 Acq: 02 Dec 2022 21:40




Instrument :
 MSVOA_N
 ClientSampleId :
 DUP-01




Tgt Ion: 62 Resp: 3290
 Ion Ratio Lower Upper
 62 100
 64 37.6 24.0 36.0

Manual Integrations
 APPROVED



Reviewed By :John Carlone 12/05/2022
 Supervised By :Mahesh Dadoda 12/05/2022

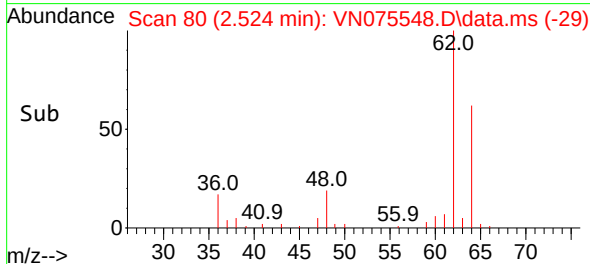


#12
 1,1-Dichloroethene
 Concen: 223.676 ug/l
 RT: 4.359 min Scan# 392
 Delta R.T. 0.017 min
 Lab File: VN075548.D
 Acq: 02 Dec 2022 21:40

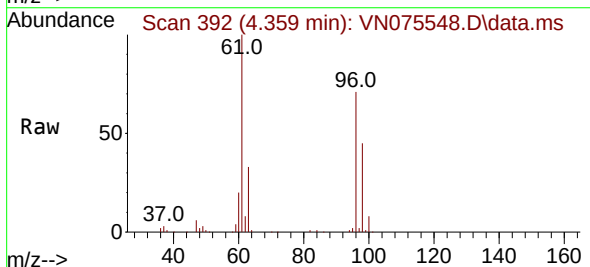

Tgt Ion: 96 Resp: 319551
 Ion Ratio Lower Upper
 96 100
 61 140.1 126.2 189.4
 98 63.7 51.5 77.3

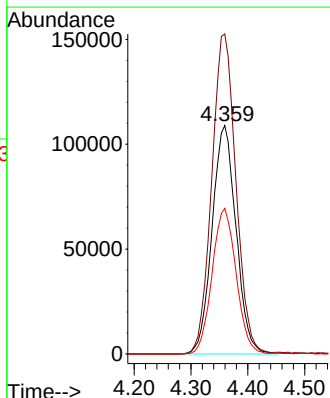







#16
Acetone
Concen: 6.133 ug/l
RT: 4.459 min Scan# 409
Delta R.T. 0.023 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

Instrument :
MSVOA_N
ClientSampleId :
DUP-01

Tgt Ion: 43 Resp: 473
Ion Ratio Lower Upper
43 100
58 29.7 25.5 38.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

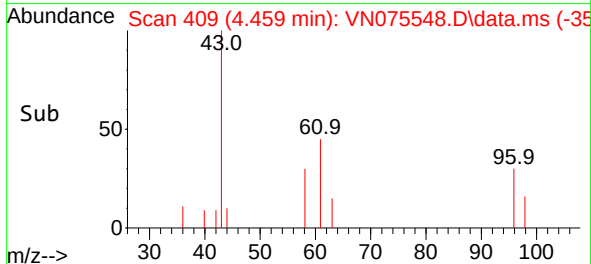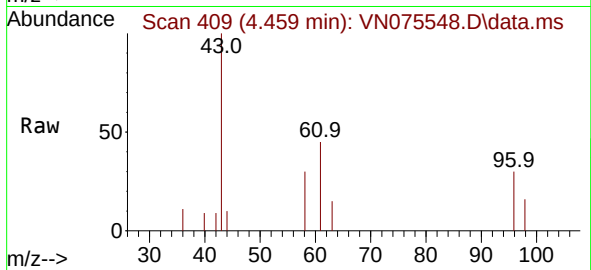

#17
Carbon Disulfide
Concen: 7.737 ug/l
RT: 4.730 min Scan# 455
Delta R.T. 0.012 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40


Tgt Ion: 76 Resp: 28725
Ion Ratio Lower Upper
76 100
78 8.1 7.4 11.2

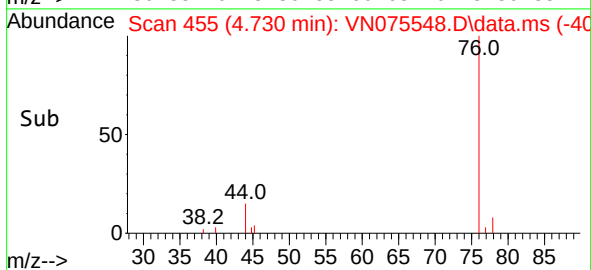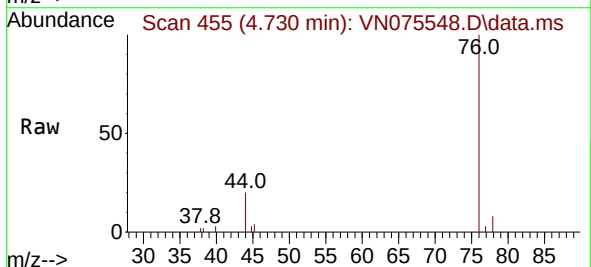

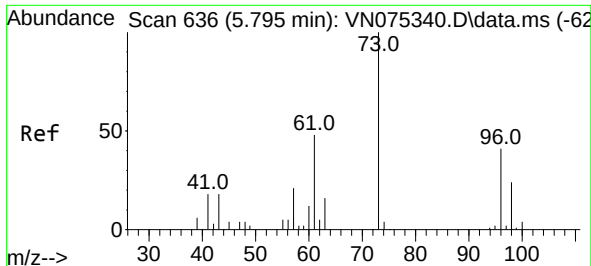

#21
trans-1,2-Dichloroethene
Concen: 418.104 ug/l
RT: 5.800 min Scan# 61
Delta R.T. 0.005 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01



Tgt Ion: 96 Resp: 680728
Ion Ratio Lower Upper
96 100
61 119.0 99.9 149.9
98 64.5 51.5 77.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

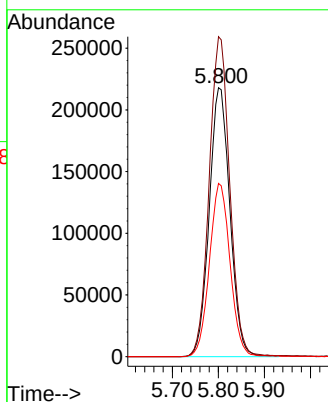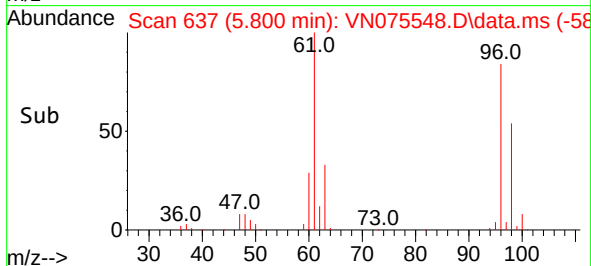

#24
1,1-Dichloroethane
Concen: 13.909 ug/l
RT: 6.583 min Scan# 770
Delta R.T. 0.006 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40


Tgt Ion: 63 Resp: 37648
Ion Ratio Lower Upper
63 100
98 8.5 3.6 10.8
100 4.5 2.4 7.2

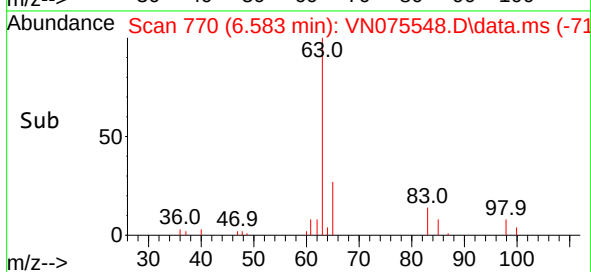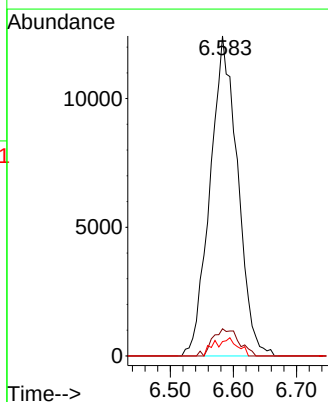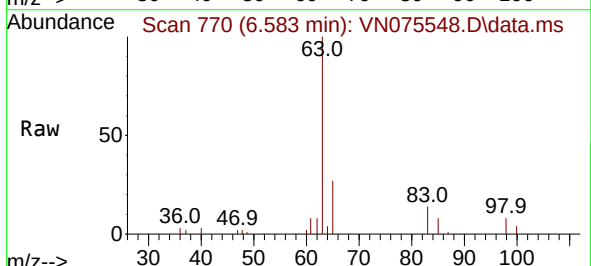



#27
cis-1,2-Dichloroethene
Concen: 30464.955 ug/l m
RT: 7.465 min Scan# 91
Delta R.T. -0.029 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01



Tgt Ion: 96 Resp: 56086330
Ion Ratio Lower Upper
96 100
61 0.0 0.0 278.8
98 0.0 0.0 128.4




Manual Integrations
APPROVED


Reviewed By : John Carlone 12/05/2022
Supervised By : Mahesh Dadoda 12/05/2022

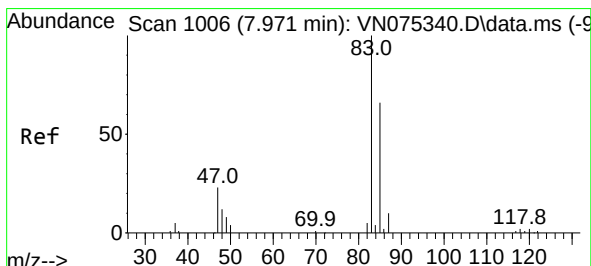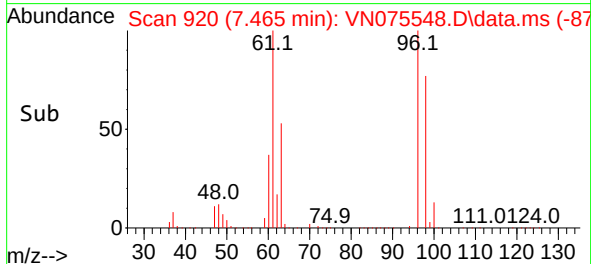

#30
Chloroform
Concen: 13.587 ug/l
RT: 7.977 min Scan# 1007
Delta R.T. 0.006 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40


Tgt Ion: 83 Resp: 42234
Ion Ratio Lower Upper
83 100
85 66.8 51.4 77.0

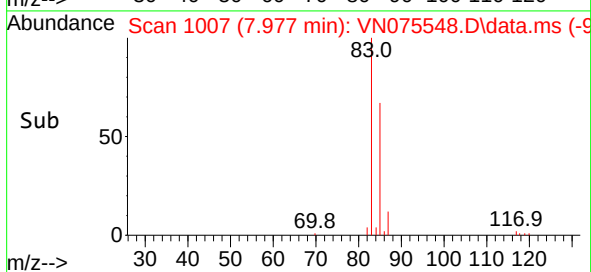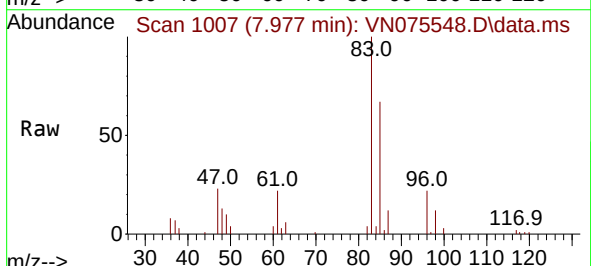



#32
1,1,1-Trichloroethane
Concen: 224.451 ug/l
RT: 8.177 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01



Tgt Ion: 97 Resp: 63348
Ion Ratio Lower Upper
97 100
99 67.6 50.2 75.2
61 39.8 37.0 55.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

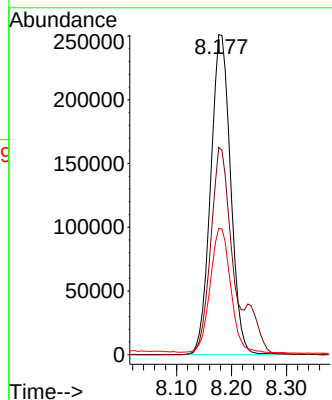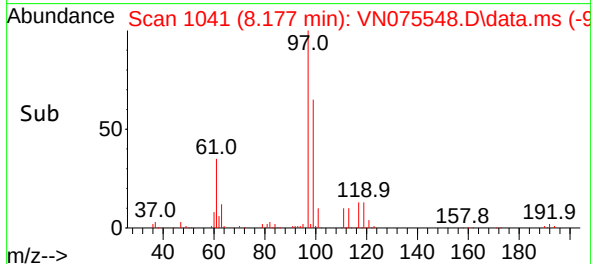

#33
1,2-Dichloroethane-d4
Concen: 54.185 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. 0.005 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

Tgt Ion: 65 Resp: 44871
Ion Ratio Lower Upper
65 100
67 52.2 0.0 102.0

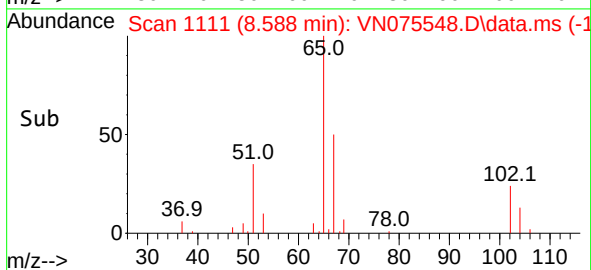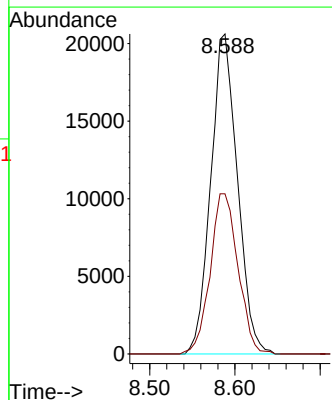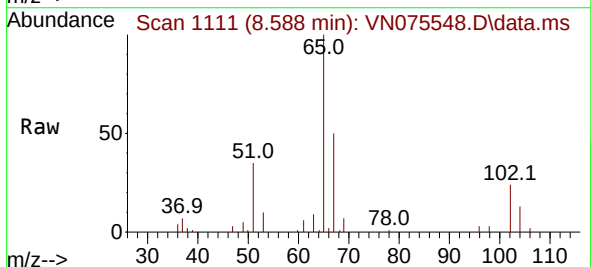

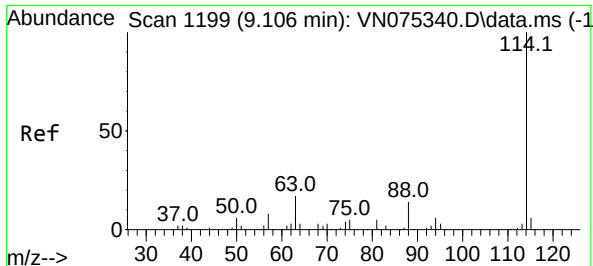

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1199

Delta R.T. 0.006 min

Lab File: VN075548.D

Acq: 02 Dec 2022 21:40

Instrument :

MSVOA_N

ClientSampleId :

DUP-01





Tgt Ion:114 Resp: 256524
 Ion Ratio Lower Upper
 114 100
 63 17.1 0.0 39.6
 88 14.1 0.0 29.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 12/05/2022

Supervised By :Mahesh Dadoda 12/05/2022

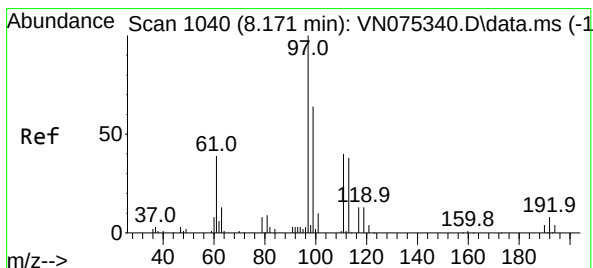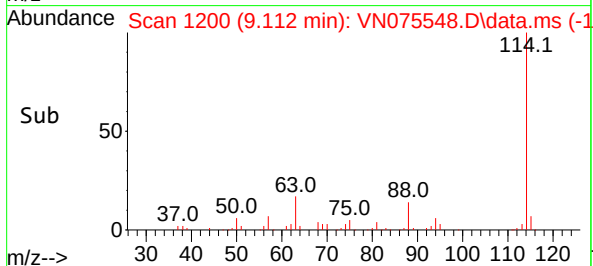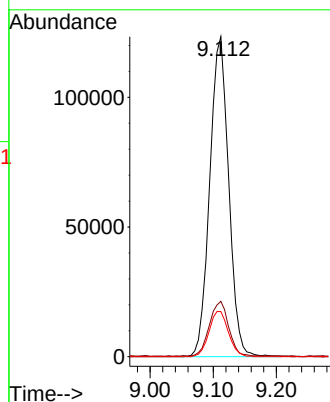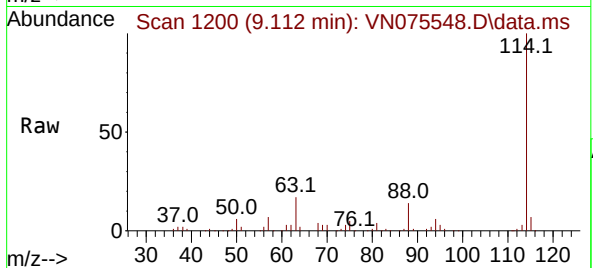

#35

Dibromofluoromethane

Concen: 60.535 ug/l




RT: 8.177 min Scan# 1041


Delta R.T. 0.006 min

Lab File: VN075548.D

Acq: 02 Dec 2022 21:40


Tgt Ion:113 Resp: 61002
 Ion Ratio Lower Upper
 113 100
 111 101.6 80.5 120.7
 192 20.1 13.2 19.8#

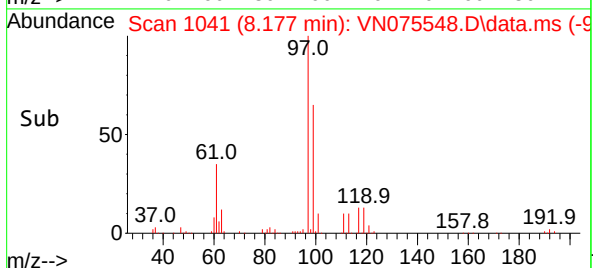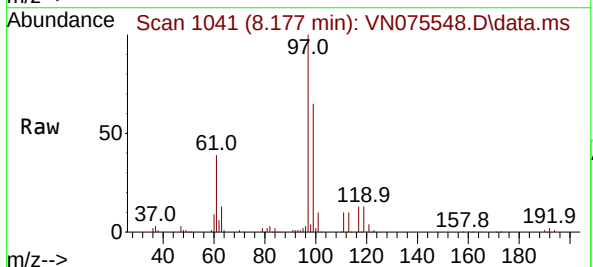

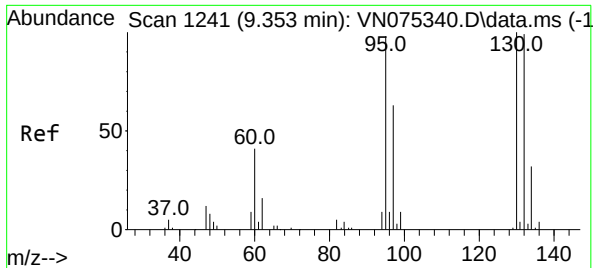

#44
Trichloroethene
Concen: 20881.612 ug/l m
RT: 9.347 min Scan# 1241
Delta R.T. -0.006 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01

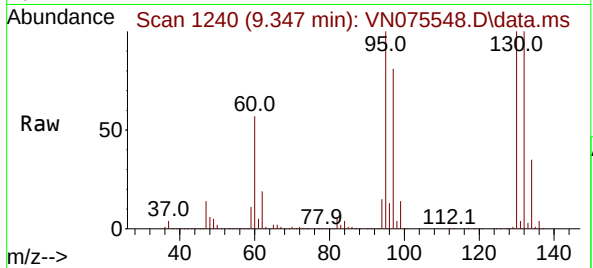

Tgt Ion:130 Resp:3844393
Ion Ratio Lower Upper
130 100
95 100.0 0.0 198.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

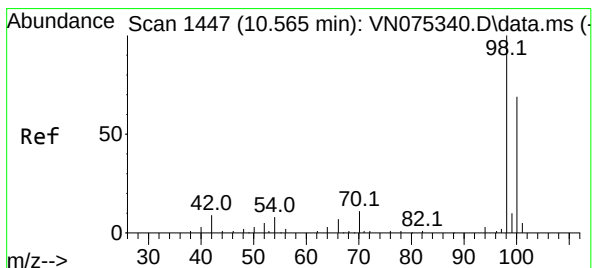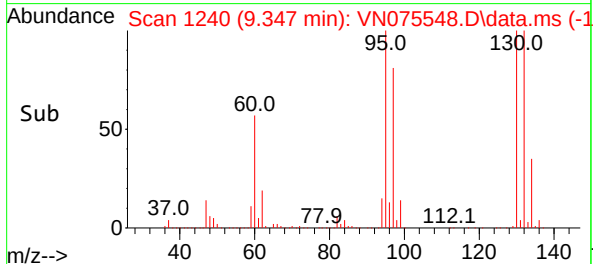

#50
Toluene-d8
Concen: 52.661 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. 0.006 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

Tgt Ion: 98 Resp: 119521
Ion Ratio Lower Upper
98 100
100 64.4 53.0 79.6

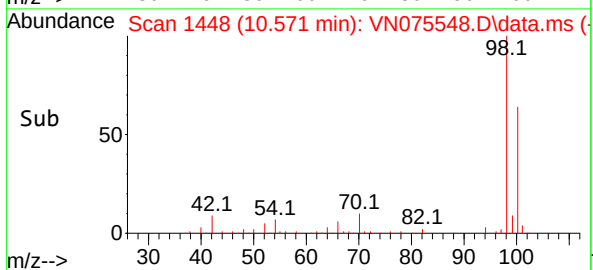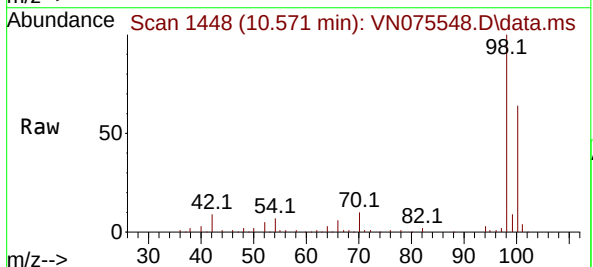



#52

Toluene

Concen: 113.443 ug/l

RT: 10.635 min Scan# 1458

Delta R.T. 0.005 min

Lab File: VN075548.D


Acq: 02 Dec 2022 21:40

Instrument :

MSVOA_N

ClientSampleId :

DUP-01



Tgt Ion: 92 Resp: 491868

Ion Ratio Lower Upper

92 100



91 169.1 135.4 203.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 12/05/2022

Supervised By :Mahesh Dadoda 12/05/2022

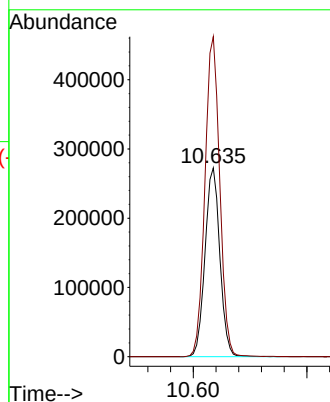

#55

1,1,2-Trichloroethane

Concen: 1.398 ug/l

RT: 11.023 min Scan# 1525

Delta R.T. 0.005 min

Lab File: VN075548.D

Acq: 02 Dec 2022 21:40

Tgt Ion: 97 Resp: 2469




Ion Ratio Lower Upper


97 100

83 78.6 65.9 98.9

85 76.5 40.4 60.6#


99 67.2 46.4 69.6

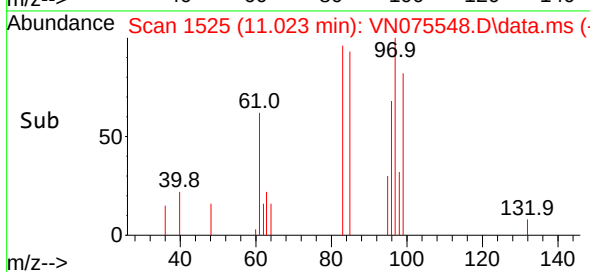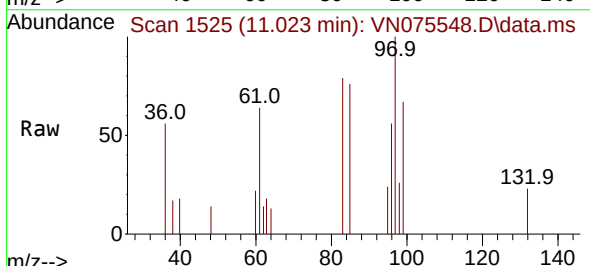

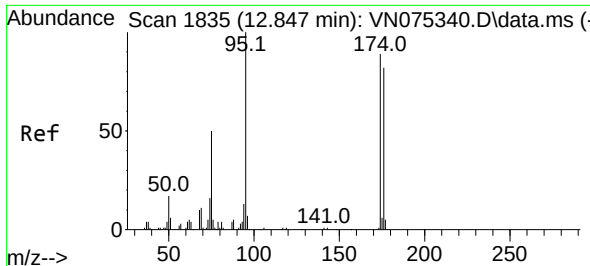

#62
4-Bromofluorobenzene
Concen: 54.358 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01




Tgt Ion: 95 Resp: 9106
Ion Ratio Lower Upper
95 100
174 88.7 0.0 147.4
176 86.4 0.0 142.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

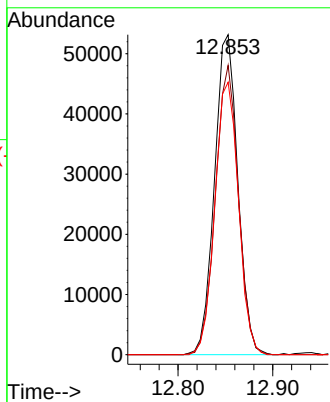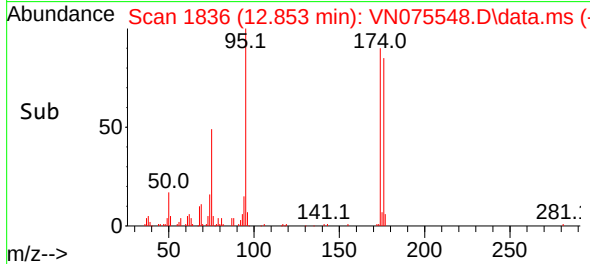


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1669
Delta R.T. 0.005 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

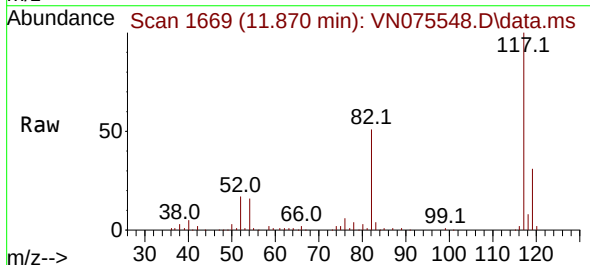


Tgt Ion:117 Resp: 237699
Ion Ratio Lower Upper
117 100
82 51.2 43.1 64.7
119 31.1 25.5 38.3

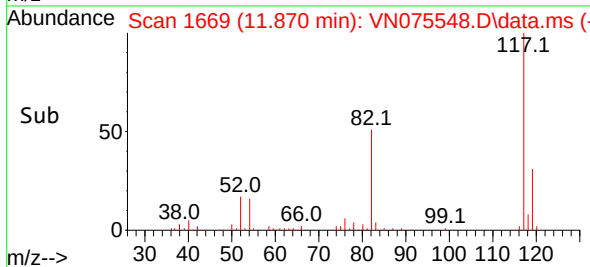

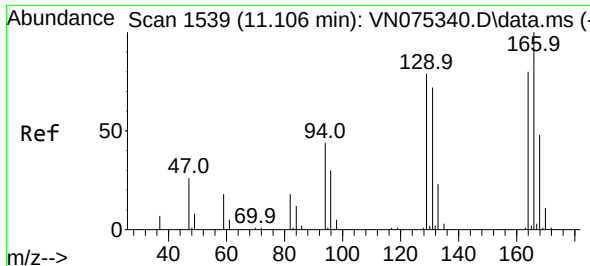

#64
Tetrachloroethene
Concen: 30.321 ug/l
RT: 11.106 min Scan# 1539
Delta R.T. -0.000 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01




Tgt Ion:164 Resp: 55039
Ion Ratio Lower Upper
164 100
166 129.0 106.5 159.7
129 96.1 81.9 122.9
131 90.7 81.4 122.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

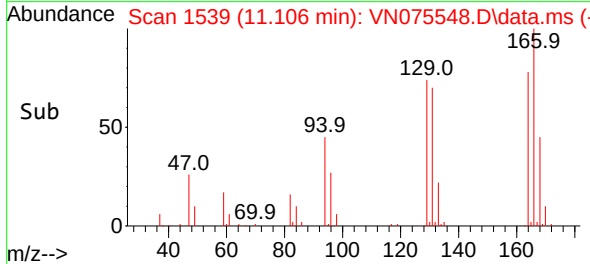


#67
Ethyl Benzene
Concen: 68.021 ug/l
RT: 11.965 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

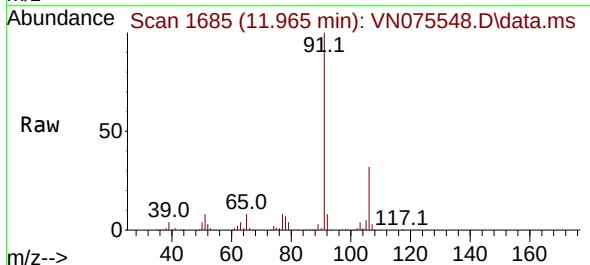

Tgt Ion: 91 Resp: 569667
Ion Ratio Lower Upper
91 100
106 31.6 24.9 37.3

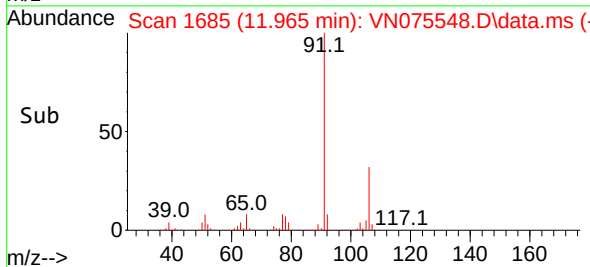







#68
m/p-Xylenes
Concen: 220.127 ug/l
RT: 12.070 min Scan# 1703
Delta R.T. -0.001 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

Instrument :
MSVOA_N
ClientSampleId :
DUP-01

Tgt Ion:106 Resp: 74863
Ion Ratio Lower Upper
106 100
91 193.6 156.0 234.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

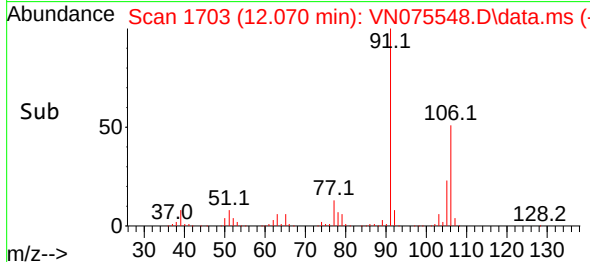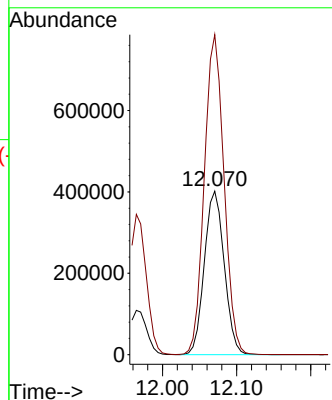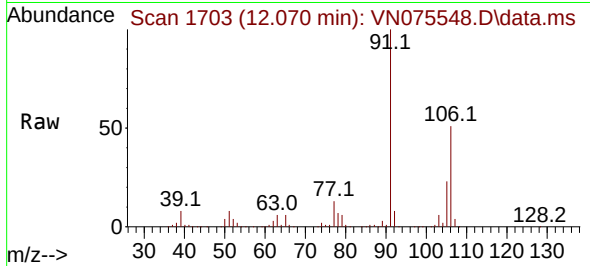

#69
o-Xylene
Concen: 103.960 ug/l
RT: 12.400 min Scan# 1759
Delta R.T. -0.000 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40


Tgt Ion:106 Resp: 351286
Ion Ratio Lower Upper
106 100
91 204.7 105.2 315.5

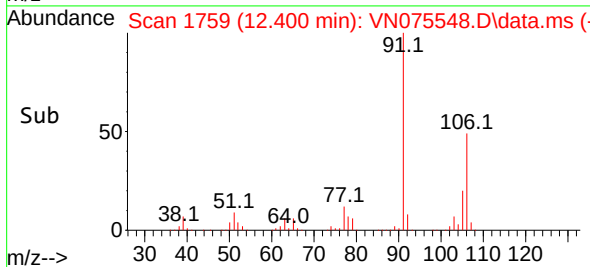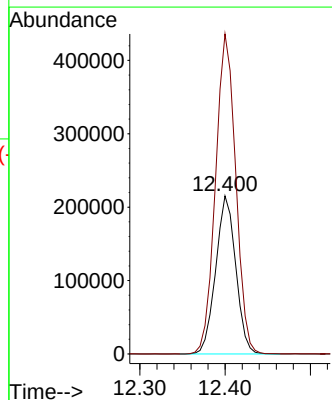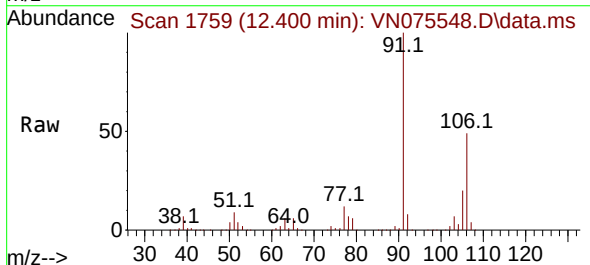

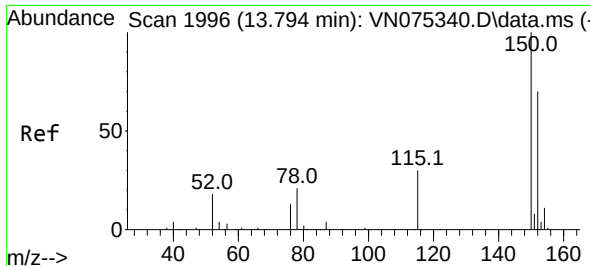

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01




Tgt Ion:152 Resp: 10923
Ion Ratio Lower Upper
152 100
115 59.4 30.2 90.6
150 158.5 0.0 348.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

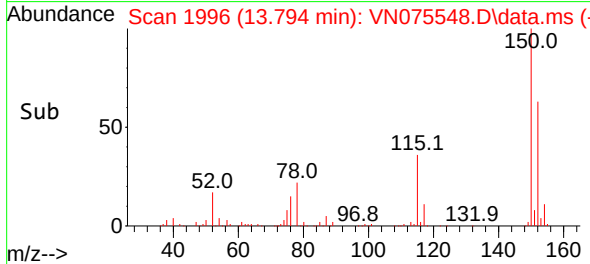


#73
Isopropylbenzene
Concen: 1.015 ug/l
RT: 12.700 min Scan# 1810
Delta R.T. 0.006 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

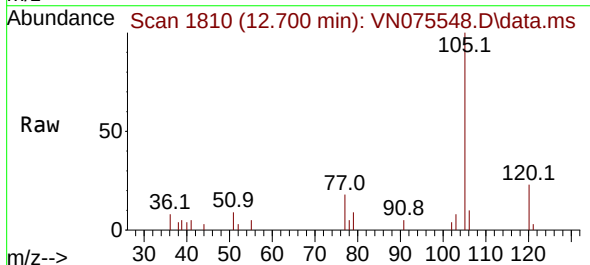


Tgt Ion:105 Resp: 8101
Ion Ratio Lower Upper
105 100
120 22.9 13.1 39.1

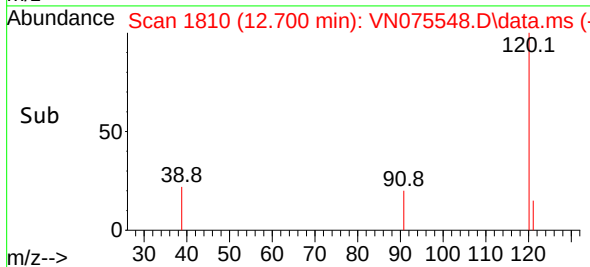

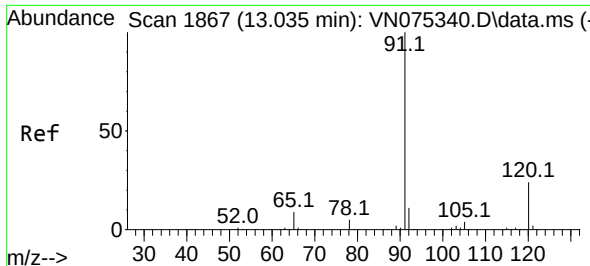

#78
n-propylbenzene
Concen: 0.981 ug/l
RT: 13.041 min Scan# 1867
Delta R.T. 0.006 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01




Tgt Ion: 91 Resp: 8734
Ion Ratio Lower Upper
91 100
120 22.1 11.9 35.5

Manual Integrations
APPROVED



Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

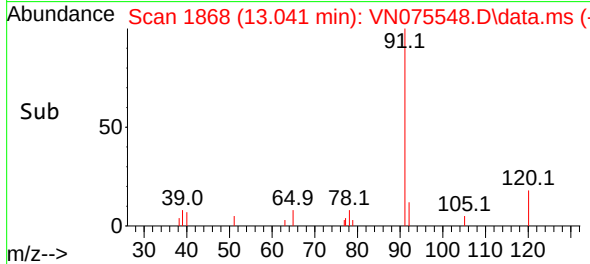


#80
1,3,5-Trimethylbenzene
Concen: 3.412 ug/l
RT: 13.176 min Scan# 1891
Delta R.T. 0.000 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

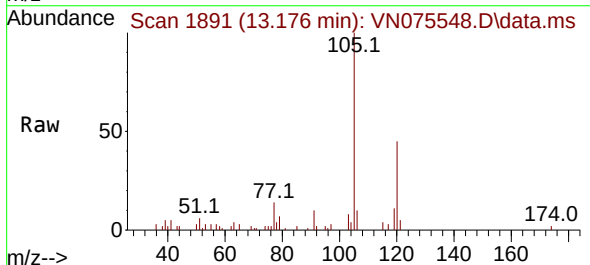


Tgt Ion:105 Resp: 22625
Ion Ratio Lower Upper
105 100
120 49.3 24.7 74.1

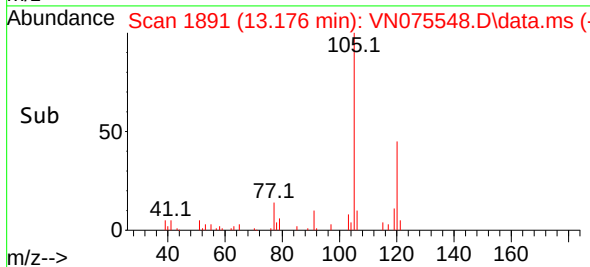



#83
tert-Butylbenzene
Concen: 0.271 ug/l
RT: 13.441 min Scan# 1936
Delta R.T. -0.000 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01




Tgt Ion:119 Resp: 1630
Ion Ratio Lower Upper
119 100
91 59.9 32.8 98.4
134 20.0 12.3 36.9

Manual Integrations
APPROVED



Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

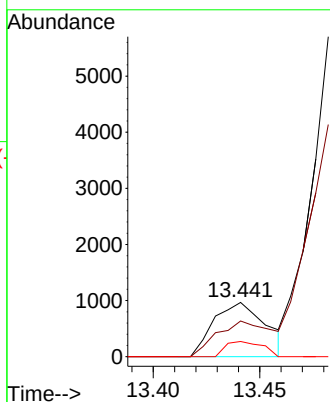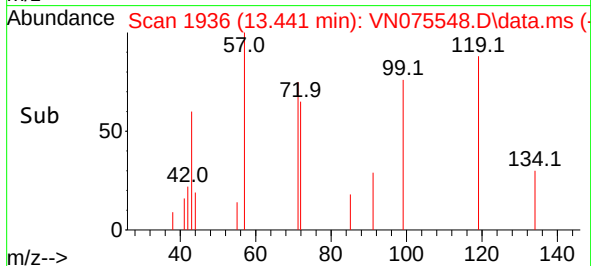


#84
1,2,4-Trimethylbenzene
Concen: 10.066 ug/l
RT: 13.482 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

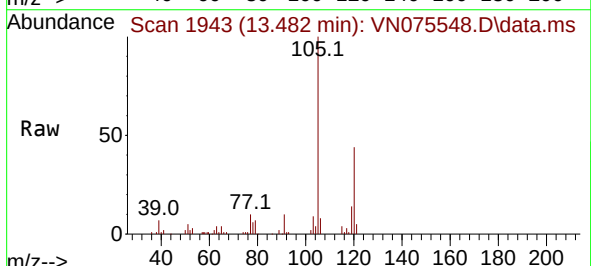


Tgt Ion:105 Resp: 66944
Ion Ratio Lower Upper
105 100
120 47.2 22.7 68.1

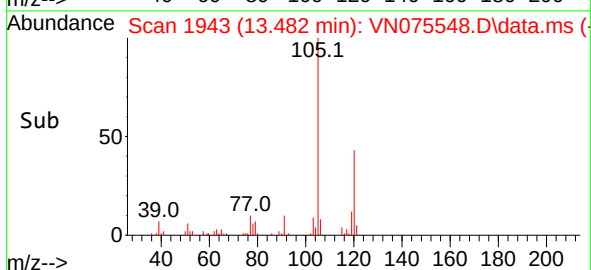

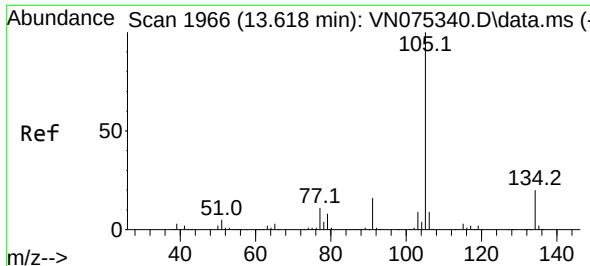

#85
 sec-Butylbenzene
 Concen: 0.488 ug/l
 RT: 13.617 min Scan# 1966
 Delta R.T. -0.001 min
 Lab File: VN075548.D
 Acq: 02 Dec 2022 21:40




Instrument :
 MSVOA_N
 ClientSampleId :
 DUP-01




Tgt Ion:105 Resp: 400
 Ion Ratio Lower Upper
 105 100
 134 39.2 10.2 30.6

Manual Integrations
 APPROVED



Reviewed By :John Carlone 12/05/2022
 Supervised By :Mahesh Dadoda 12/05/2022

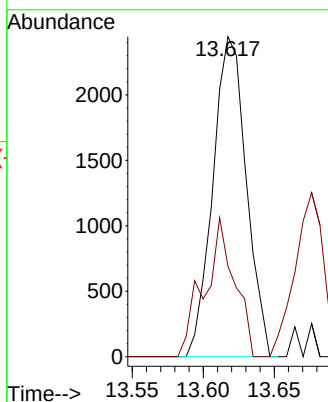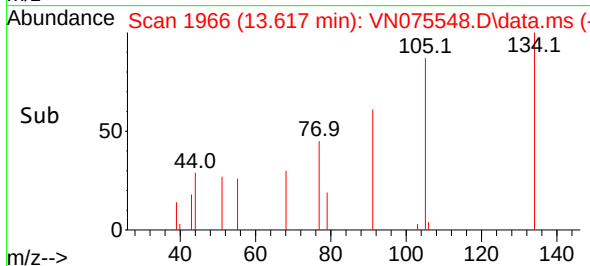


#86
 p-Isopropyltoluene
 Concen: 0.641 ug/l m
 RT: 13.729 min Scan# 1985
 Delta R.T. 0.000 min
 Lab File: VN075548.D
 Acq: 02 Dec 2022 21:40

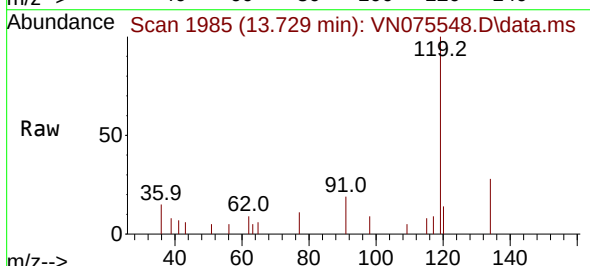


Tgt Ion:119 Resp: 4423
 Ion Ratio Lower Upper
 119 100
 134 41.4 13.1 39.3#
 91 35.4 11.9 35.5

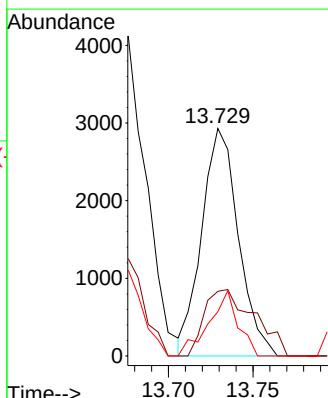



#89
n-Butylbenzene
Concen: 0.540 ug/l
RT: 14.059 min Scan# 2041
Delta R.T. -0.000 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40




Instrument :
MSVOA_N
ClientSampleId :
DUP-01

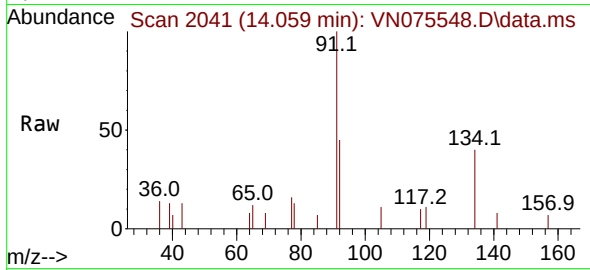

Tgt Ion: 91 Resp: 3150
Ion Ratio Lower Upper
91 100
92 63.2 26.5 79.4
134 0.0 13.0 39.0

Manual Integrations
APPROVED

Reviewed By :John Carlone 12/05/2022
Supervised By :Mahesh Dadoda 12/05/2022

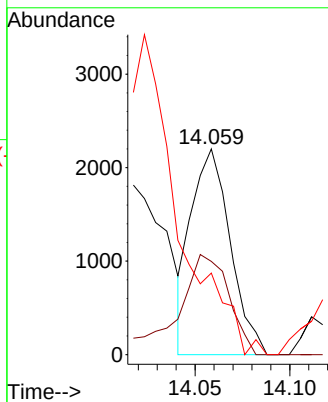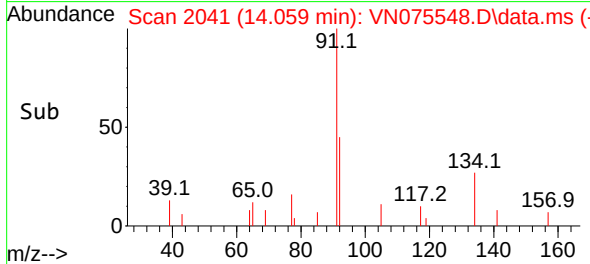

#95
Naphthalene
Concen: 10.332 ug/l
RT: 15.647 min Scan# 2311
Delta R.T. 0.006 min
Lab File: VN075548.D
Acq: 02 Dec 2022 21:40

Tgt Ion:128 Resp: 60610
Ion Ratio Lower Upper
128 100
127 12.3 10.4 15.6
129 10.8 8.6 12.8

